




Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG020322\
Data File : BG052267.D
Acq On : 3 Feb 2022 14:00
Operator : CG/JU
Sample : N1349-13
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
C0HQ2

Manual IntegrationsAPPROVED

Quant Time: Feb 04 00:00:07 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG013122.M
Quant Title : SVOA CALIBRATION
QLast Update : Mon Jan 31 18:07:10 2022
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 02/04/2022
Supervised By :Yogesh Patel 02/08/2022

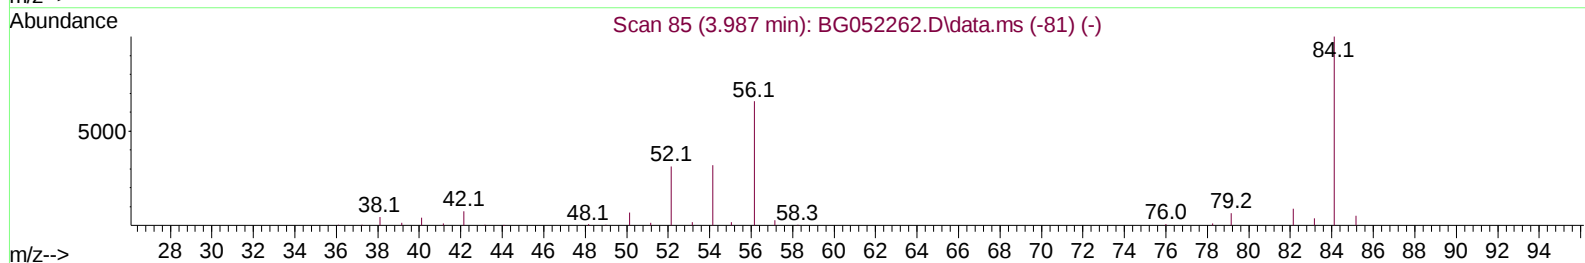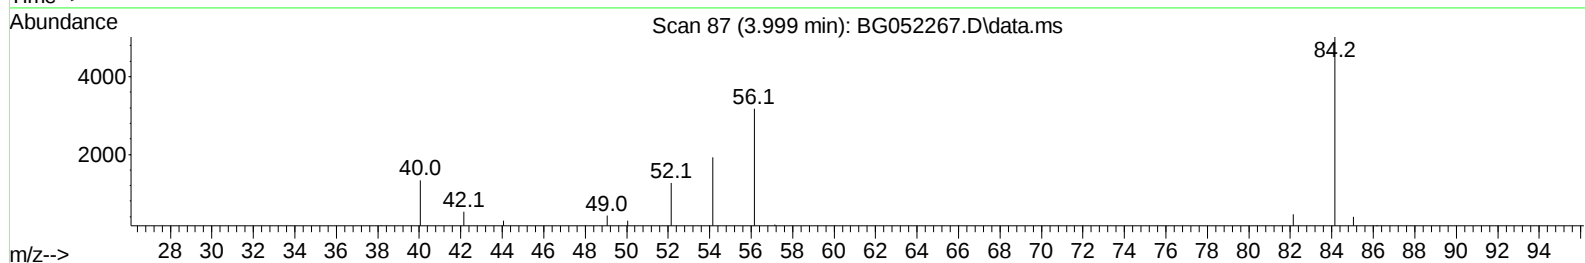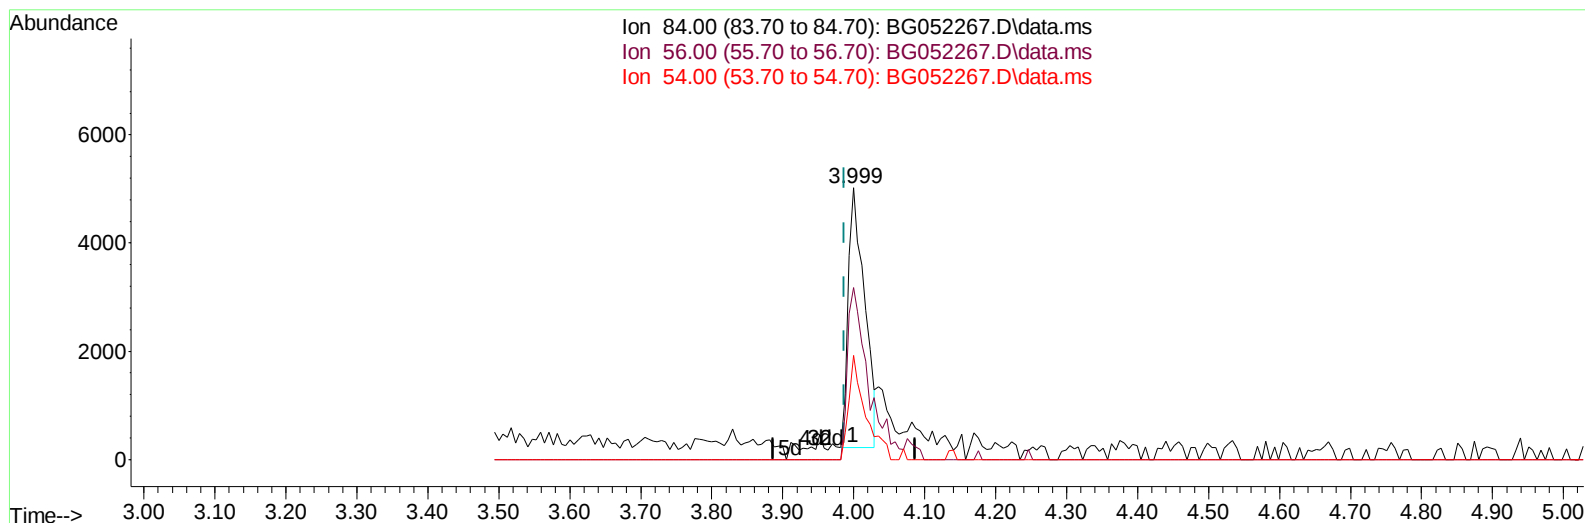

TIC: BG052267.D\data.ms

(4) Pyridine-d5 (S)

3.999min (+ 0.012) 3.70 ng/u1

response 7723

Ion	Exp%	Act%
84.00	100.00	100.00
56.00	68.00	63.24
54.00	31.50	38.29#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG020322\
 Data File : BG052267.D
 Acq On : 3 Feb 2022 14:00
 Operator : CG/JU
 Sample : N1349-13
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 C0HQ2

Manual IntegrationsAPPROVED

Quant Time: Feb 04 00:00:07 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG013122.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Mon Jan 31 18:07:10 2022
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 02/04/2022
 Supervised By :Yogesh Patel 02/08/2022

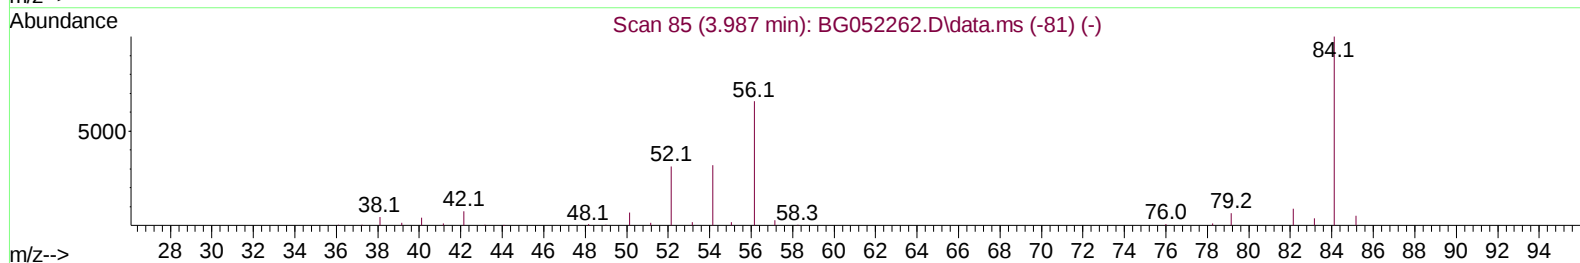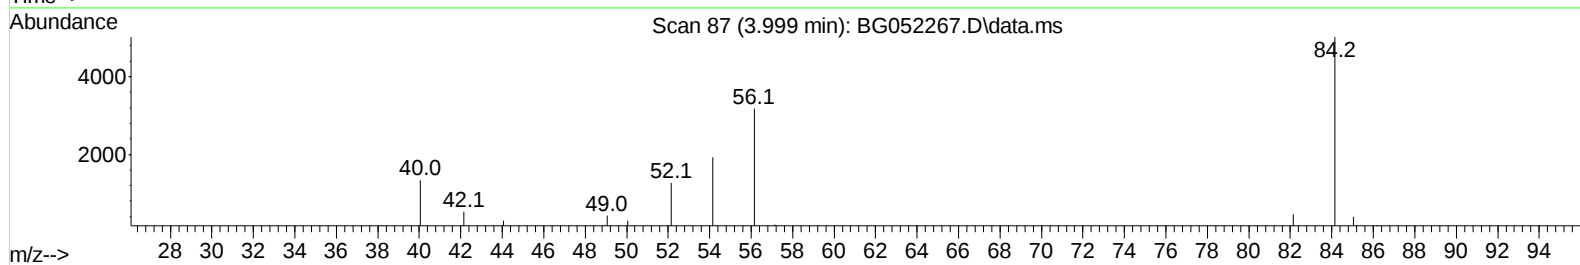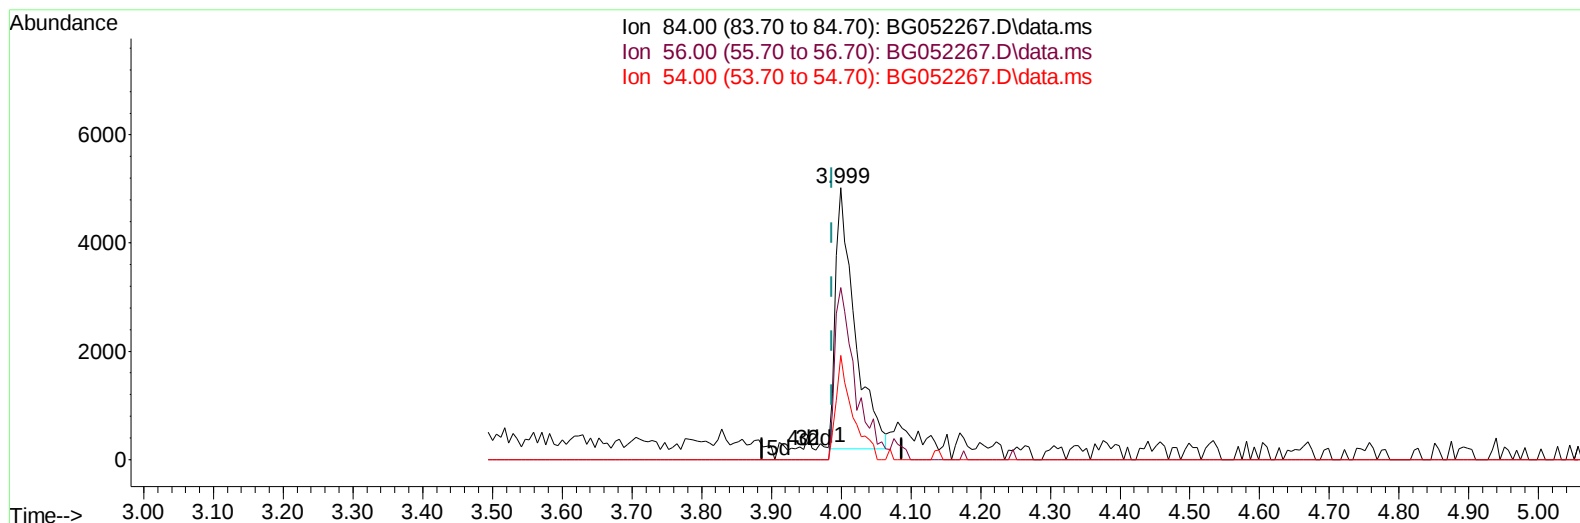

TIC: BG052267.D\data.ms

(4) Pyridine-d5 (S)

3.999min (+ 0.012) 4.43 ng/ul m

response 9247

Ion	Exp%	Act%
84.00	100.00	100.00
56.00	68.00	63.24
54.00	31.50	38.29#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG020322\
Data File : BG052267.D
Acq On : 3 Feb 2022 14:00
Operator : CG/JU
Sample : N1349-13
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
C0HQ2

Manual IntegrationsAPPROVED

Quant Time: Feb 04 00:00:07 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG013122.M
Quant Title : SVOA CALIBRATION
QLast Update : Mon Jan 31 18:07:10 2022
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 02/04/2022
Supervised By :Yogesh Patel 02/08/2022

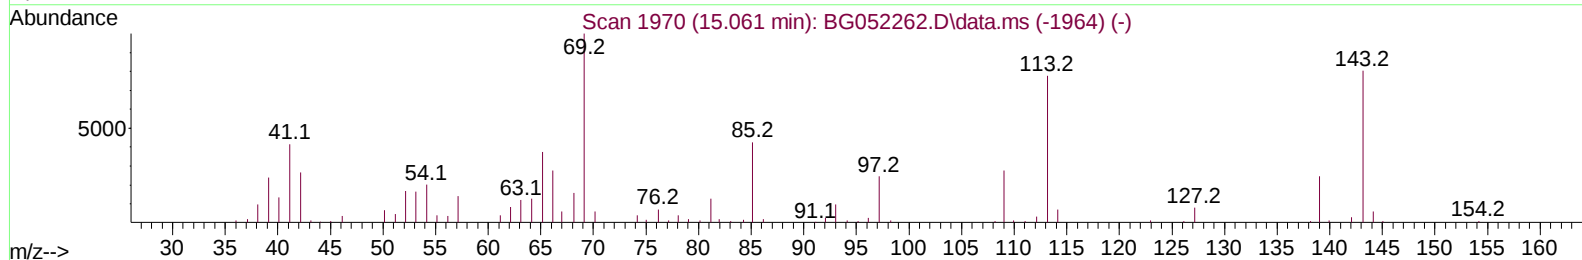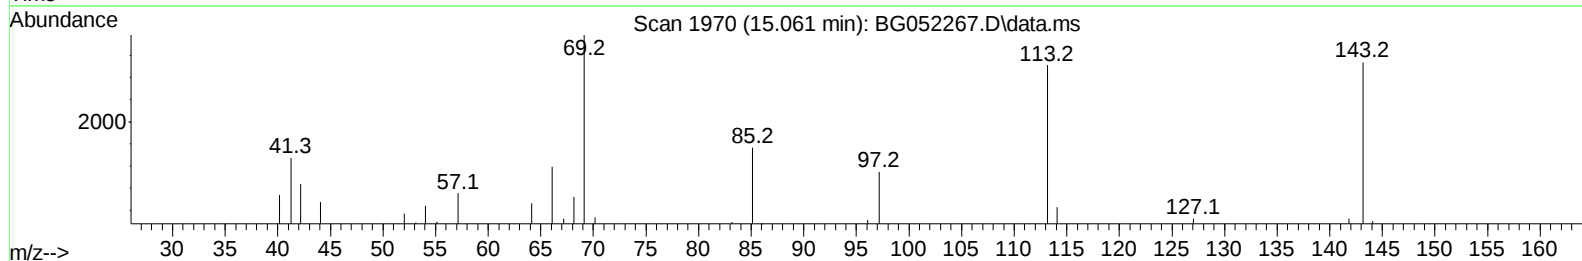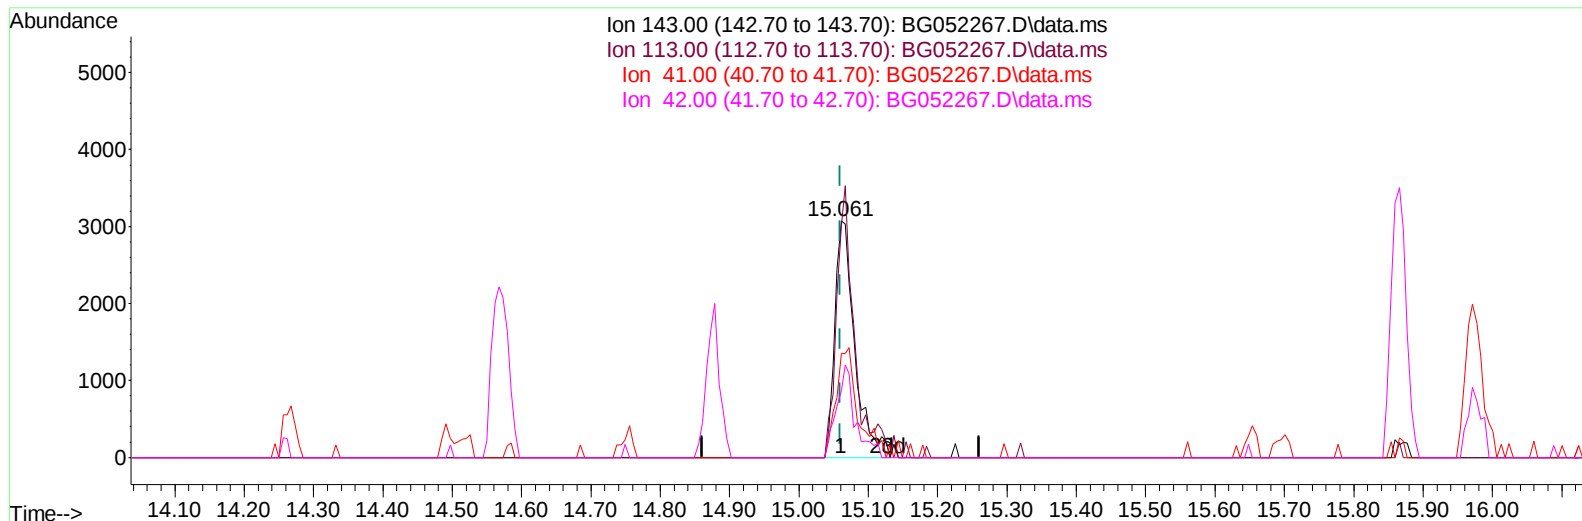

TIC: BG052267.D\data.ms

(54) 4-Nitrophenol-d4 (S)

15.061min (+ 0.001) 6.55 ng/ul m

response 6116

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	80.30	98.31#
41.00	44.40	43.94
42.00	29.70	28.44

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG020322\
 Data File : BG052267.D
 Acq On : 3 Feb 2022 14:00
 Operator : CG/JU
 Sample : N1349-13
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 C0HQ2

Manual IntegrationsAPPROVED

Quant Time: Feb 04 00:00:07 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG013122.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Mon Jan 31 18:07:10 2022
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 02/04/2022
 Supervised By :Yogesh Patel 02/08/2022

Compound	R.T.	Q	Ion	Response	Conc	Units	Dev(Min)

Internal Standards							
1) 1,4-Dichlorobenzene-d4	8.235	152		27055	20.000	ng/ul	0.00
20) Naphthalene-d8	11.072	136		114914	20.000	ng/ul	# 0.00
38) Acenaphthene-d10	14.873	164		78412	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.622	188		193692	20.000	ng/ul	# 0.00
79) Chrysene-d12	21.940	240		202025	20.000	ng/ul	# 0.00
88) Perylene-d12	25.411	264		201154	20.000	ng/ul	-0.01
System Monitoring Compounds							
3) 1,4-Dioxane-d8	3.565	96		3602	5.371	ng/uL	0.00
4) Pyridine-d5	3.999	84		9247m	4.433	ng/ul	0.01
7) Phenol-d5	7.377	99		17413	7.076	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.536	67		54302	36.321	ng/ul	0.00
11) 2-Chlorophenol-d4	7.759	132		45720	26.661	ng/ul	0.00
15) 4-Methylphenol-d8	8.940	113		30381	16.268	ng/ul	0.00
21) Nitrobenzene-d5	9.404	128		31502	33.668	ng/ul	0.00
24) 2-Nitrophenol-d4	10.138	143		33101	32.375	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.684	165		57724	28.960	ng/ul	0.00
31) 4-Chloroaniline-d4	11.195	131		55658	22.014	ng/ul	0.00
46) Dimethylphthalate-d6	14.268	166		228973	37.150	ng/ul	0.00
49) Acenaphthylene-d8	14.573	160		282443	36.765	ng/ul	0.00
54) 4-Nitrophenol-d4	15.061	143		6116m	6.552	ng/ul	0.00
60) Fluorene-d10	15.866	176		207693	38.463	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.977	200		38403	32.115	ng/ul	0.00
73) Anthracene-d10	17.722	188		384227	42.077	ng/ul	0.00
81) Pyrene-d10	20.001	212		481654	39.780	ng/ul	0.00
92) Benzo(a)pyrene-d12	25.177	264		454024	42.486	ng/ul	0.00

Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG020322\
Data File : BG052267.D
Acq On : 3 Feb 2022 14:00
Operator : CG/JU
Sample : N1349-13
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
C0HQ2

Manual IntegrationsAPPROVED

Quant Time: Feb 04 00:00:07 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG013122.M
Quant Title : SVOA CALIBRATION
QLast Update : Mon Jan 31 18:07:10 2022
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 02/04/2022
Supervised By :Yogesh Patel 02/08/2022

