




Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG020322\
Data File : BG052268.D
Acq On : 3 Feb 2022 14:38
Operator : CG/JU
Sample : N1349-04
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
C0HP3

Manual IntegrationsAPPROVED

Quant Time: Feb 04 00:00:20 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG013122.M
Quant Title : SVOA CALIBRATION
QLast Update : Mon Jan 31 18:07:10 2022
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 02/04/2022
Supervised By :Yogesh Patel 02/08/2022

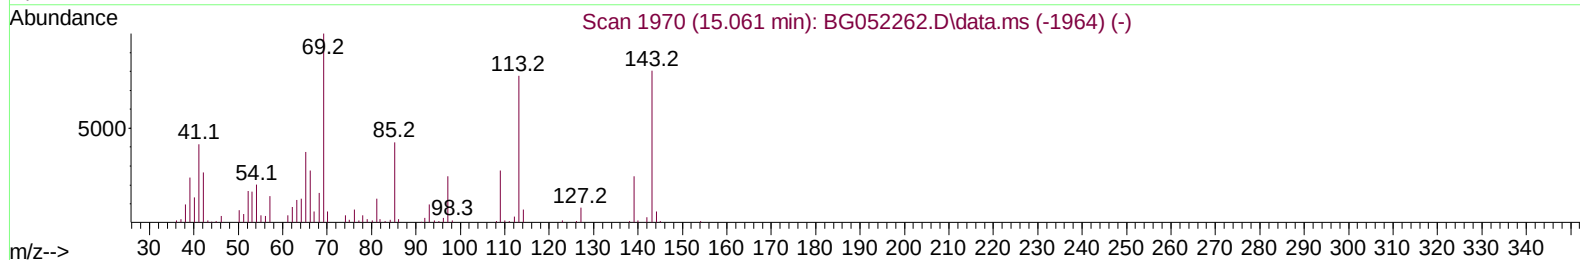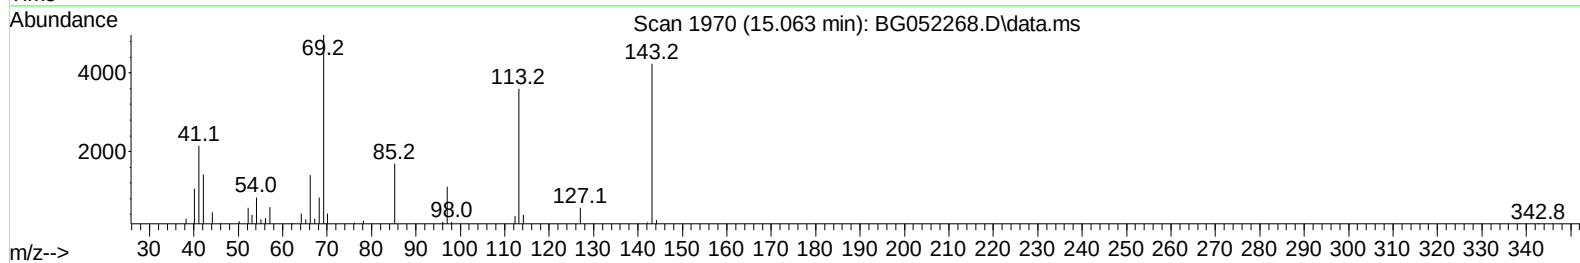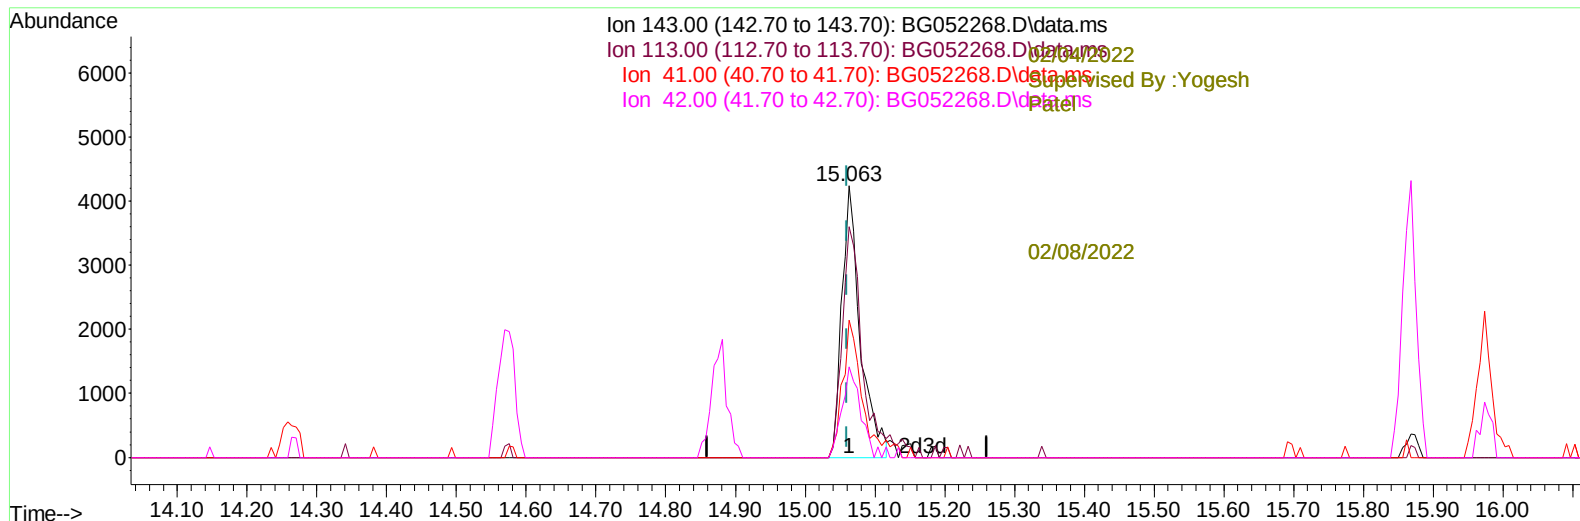

TIC: BG052268.D\data.ms

(54) 4-Nitrophenol-d4 (S)

15.063min (+ 0.003) 8.06 ng/ul

response 7720

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	80.30	85.08
41.00	44.40	50.70
42.00	29.70	33.44

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG020322\
Data File : BG052268.D
Acq On : 3 Feb 2022 14:38
Operator : CG/JU
Sample : N1349-04
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :

BNA_G




ClientSampleId :

C0HP3

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 02/04/2022
Supervised By :Yogesh Patel 02/08/2022

Quant Time: Feb 04 00:00:20 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG013122.M
Quant Title : SVOA CALIBRATION
QLast Update : Mon Jan 31 18:07:10 2022
Response via : Initial Calibration

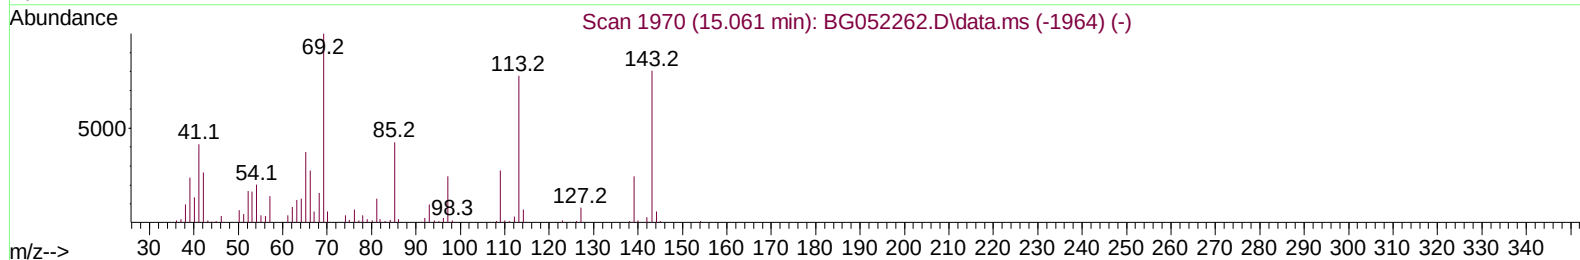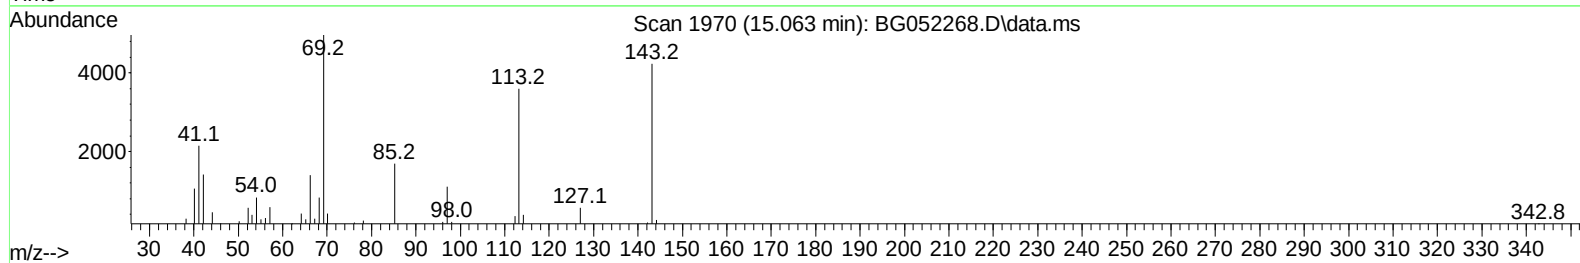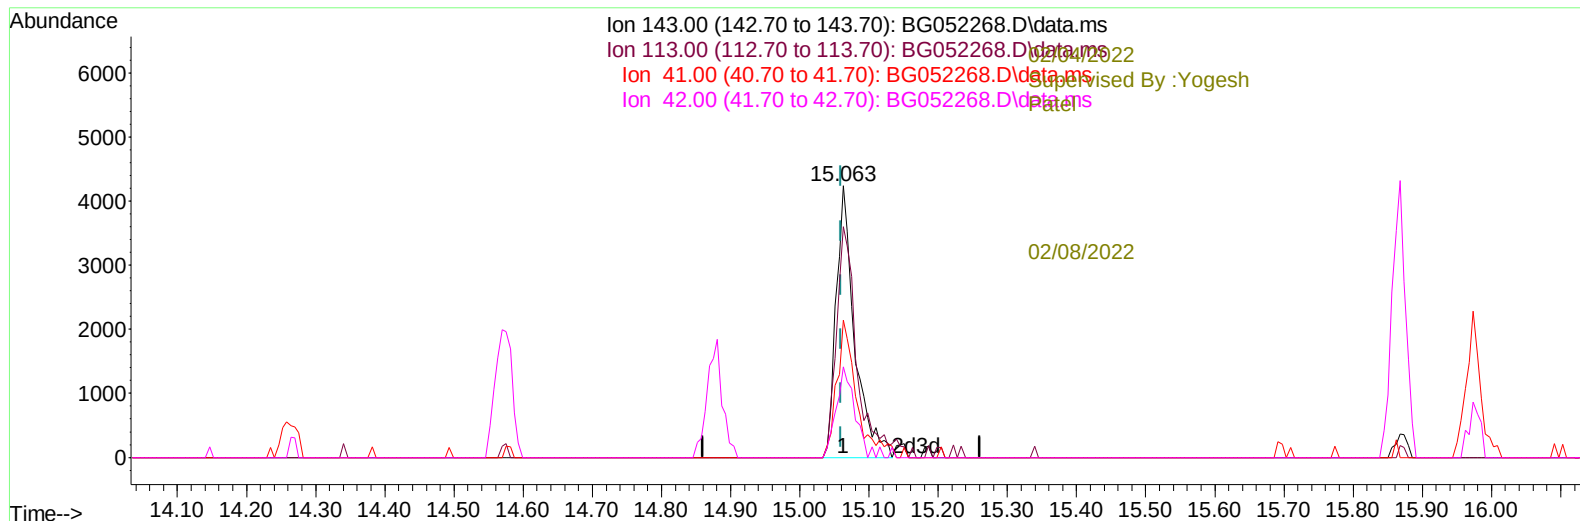

TIC: BG052268.D\data.ms

(54) 4-Nitrophenol-d4 (S)

15.063min (+ 0.003) 8.24 ng/ul m

response 7890

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	80.30	85.08
41.00	44.40	50.70
42.00	29.70	33.44

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG020322\
 Data File : BG052268.D
 Acq On : 3 Feb 2022 14:38
 Operator : CG/JU
 Sample : N1349-04
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 C0HP3

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 02/04/2022
 Supervised By :Yogesh Patel 02/08/2022

Quant Time: Feb 04 00:00:20 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG013122.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Mon Jan 31 18:07:10 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
-----02/04/2022						
Supervised By :Yogesh Patel						
Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.237	152	29256	20.000	ng/ul	0.00
20) Naphthalene-d8	11.074	136	115309	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.881	164	80462	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.624	188	196797	20.000	ng/ul	# 0.00
79) Chrysene-d12	21.936	240	206012	20.000	ng/ul	# 0.00
88) Perylene-d12	25.408	264	206286	20.000	ng/ul	-0.0108/2022
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.567	96	3530	4.868	ng/uL	0.00
4) Pyridine-d5	4.001	84	10136	4.494	ng/ul	0.01
7) Phenol-d5	7.379	99	22585	8.487	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.538	67	58900	36.432	ng/ul	0.00
11) 2-Chlorophenol-d4	7.761	132	53763	28.993	ng/ul	0.00
15) 4-Methylphenol-d8	8.942	113	38444	19.037	ng/ul	0.00
21) Nitrobenzene-d5	9.406	128	35227	37.520	ng/ul	0.00
24) 2-Nitrophenol-d4	10.134	143	37215	36.274	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.687	165	62091	31.044	ng/ul	0.00
31) 4-Chloroaniline-d4	11.198	131	69394	27.353	ng/ul	0.00
46) Dimethylphthalate-d6	14.270	166	236320	37.365	ng/ul	0.00
49) Acenaphthylene-d8	14.575	160	299325	37.970	ng/ul	0.00
54) 4-Nitrophenol-d4	15.063	143	7890m	8.237	ng/ul	0.00
60) Fluorene-d10	15.868	176	213623	38.554	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.974	200	39194	32.259	ng/ul	0.00
73) Anthracene-d10	17.724	188	381740	41.145	ng/ul	0.00
81) Pyrene-d10	20.003	212	475793	38.536	ng/ul	0.00
92) Benzo(a)pyrene-d12	25.173	264	450372	41.095	ng/ul	0.00

Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG020322\
Data File : BG052268.D
Acq On : 3 Feb 2022 14:38
Operator : CG/JU
Sample : N1349-04
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
C0HP3

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 02/04/2022
Supervised By :Yogesh Patel 02/08/2022

Quant Time: Feb 04 00:00:20 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG013122.M
Quant Title : SVOA CALIBRATION
QLast Update : Mon Jan 31 18:07:10 2022
Response via : Initial Calibration

