




Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG020322\
Data File : BG052286.D
Acq On : 4 Feb 2022 2:37
Operator : CG/JU
Sample : N1328-17
Misc :
ALS Vial : 26 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
COHN6

Manual IntegrationsAPPROVED

Quant Time: Feb 04 04:19:10 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG013122.M
Quant Title : SVOA CALIBRATION
QLast Update : Mon Jan 31 18:07:10 2022
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 02/04/2022
Supervised By :Yogesh Patel 02/08/2022

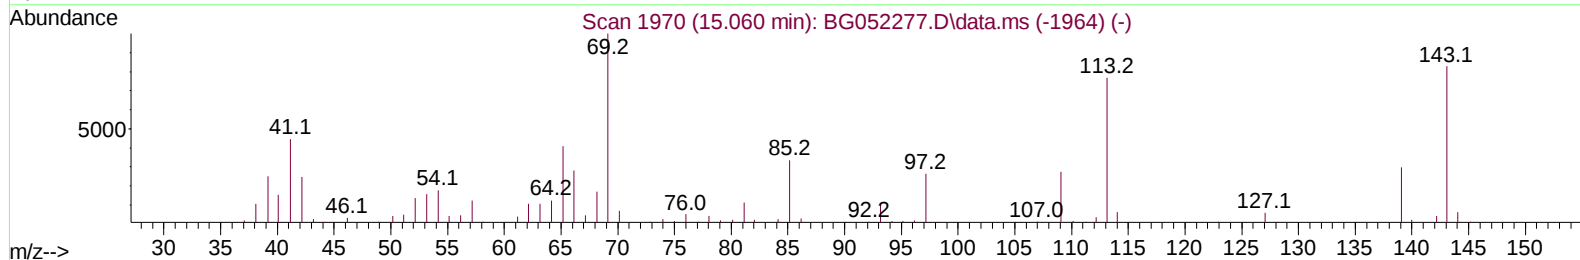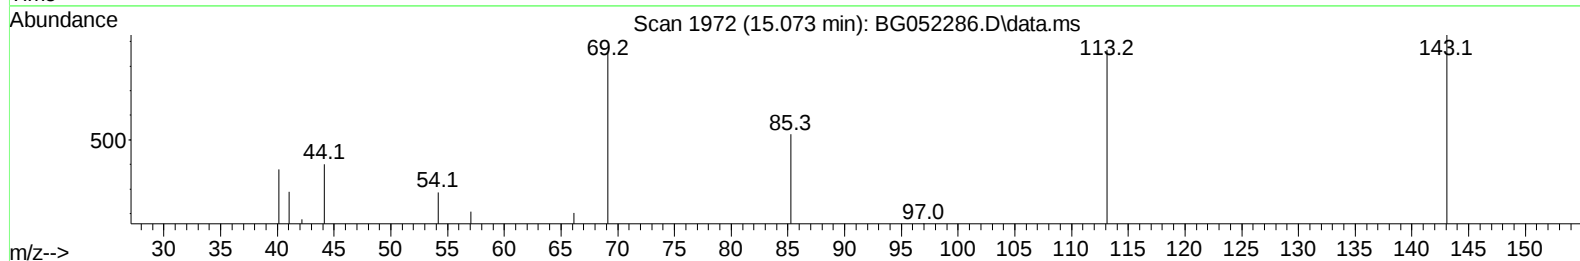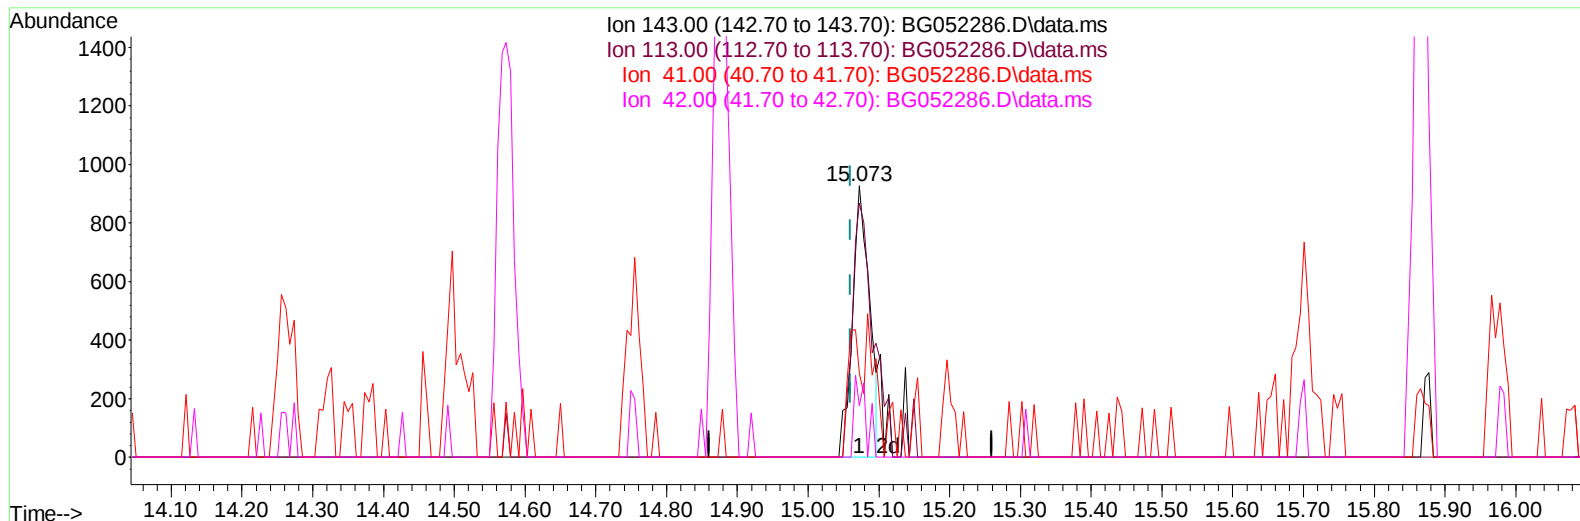

TIC: BG052286.D\data.ms

(54) 4-Nitrophenol-d4 (S)

15.073min (+ 0.012) 1.58 ng/ul

response 1556

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	80.30	93.64
41.00	44.40	31.07#
42.00	29.70	19.09#




Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG020322\
Data File : BG052286.D
Acq On : 4 Feb 2022 2:37
Operator : CG/JU
Sample : N1328-17
Misc :
ALS Vial : 26 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
COHN6

Manual IntegrationsAPPROVED

Quant Time: Feb 04 04:19:10 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG013122.M
Quant Title : SVOA CALIBRATION
QLast Update : Mon Jan 31 18:07:10 2022
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 02/04/2022
Supervised By :Yogesh Patel 02/08/2022

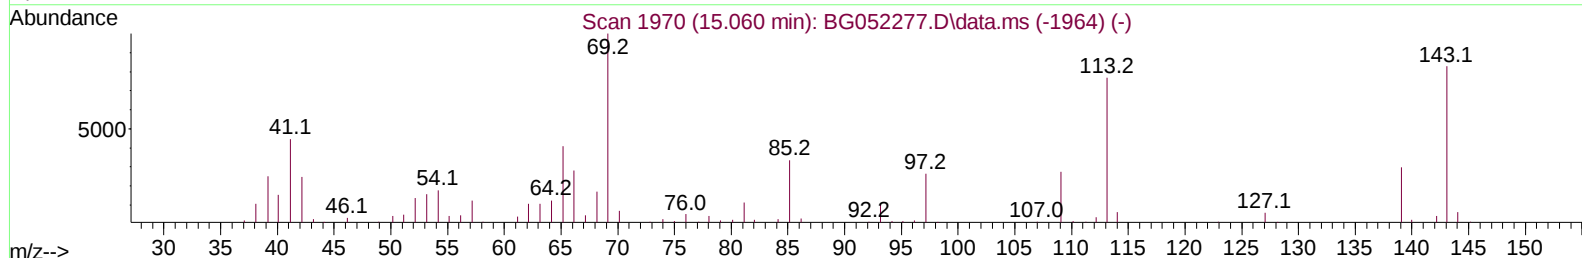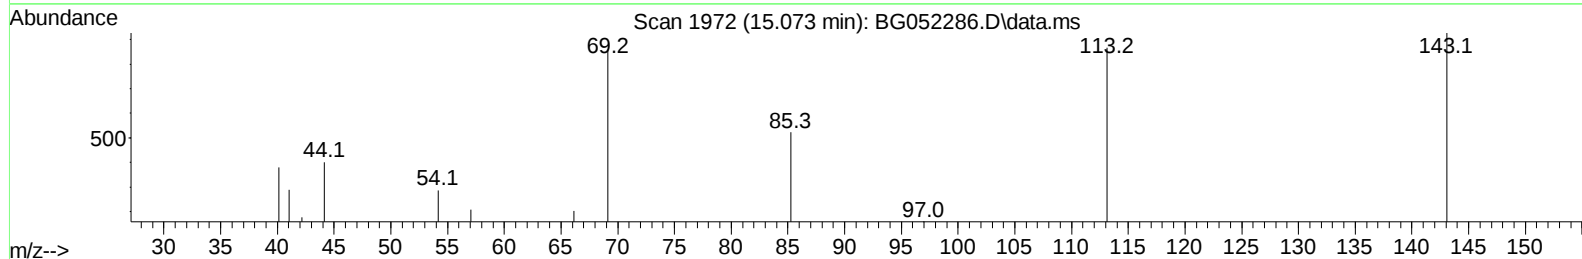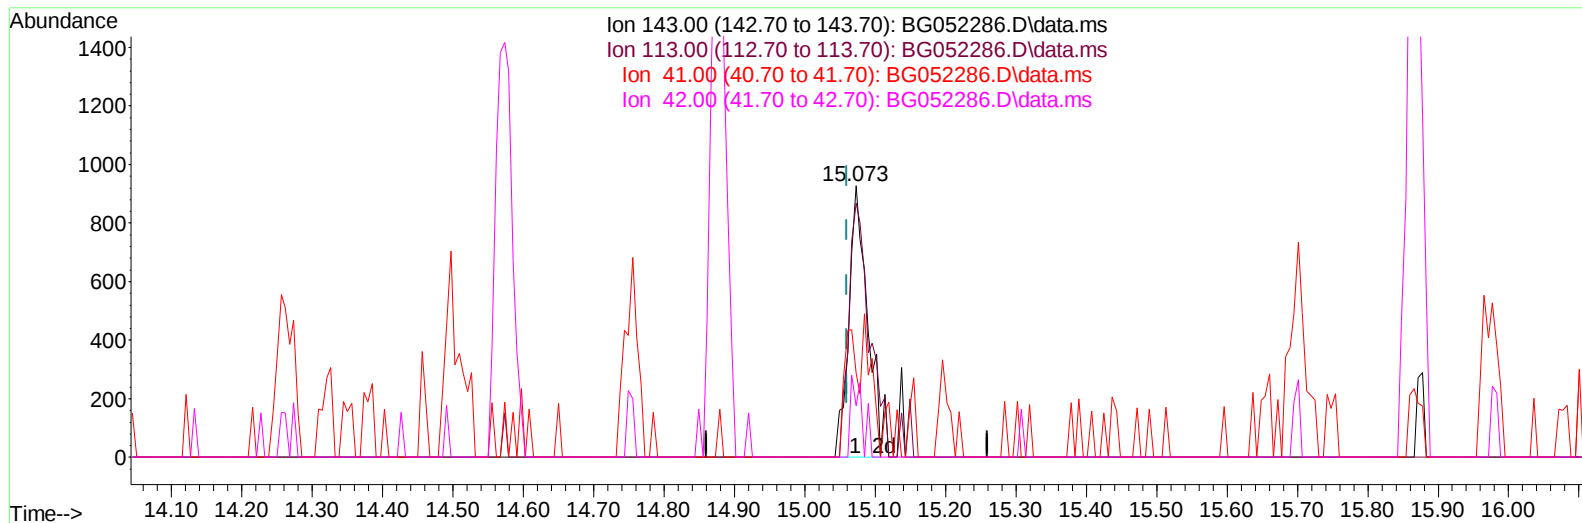

TIC: BG052286.D\data.ms

(54) 4-Nitrophenol-d4 (S)

15.073min (+ 0.012) 1.71 ng/ul m

response 1681

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	80.30	93.64
41.00	44.40	31.07#
42.00	29.70	19.09#

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG020322\
 Data File : BG052286.D
 Acq On : 4 Feb 2022 2:37
 Operator : CG/JU
 Sample : N1328-17
 Misc :
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 COHN6

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 02/04/2022
 Supervised By :Yogesh Patel 02/08/2022

Quant Time: Feb 04 04:19:10 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG013122.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Mon Jan 31 18:07:10 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.235	152	30243	20.000	ng/ul	0.00
20) Naphthalene-d8	11.078	136	121023	20.000	ng/ul	# 0.00
38) Acenaphthene-d10	14.879	164	82616	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.628	188	195684	20.000	ng/ul	# 0.00
79) Chrysene-d12	21.940	240	190245	20.000	ng/ul	# 0.00
88) Perylene-d12	25.411	264	189563	20.000	ng/ul	-0.01
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.565	96	3032	4.045	ng/uL	0.00
4) Pyridine-d5	3.999	84	20150	8.642	ng/ul	0.01
7) Phenol-d5	7.383	99	6240	2.268	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.542	67	33608	20.110	ng/ul	0.00
11) 2-Chlorophenol-d4	7.765	132	14670	7.653	ng/ul	0.00
15) 4-Methylphenol-d8	8.940	113	11785	5.645	ng/ul	0.00
21) Nitrobenzene-d5	9.404	128	19323	19.609	ng/ul	0.00
24) 2-Nitrophenol-d4	10.138	143	9643	8.955	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.690	165	17438	8.307	ng/ul	0.00
31) 4-Chloroaniline-d4	11.201	131	62973	23.650	ng/ul	0.00
46) Dimethylphthalate-d6	14.268	166	136229	20.978	ng/ul	0.00
49) Acenaphthylene-d8	14.573	160	163796	20.236	ng/ul	0.00
54) 4-Nitrophenol-d4	15.073	143	1681m	1.709	ng/ul	0.01
60) Fluorene-d10	15.866	176	121055	21.278	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.977	200	8269	6.845	ng/ul	0.00
73) Anthracene-d10	17.728	188	214346	23.234	ng/ul	0.00
81) Pyrene-d10	20.001	212	244357	21.431	ng/ul	0.00
92) Benzo(a)pyrene-d12	25.177	264	224868	22.329	ng/ul	0.00

Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG020322\
Data File : BG052286.D
Acq On : 4 Feb 2022 2:37
Operator : CG/JU
Sample : N1328-17
Misc :
ALS Vial : 26 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
COHN6

Manual IntegrationsAPPROVED

Quant Time: Feb 04 04:19:10 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG013122.M
Quant Title : SVOA CALIBRATION
QLast Update : Mon Jan 31 18:07:10 2022
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 02/04/2022
Supervised By :Yogesh Patel 02/08/2022

