




Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG020322\
Data File : BG052295.D
Acq On : 4 Feb 2022 11:00
Operator : CG/JU
Sample : N1349-02DL 5X
Misc :
ALS Vial : 36 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
C0HP1DL

Manual IntegrationsAPPROVED

Quant Time: Feb 04 11:33:54 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG013122.M
Quant Title : SVOA CALIBRATION
QLast Update : Mon Jan 31 18:07:10 2022
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 02/07/2022
Supervised By :Yogesh Patel 02/08/2022

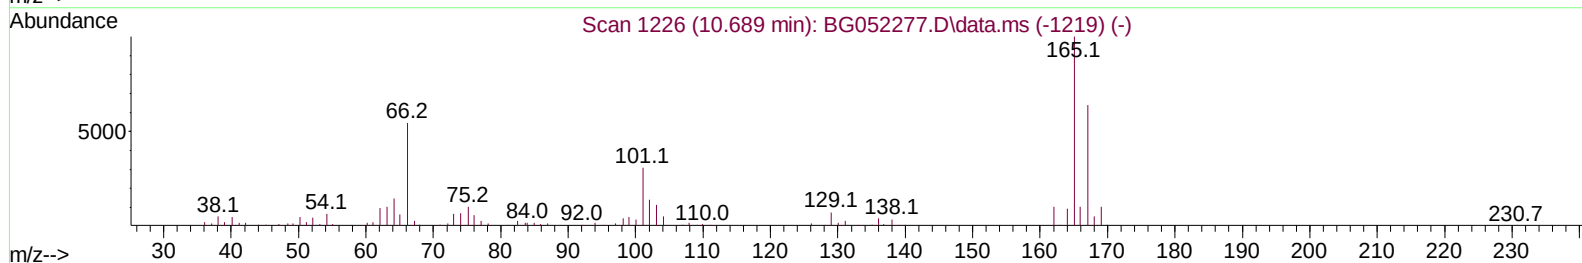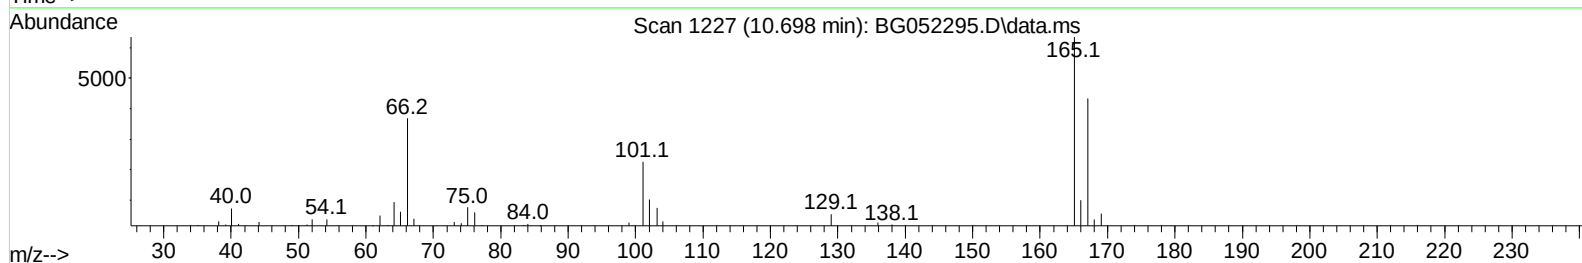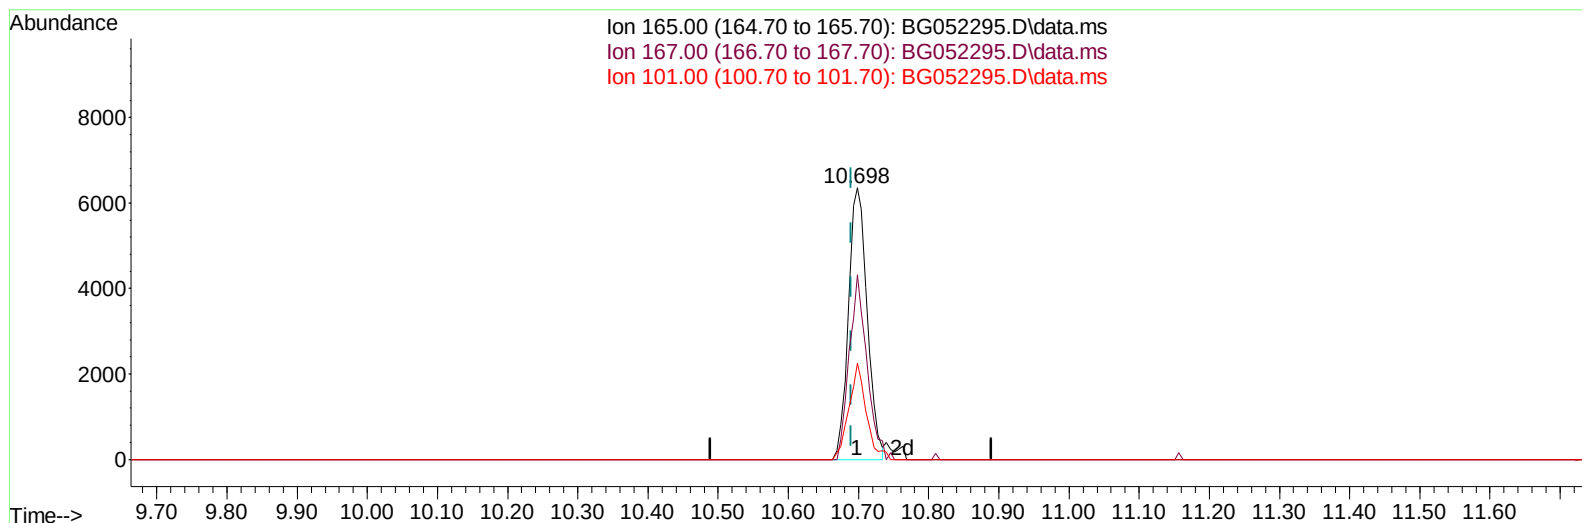

TIC: BG052295.D\data.ms

(28) 2,4-Dichlorophenol-d3 (S)

10.698min (+ 0.009) 5.17 ng/ul

response 11830

Ion	Exp%	Act%
165.00	100.00	100.00
167.00	64.30	68.12
101.00	34.40	35.61
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG020322\
Data File : BG052295.D
Acq On : 4 Feb 2022 11:00
Operator : CG/JU
Sample : N1349-02DL 5X
Misc :
ALS Vial : 36 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
C0HP1DL

Manual IntegrationsAPPROVED

Quant Time: Feb 04 11:33:54 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG013122.M
Quant Title : SVOA CALIBRATION
QLast Update : Mon Jan 31 18:07:10 2022
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 02/07/2022
Supervised By :Yogesh Patel 02/08/2022

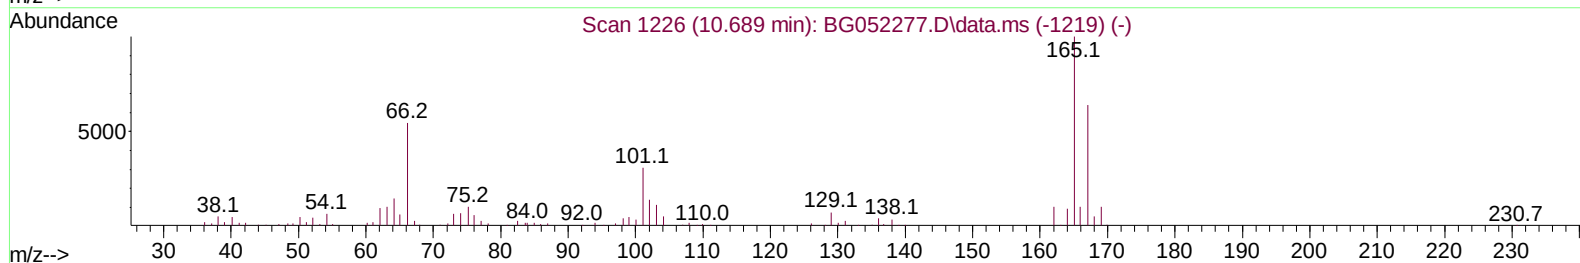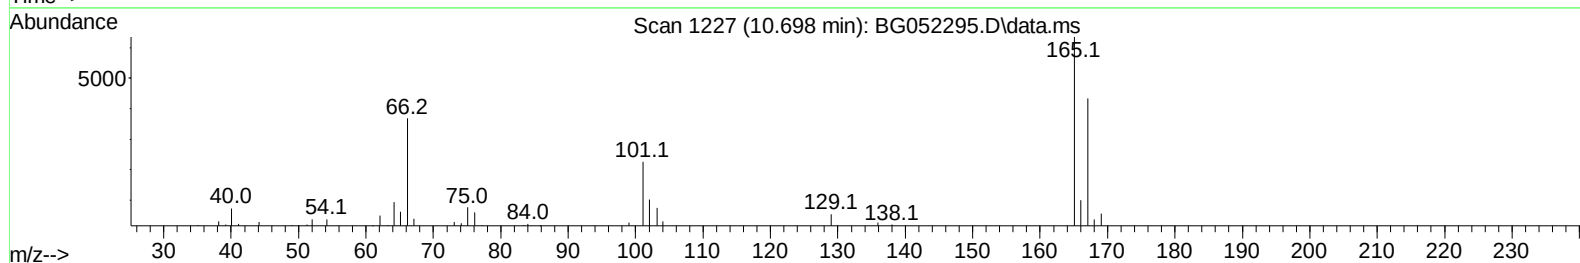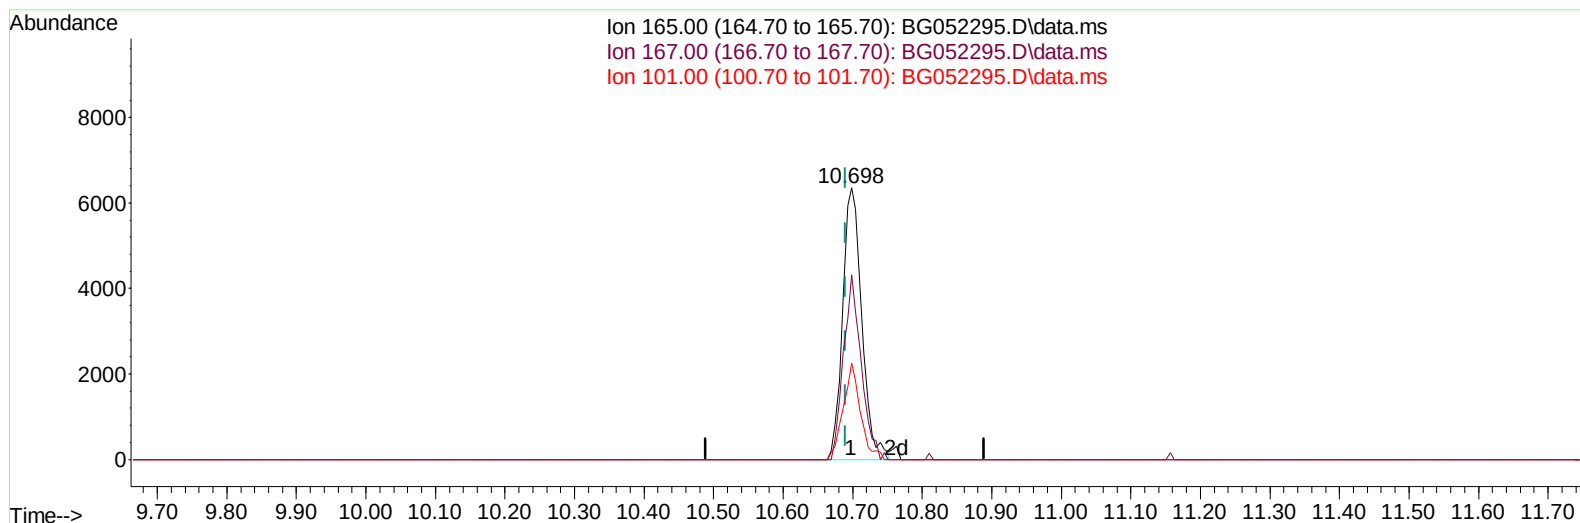

TIC: BG052295.D\data.ms

(28) 2,4-Dichlorophenol-d3 (S)

10.698min (+ 0.009) 5.29 ng/ul m

response 12116

Ion	Exp%	Act%
165.00	100.00	100.00
167.00	64.30	68.12
101.00	34.40	35.61
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG020322\
 Data File : BG052295.D
 Acq On : 4 Feb 2022 11:00
 Operator : CG/JU
 Sample : N1349-02DL 5X
 Misc :
 ALS Vial : 36 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 C0HP1DL

Manual IntegrationsAPPROVED

Quant Time: Feb 04 11:33:54 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG013122.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Mon Jan 31 18:07:10 2022
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 02/07/2022
 Supervised By :Yogesh Patel 02/08/2022

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.249	152	33466	20.000	ng/ul	0.01
20) Naphthalene-d8	11.080	136	132042	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.881	164	92041	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.630	188	219945	20.000	ng/ul	# 0.00
79) Chrysene-d12	21.948	240	226015	20.000	ng/ul	# 0.00
88) Perylene-d12	25.426	264	227326	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.543	96	96793	116.683	ng/uL	-0.02
4) Pyridine-d5	0.000	84	0d	0.000	ng/ul	
7) Phenol-d5	7.391	99	4665	1.532	ng/ul	0.01
9) Bis-(2-Chloroethyl)eth...	7.544	67	11956	6.465	ng/ul	0.00
11) 2-Chlorophenol-d4	7.773	132	9741	4.592	ng/ul	0.00
15) 4-Methylphenol-d8	8.948	113	7252	3.139	ng/ul	0.00
21) Nitrobenzene-d5	9.412	128	7218	6.714	ng/ul	0.00
24) 2-Nitrophenol-d4	10.146	143	7095	6.039	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.698	165	12116m	5.290	ng/ul	0.00
31) 4-Chloroaniline-d4	11.204	131	17477	6.016	ng/ul	0.00
46) Dimethylphthalate-d6	14.270	166	50324	6.956	ng/ul	0.00
49) Acenaphthylene-d8	14.581	160	63594	7.052	ng/ul	0.00
54) 4-Nitrophenol-d4	0.000	143	0d	0.000	ng/ul	
60) Fluorene-d10	15.874	176	48570	7.663	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	0.000	200	0d	0.000	ng/ul	
73) Anthracene-d10	17.730	188	84236	8.124	ng/ul	0.00
81) Pyrene-d10	20.009	212	100867	7.446	ng/ul	0.00
92) Benzo(a)pyrene-d12	25.185	264	90421	7.487	ng/ul	0.00
Target Compounds						
					Qvalue	
2) 1,4-Dioxane	3.602	88	13593	14.701	ng/uL	97

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG020322\
Data File : BG052295.D
Acq On : 4 Feb 2022 11:00
Operator : CG/JU
Sample : N1349-02DL 5X
Misc :
ALS Vial : 36 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
C0HP1DL

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 02/07/2022
Supervised By :Yogesh Patel 02/08/2022

Quant Time: Feb 04 11:33:54 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG013122.M
Quant Title : SVOA CALIBRATION
QLast Update : Mon Jan 31 18:07:10 2022
Response via : Initial Calibration

