

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG020322\
 Data File : BG052272.D
 Acq On : 3 Feb 2022 17:10
 Operator : CG/JU
 Sample : N1349-03
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 C0HP2

Manual Integrations
 APPROVED

Reviewed By :Jagrut Upadhyay 02/04/2022
 Supervised By :Yogesh Patel 02/08/2022

Quant Time: Feb 04 00:01:24 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG013122.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Mon Jan 31 18:07:10 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.237	152	27092	20.000	ng/u1	0.00
20) Naphthalene-d8	11.074	136	108708	20.000	ng/u1	0.00
38) Acenaphthene-d10	14.881	164	74806	20.000	ng/u1	0.00
64) Phenanthrene-d10	17.624	188	184449	20.000	ng/u1	# 0.00
79) Chrysene-d12	21.936	240	188926	20.000	ng/u1	# 0.00
88) Perylene-d12	25.408	264	188523	20.000	ng/u1	-0.01
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.567	96	3244	4.831	ng/uL	0.00
4) Pyridine-d5	4.002	84	9556m	4.575	ng/u1	0.01
7) Phenol-d5	7.379	99	17778	7.214	ng/u1	0.00
9) Bis-(2-Chloroethyl)eth...	7.538	67	49829	33.283	ng/u1	0.00
11) 2-Chlorophenol-d4	7.761	132	44933	26.166	ng/u1	0.00
15) 4-Methylphenol-d8	8.936	113	30545	16.334	ng/u1	0.00
21) Nitrobenzene-d5	9.406	128	29885	33.763	ng/u1	0.00
24) 2-Nitrophenol-d4	10.140	143	30790	31.834	ng/u1	0.00
28) 2,4-Dichlorophenol-d3	10.687	165	52852	28.030	ng/u1	0.00
31) 4-Chloroaniline-d4	11.198	131	57665	24.110	ng/u1	0.00
46) Dimethylphthalate-d6	14.270	166	201747	34.311	ng/u1	0.00
49) Acenaphthylene-d8	14.575	160	248393	33.892	ng/u1	0.00
54) 4-Nitrophenol-d4	15.063	143	6407m	7.195	ng/u1	0.00
60) Fluorene-d10	15.868	176	179769	34.897	ng/u1	0.00
65) 4,6-Dinitro-2-methylph...	15.974	200	32944	28.930	ng/u1	0.00
73) Anthracene-d10	17.724	188	328438	37.770	ng/u1	0.00
81) Pyrene-d10	20.003	212	395393	34.920	ng/u1	0.00
92) Benzo(a)pyrene-d12	25.167	264	369361	36.879	ng/u1	-0.01
Target Compounds						
2) 1,4-Dioxane	3.608	88	2155	2.879	ng/uL#	Qvalue 91

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG020322\
Data File : BG052272.D
Acq On : 3 Feb 2022 17:10
Operator : CG/JU
Sample : N1349-03
Misc :
ALS Vial : 12 Sample Multiplier: 1


Instrument :
BNA_G
ClientSampleId :
C0HP2

Quant Time: Feb 04 00:01:24 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG013122.M
Quant Title : SVOA CALIBRATION
QLast Update : Mon Jan 31 18:07:10 2022
Response via : Initial Calibration

Manual Integrations
APPROVED


Reviewed By :Jagrut Upadhyay 02/04/2022
Supervised By :Yogesh Patel 02/08/2022

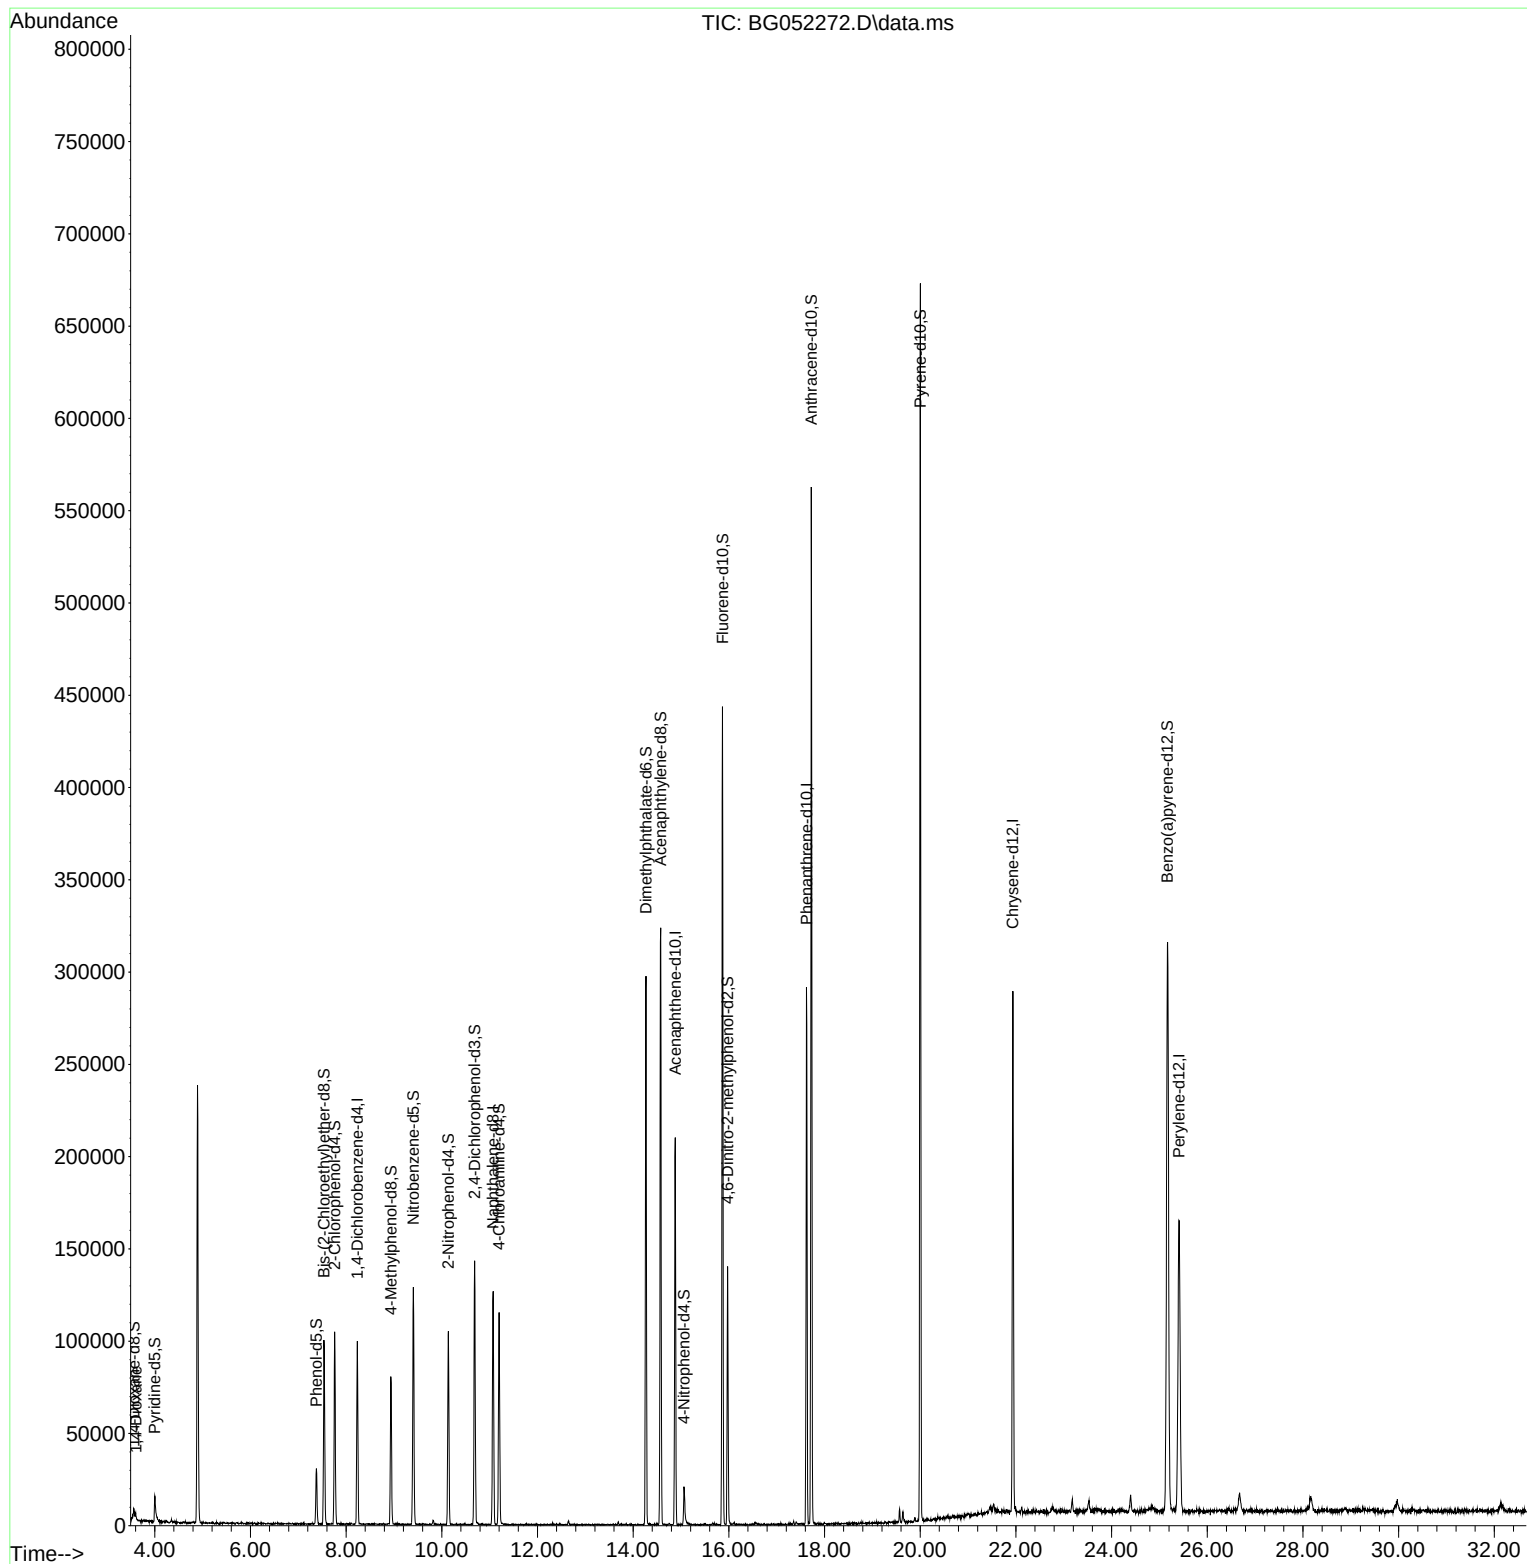

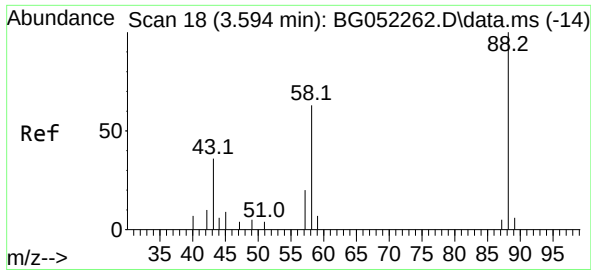

#2
 1,4-Dioxane
 Concen: 2.879 ng/uL
 RT: 3.608 min Scan# 20
 Delta R.T. 0.009 min
 Lab File: BG052272.D
 Acq: 3 Feb 2022 17:10

Instrument :
 BNA_G
 ClientSampleId :
 C0HP2

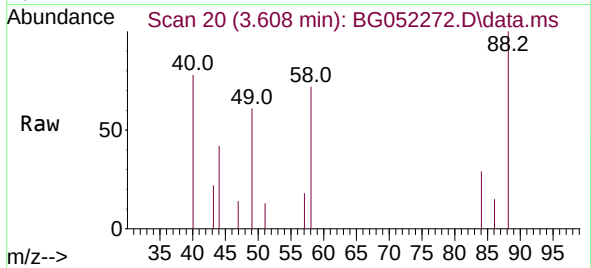

Tgt Ion: 88 Resp: 215
 Ion Ratio Lower Upper
 88 100
 43 21.9 23.0 34.4
 58 71.5 62.4 93.6

Manual Integrations
 APPROVED

Reviewed By :Jagrut Upadhyay 02/04/2022
 Supervised By :Yogesh Patel 02/08/2022

