

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG020322\
 Data File : BG052263.D
 Acq On : 3 Feb 2022 11:15
 Operator : CG/JU
 Sample : PB142430BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK430

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG013122.M
 Title : SVOA CALIBRATION

Signal : TIC: BG052263.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.561	9	12	21	rVV2	9418	14830	1.38%	0.148%
2	3.655	24	28	33	rVV4	1037	1653	0.15%	0.017%
3	3.848	59	61	67	rVB5	1173	1821	0.17%	0.018%
4	3.995	81	86	100	rBV	104639	195685	18.26%	1.956%
5	7.385	656	663	673	rBV	144305	246512	23.00%	2.464%
6	7.549	684	691	699	rVB	101870	176350	16.45%	1.763%
7	7.767	721	728	735	rBV	133101	233976	21.83%	2.339%
8	8.242	802	809	816	rBV	102379	169622	15.82%	1.696%
9	8.947	920	929	936	rBV	169027	292337	27.27%	2.922%
10	9.411	999	1008	1019	rVB	138562	241861	22.56%	2.418%
11	10.146	1126	1133	1144	rVB	115876	207606	19.37%	2.075%
12	10.692	1218	1226	1234	rBV	173198	304919	28.45%	3.048%
13	11.080	1284	1292	1300	rVB	132445	238742	22.27%	2.387%
14	11.203	1305	1313	1322	rBV	164068	299118	27.91%	2.990%
15	12.654	1557	1560	1567	rVB4	2655	3832	0.36%	0.038%
16	14.270	1827	1835	1842	rBV	351690	491684	45.87%	4.915%
17	14.575	1879	1887	1895	rBV	375487	584786	54.56%	5.846%
18	14.881	1933	1939	1946	rVB	224156	346424	32.32%	3.463%
19	15.063	1964	1970	1983	rBV	126212	232177	21.66%	2.321%
20	15.867	2100	2107	2114	rBV	468515	733999	68.48%	7.337%
21	15.979	2120	2126	2137	rBV	141651	215255	20.08%	2.152%
22	16.108	2145	2148	2153	rVB3	1913	2193	0.20%	0.022%
23	17.060	2306	2310	2314	rVB	1924	2333	0.22%	0.023%
24	17.630	2400	2407	2413	rBV	302661	454264	42.38%	4.541%
25	17.730	2417	2424	2435	rVB	543291	861114	80.34%	8.608%
26	18.029	2472	2475	2480	rVB2	2886	4058	0.38%	0.041%
27	18.570	2563	2567	2572	rVB	4468	5432	0.51%	0.054%
28	19.574	2733	2738	2744	rVV3	7663	10669	1.00%	0.107%
29	19.645	2745	2750	2752	rVV2	7128	10085	0.94%	0.101%
30	19.674	2752	2755	2759	rVV2	6504	8315	0.78%	0.083%
31	20.003	2805	2811	2822	rBV	745861	1071884	100.00%	10.715%
32	20.162	2836	2838	2841	rVV2	1131	1653	0.15%	0.017%
33	20.361	2871	2872	2874	rBV	1812	1869	0.17%	0.019%
34	20.690	2924	2928	2930	rBV5	1420	1913	0.18%	0.019%
35	20.902	2960	2964	2966	rBV3	4358	4692	0.44%	0.047%
36	21.219	3015	3018	3020	rVB3	1657	1859	0.17%	0.019%

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG020322\
 Data File : BG052263.D
 Acq On : 3 Feb 2022 11:15
 Operator : CG/JU
 Sample : PB142430BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK430

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG013122.M
 Title : SVOA CALIBRATION

37	21.248	3020	3023	3026	rBV5	1701	2708	0.25%	0.027%
38	21.313	3030	3034	3037	rBV5	2217	3211	0.30%	0.032%
39	21.354	3039	3041	3042	rBV2	1934	1803	0.17%	0.018%
40	21.454	3056	3058	3061	rBV3	1737	1860	0.17%	0.019%
41	21.654	3089	3092	3093	rVB2	2500	1843	0.17%	0.018%
42	21.736	3104	3106	3109	rVB4	2121	1758	0.16%	0.018%
43	21.801	3112	3117	3121	rVV5	5091	7803	0.73%	0.078%
44	21.942	3133	3141	3148	rBV	304481	526198	49.09%	5.260%
45	21.989	3148	3149	3156	rVB4	8665	9801	0.91%	0.098%
46	22.288	3196	3200	3201	rVB4	1859	1774	0.17%	0.018%
47	22.400	3216	3219	3222	rBV3	3183	4127	0.39%	0.041%
48	22.523	3238	3240	3243	rVB3	1641	1636	0.15%	0.016%
49	22.758	3278	3280	3281	rBV3	2318	2287	0.21%	0.023%
50	22.952	3311	3313	3316	rBV2	1604	1845	0.17%	0.018%
51	23.099	3331	3338	3341	rBV5	4909	9238	0.86%	0.092%
52	23.316	3371	3375	3377	rBV4	2508	3486	0.33%	0.035%
53	23.522	3406	3410	3418	rVB6	6778	12874	1.20%	0.129%
54	23.745	3445	3448	3450	rBV4	2161	2434	0.23%	0.024%
55	24.009	3488	3493	3494	rBV5	1405	2027	0.19%	0.020%
56	24.233	3529	3531	3534	rBV4	2146	2429	0.23%	0.024%
57	24.297	3539	3542	3544	rBV3	3436	3858	0.36%	0.039%
58	24.397	3552	3559	3561	rBV7	8173	17168	1.60%	0.172%
59	24.550	3582	3585	3587	rBV3	1999	1885	0.18%	0.019%
60	24.650	3600	3602	3603	rVB	3616	1791	0.17%	0.018%
61	24.673	3603	3606	3607	rBV3	2326	2711	0.25%	0.027%
62	25.172	3680	3691	3703	rBV2	327754	1002993	93.57%	10.027%
63	25.419	3720	3733	3747	rVB2	168000	537758	50.17%	5.376%
64	25.525	3747	3751	3752	rBV3	1807	1805	0.17%	0.018%
65	25.590	3760	3762	3764	rBV3	2194	2211	0.21%	0.022%
66	25.607	3764	3765	3769	rBV3	2132	2514	0.23%	0.025%
67	25.842	3803	3805	3808	rVB4	2038	2238	0.21%	0.022%
68	25.877	3808	3811	3813	rBV3	2231	3063	0.29%	0.031%
69	25.960	3822	3825	3828	rBV4	2067	2529	0.24%	0.025%
70	25.995	3828	3831	3834	rBV5	1889	2443	0.23%	0.024%
71	26.112	3849	3851	3855	rBV4	2178	2666	0.25%	0.027%
72	26.635	3938	3940	3941	rBV2	2414	2260	0.21%	0.023%
73	26.676	3941	3947	3957	rVB10	10819	32746	3.05%	0.327%
74	27.023	4004	4006	4009	rVB2	2641	2686	0.25%	0.027%
75	27.046	4009	4010	4013	rBV4	2086	1922	0.18%	0.019%
76	27.182	4030	4033	4034	rBV3	1635	2055	0.19%	0.021%

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG020322\
 Data File : BG052263.D
 Acq On : 3 Feb 2022 11:15
 Operator : CG/JU
 Sample : PB142430BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK430

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG013122.M
 Title : SVOA CALIBRATION

77	27.287	4048	4051	4053	rVB3	3406	2777	0.26%	0.028%
78	27.364	4062	4064	4067	rBV3	2349	2417	0.23%	0.024%
79	27.393	4067	4069	4071	rBV3	2041	2101	0.20%	0.021%
80	28.074	4183	4185	4187	rBV3	1941	1986	0.19%	0.020%
81	28.174	4193	4202	4212	rBV9	9385	37711	3.52%	0.377%
82	28.826	4309	4313	4316	rBV6	2549	3503	0.33%	0.035%
83	28.914	4327	4328	4332	rVB3	2530	2509	0.23%	0.025%
84	29.191	4373	4375	4377	rBV3	2129	1758	0.16%	0.018%
85	29.290	4390	4392	4393	rVB2	3100	1673	0.16%	0.017%
86	29.514	4428	4430	4433	rBV3	1895	2212	0.21%	0.022%
87	29.619	4444	4448	4451	rBV6	2439	4033	0.38%	0.040%
88	29.801	4476	4479	4482	rBV4	2000	3109	0.29%	0.031%
89	30.313	4564	4566	4567	rBV2	1796	1756	0.16%	0.018%
90	30.465	4590	4592	4594	rBV3	2152	1662	0.16%	0.017%
91	30.542	4603	4605	4608	rBV4	2411	2247	0.21%	0.022%
92	30.865	4659	4660	4665	rVB5	1758	2244	0.21%	0.022%
93	30.935	4669	4672	4673	rBV3	1613	1820	0.17%	0.018%
94	31.006	4681	4684	4686	rBV4	1907	2176	0.20%	0.022%
95	31.153	4707	4709	4711	rBV2	1810	1788	0.17%	0.018%
96	31.305	4734	4735	4738	rBV3	2068	1970	0.18%	0.020%
97	32.134	4868	4876	4877	rBV7	4195	9089	0.85%	0.091%
98	32.145	4877	4878	4881	rVV3	2741	3047	0.28%	0.030%
99	32.333	4908	4910	4913	rBV3	2005	1781	0.17%	0.018%
100	32.557	4945	4948	4949	rBV3	2059	2081	0.19%	0.021%




Sum of corrected areas: 10003416

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG020322\
Data File : BG052263.D
Acq On : 3 Feb 2022 11:15
Operator : CG/JU
Sample : PB142430BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK430

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG013122.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

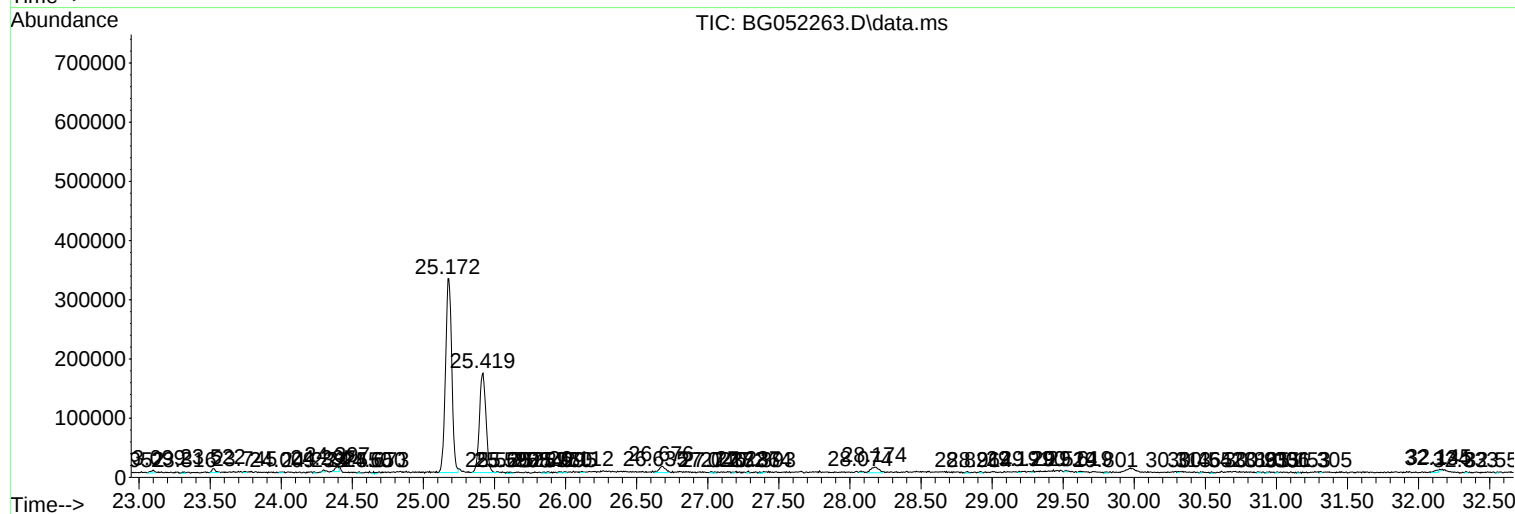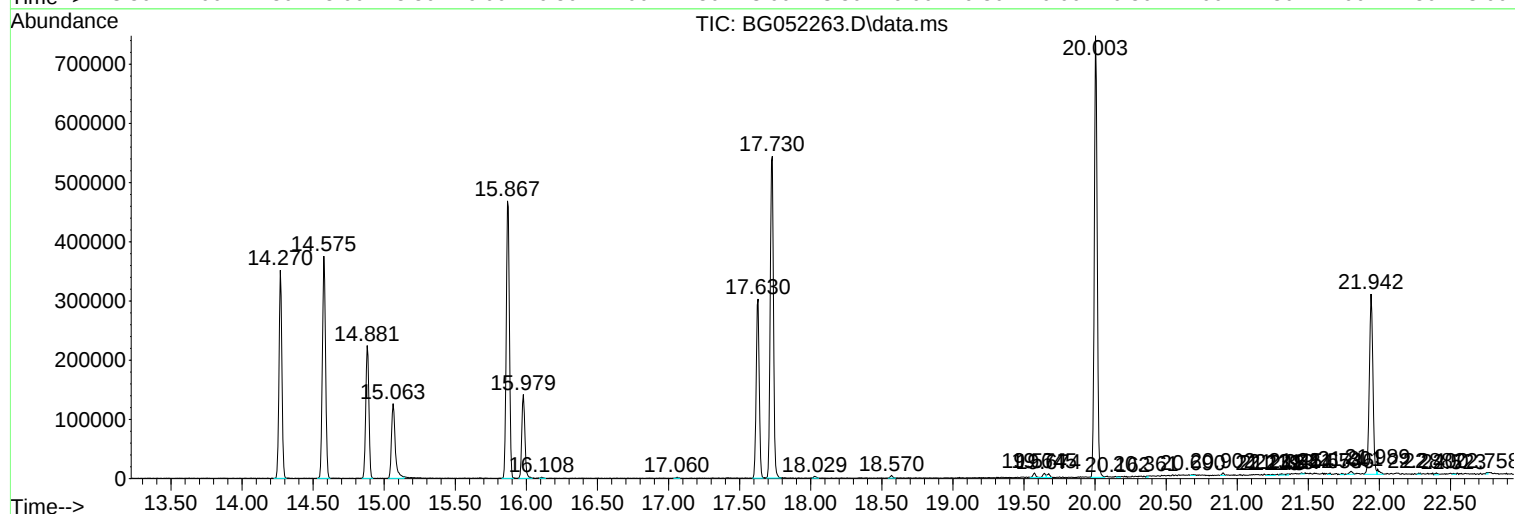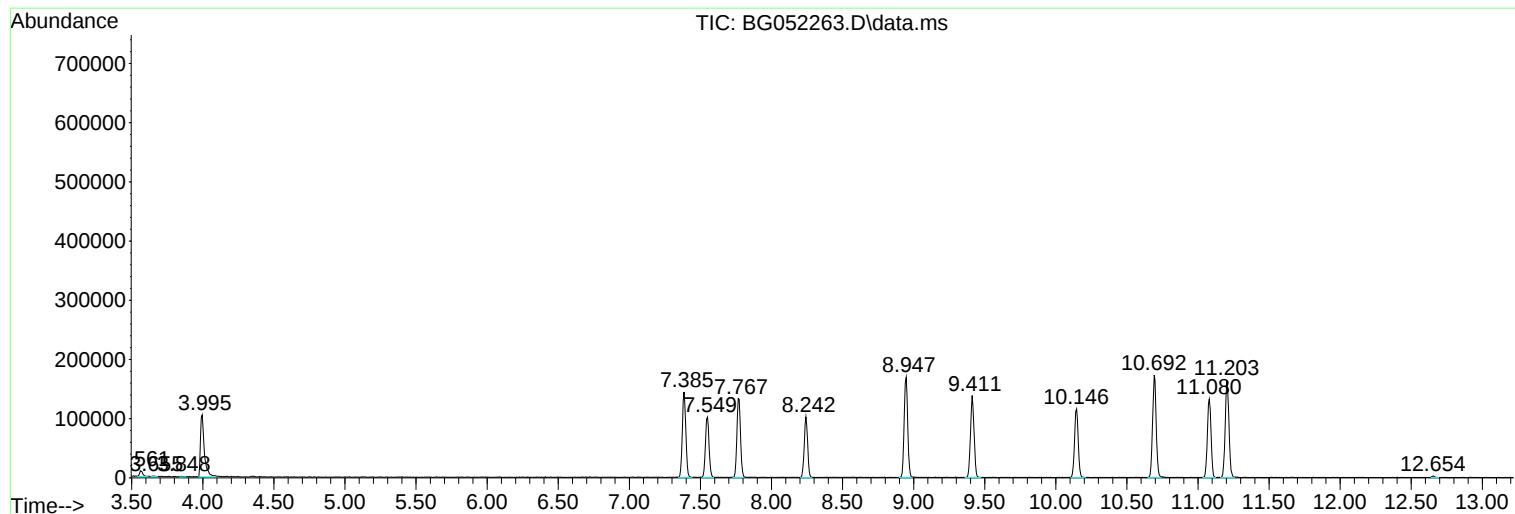

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG020322\
Data File : BG052263.D
Acq On : 3 Feb 2022 11:15
Operator : CG/JU
Sample : PB142430BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK430

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG013122.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG020322\
Data File : BG052263.D
Acq On : 3 Feb 2022 11:15
Operator : CG/JU
Sample : PB142430BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK430

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG013122.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc