

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG020322\
 Data File : BG052272.D
 Acq On : 3 Feb 2022 17:10
 Operator : CG/JU
 Sample : N1349-03
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 C0HP2

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG013122.M
 Title : SVOA CALIBRATION

Signal : TIC: BG052272.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.561	6	12	16	rBV5	5511	9009	0.93%	0.104%
2	3.772	44	48	50	rBV3	962	1325	0.14%	0.015%
3	4.002	83	87	95	rBV3	14067	26748	2.77%	0.308%
4	4.348	145	146	151	rVB4	1830	1614	0.17%	0.019%
5	4.894	233	239	250	rVB	237125	406256	42.07%	4.685%
6	5.218	293	294	301	rVB	1243	1514	0.16%	0.017%
7	5.717	374	379	382	rBV3	824	1632	0.17%	0.019%
8	7.379	653	662	670	rVB	30132	55161	5.71%	0.636%
9	7.538	683	689	698	rBV	99835	169391	17.54%	1.954%
10	7.761	721	727	736	rVB	104304	176081	18.24%	2.031%
11	8.237	800	808	815	rBV	99191	166221	17.21%	1.917%
12	8.936	921	927	936	rVB2	79841	140230	14.52%	1.617%
13	9.406	1000	1007	1016	rVB	128581	228774	23.69%	2.638%
14	9.817	1070	1077	1081	rBV3	2385	4213	0.44%	0.049%
15	10.140	1125	1132	1141	rBV	104924	186566	19.32%	2.152%
16	10.687	1218	1225	1234	rBV	142858	254896	26.40%	2.940%
17	11.074	1284	1291	1300	rVB	126560	233607	24.19%	2.694%
18	11.198	1304	1312	1321	rBV	115008	206795	21.42%	2.385%
19	12.643	1555	1558	1559	rBV	1855	1888	0.20%	0.022%
20	13.688	1732	1736	1741	rVB3	1716	2192	0.23%	0.025%
21	13.853	1760	1764	1768	rVB3	952	1280	0.13%	0.015%
22	14.270	1827	1835	1843	rBV	297435	442924	45.87%	5.108%
23	14.575	1879	1887	1894	rBV	323519	521894	54.05%	6.019%
24	14.752	1913	1917	1921	rBV2	912	1347	0.14%	0.016%
25	14.881	1928	1939	1946	rVB	210078	329755	34.15%	3.803%
26	15.063	1964	1970	1982	rBV2	20957	43495	4.50%	0.502%
27	15.697	2076	2078	2083	rVB2	1222	1307	0.14%	0.015%
28	15.868	2100	2107	2116	rBV	443473	668490	69.23%	7.710%
29	15.974	2120	2125	2136	rVV	139716	208098	21.55%	2.400%
30	16.115	2145	2149	2152	rVB2	1499	1612	0.17%	0.019%
31	17.354	2357	2360	2364	rVB4	2079	2631	0.27%	0.030%
32	17.413	2364	2370	2373	rBV2	1712	3143	0.33%	0.036%
33	17.624	2400	2406	2412	rBV	290694	431275	44.66%	4.974%
34	17.724	2416	2423	2431	rBV	561659	815095	84.41%	9.401%
35	18.564	2561	2566	2568	rBV2	963	1514	0.16%	0.017%
36	19.122	2658	2661	2662	rBV	1310	1364	0.14%	0.016%

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG020322\
 Data File : BG052272.D
 Acq On : 3 Feb 2022 17:10
 Operator : CG/JU
 Sample : N1349-03
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 C0HP2

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG013122.M
 Title : SVOA CALIBRATION

37	19.181	2667	2671	2672	rVB2	1263	1404	0.15%	0.016%
38	19.345	2697	2699	2701	rBV2	1292	1452	0.15%	0.017%
39	19.569	2731	2737	2742	rBV3	7589	10432	1.08%	0.120%
40	19.639	2744	2749	2758	rVB2	6351	12100	1.25%	0.140%
41	19.892	2788	2792	2795	rVB3	2230	2295	0.24%	0.026%
42	20.003	2804	2811	2819	rBV	670707	965619	100.00%	11.137%
43	20.368	2869	2873	2874	rBV2	2289	2031	0.21%	0.023%
44	20.873	2957	2959	2962	rBV3	1481	1631	0.17%	0.019%
45	21.208	3014	3016	3018	rBV2	2080	1729	0.18%	0.020%
46	21.936	3134	3140	3150	rBV	281736	475495	49.24%	5.484%
47	23.646	3429	3431	3432	rBV2	3013	1471	0.15%	0.017%
48	24.397	3556	3559	3566	rVB6	8707	13998	1.45%	0.161%
49	25.173	3679	3691	3703	rBV2	307472	912804	94.53%	10.527%
50	25.331	3716	3718	3720	rBV3	2467	1775	0.18%	0.020%
51	25.408	3721	3731	3745	rVB3	158166	499469	51.73%	5.760%
52	28.163	4195	4200	4202	rBV6	5739	10900	1.13%	0.126%
53	30.278	4558	4560	4561	rBV	2569	1538	0.16%	0.018%
54	31.376	4745	4747	4750	rBV4	2785	3417	0.35%	0.039%
55	31.952	4844	4845	4846	rBV	3182	1774	0.18%	0.020%




Sum of corrected areas: 8670671

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG020322\
Data File : BG052272.D
Acq On : 3 Feb 2022 17:10
Operator : CG/JU
Sample : N1349-03
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
C0HP2

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG013122.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

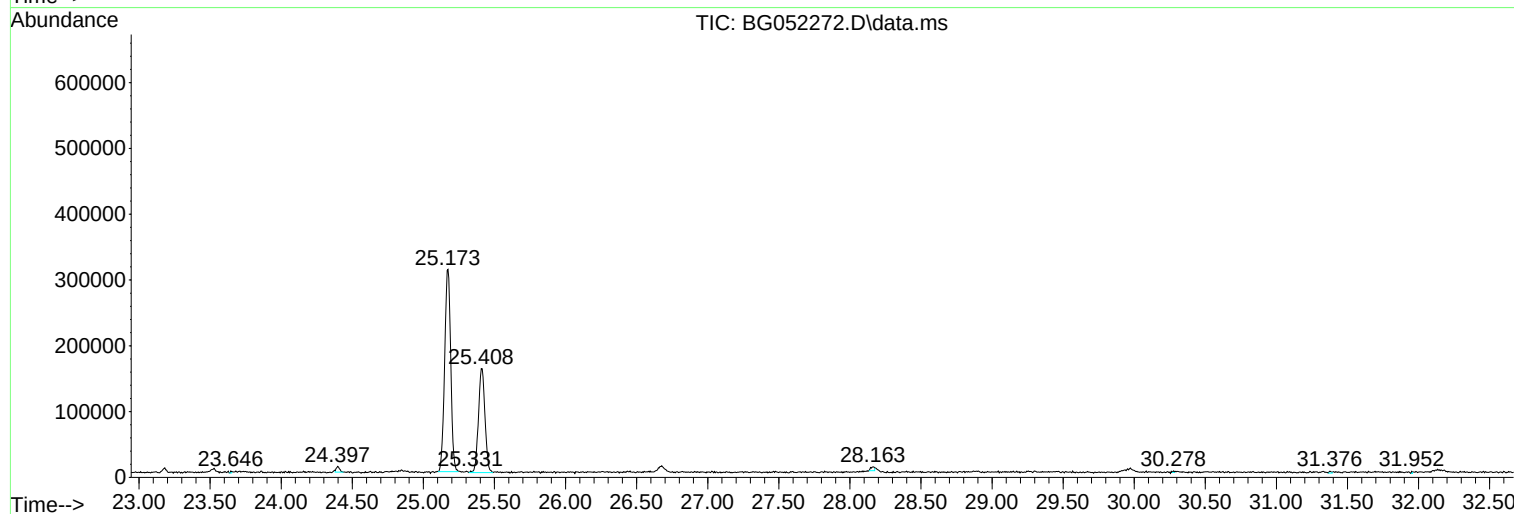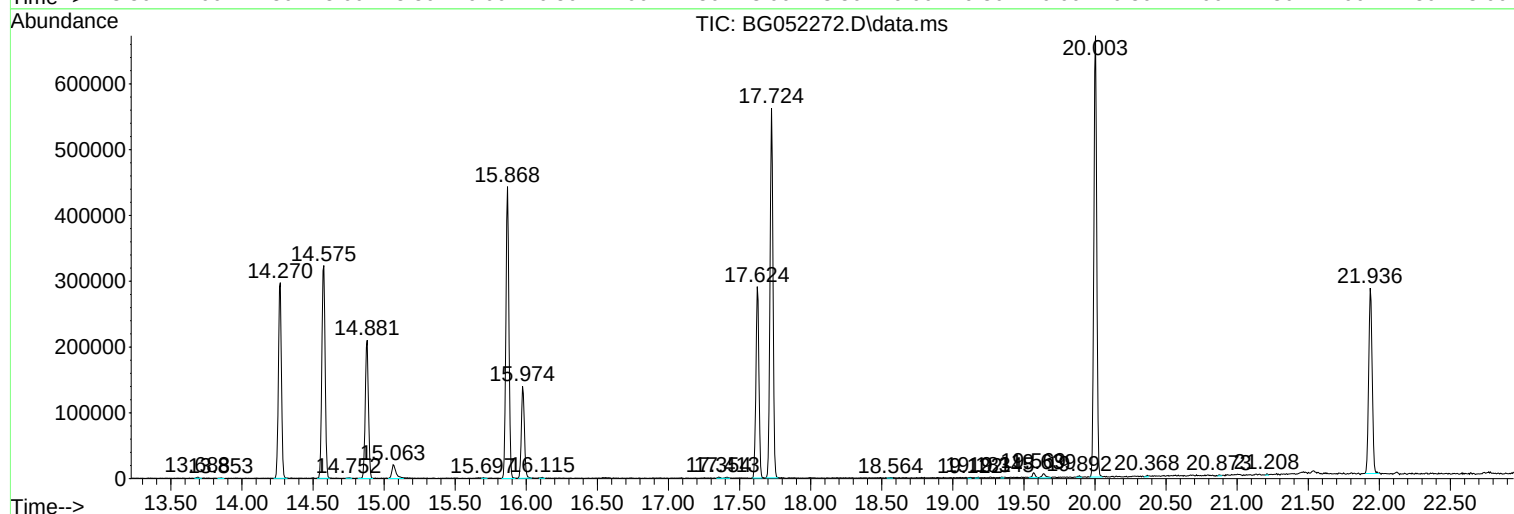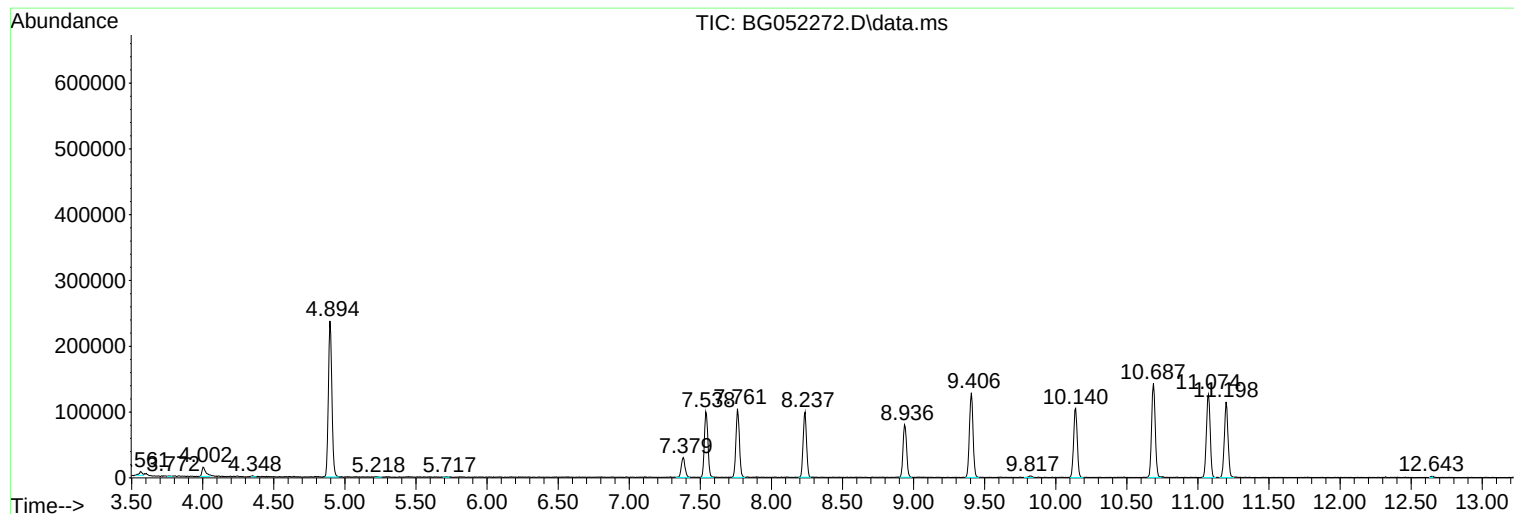

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG020322\
Data File : BG052272.D
Acq On : 3 Feb 2022 17:10
Operator : CG/JU
Sample : N1349-03
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
C0HP2

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG013122.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG020322\
Data File : BG052272.D
Acq On : 3 Feb 2022 17:10
Operator : CG/JU
Sample : N1349-03
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
C0HP2

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG013122.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc