

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG020322\
 Data File : BG052278.D
 Acq On : 3 Feb 2022 21:35
 Operator : CG/JU
 Sample : PB142431BL
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK431

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG013122.M
 Title : SVOA CALIBRATION

Signal : TIC: BG052278.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.564	9	13	18	rVV	9687	14125	1.30%	0.140%
2	3.893	65	69	72	rBV3	916	1456	0.13%	0.014%
3	3.993	81	86	100	rBV	106549	198800	18.25%	1.969%
4	4.087	100	102	106	rVB4	2330	2632	0.24%	0.026%
5	4.351	143	147	150	rVB4	1550	1997	0.18%	0.020%
6	7.376	655	662	676	rBV	144677	247499	22.72%	2.451%
7	7.541	683	690	698	rBV	107591	180229	16.55%	1.785%
8	7.764	720	728	735	rBV	139498	234525	21.53%	2.323%
9	8.234	799	808	815	rBV	102055	174956	16.06%	1.733%
10	8.939	920	928	938	rBV2	171495	298524	27.41%	2.956%
11	9.403	998	1007	1016	rVB	138058	245737	22.56%	2.434%
12	10.137	1124	1132	1138	rBV	119134	209883	19.27%	2.079%
13	10.684	1218	1225	1238	rBV2	163834	300886	27.62%	2.980%
14	11.071	1284	1291	1299	rVB	142167	245392	22.53%	2.430%
15	11.201	1305	1313	1324	rBV	165148	305605	28.06%	3.027%
16	12.646	1553	1559	1564	rBV2	3070	4271	0.39%	0.042%
17	14.267	1828	1835	1841	rBV	355545	502266	46.11%	4.974%
18	14.573	1880	1887	1897	rBV	374759	594807	54.61%	5.891%
19	14.878	1933	1939	1946	rVB2	221694	352613	32.37%	3.492%
20	15.060	1964	1970	1983	rBV2	130524	231123	21.22%	2.289%
21	15.871	2100	2108	2115	rBV	492264	747578	68.63%	7.404%
22	15.976	2120	2126	2139	rBV	146224	221510	20.34%	2.194%
23	16.112	2144	2149	2154	rVB2	1750	2893	0.27%	0.029%
24	17.416	2366	2371	2373	rBV	1454	1728	0.16%	0.017%
25	17.627	2400	2407	2417	rVB	316710	468634	43.02%	4.641%
26	17.727	2417	2424	2433	rBV	589769	872714	80.12%	8.643%
27	18.737	2593	2596	2601	rBV	701	1490	0.14%	0.015%
28	19.407	2707	2710	2715	rBV2	722	1439	0.13%	0.014%
29	19.478	2718	2722	2724	rVV3	1049	1550	0.14%	0.015%
30	19.572	2734	2738	2742	rVV4	9459	11714	1.08%	0.116%
31	19.636	2746	2749	2757	rVB2	6857	10909	1.00%	0.108%
32	19.924	2794	2798	2801	rBV4	1015	1622	0.15%	0.016%
33	20.006	2805	2812	2821	rVB	764012	1089285	100.00%	10.788%
34	20.106	2826	2829	2831	rBV4	1258	1539	0.14%	0.015%
35	20.388	2876	2877	2881	rVB3	1764	1579	0.14%	0.016%
36	20.435	2881	2885	2886	rBV2	1474	1819	0.17%	0.018%

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG020322\
 Data File : BG052278.D
 Acq On : 3 Feb 2022 21:35
 Operator : CG/JU
 Sample : PB142431BL
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK431

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG013122.M
 Title : SVOA CALIBRATION

37	20.476	2889	2892	2893	rBV	2196	1880	0.17%	0.019%
38	20.588	2907	2911	2912	rVV3	2019	2212	0.20%	0.022%
39	20.605	2912	2914	2917	rVB3	1188	1404	0.13%	0.014%
40	20.776	2941	2943	2945	rBV2	1473	1381	0.13%	0.014%
41	20.952	2970	2973	2976	rBV5	1213	1657	0.15%	0.016%
42	20.993	2979	2980	2982	rBV	2242	1411	0.13%	0.014%
43	21.463	3058	3060	3063	rBV3	2191	2814	0.26%	0.028%
44	21.757	3109	3110	3114	rVB4	2261	2204	0.20%	0.022%
45	21.798	3114	3117	3119	rBV4	1610	1895	0.17%	0.019%
46	21.939	3134	3141	3150	rVV	322916	535512	49.16%	5.304%
47	22.062	3160	3162	3167	rVB5	1897	2500	0.23%	0.025%
48	22.109	3168	3170	3172	rBV3	1682	1473	0.14%	0.015%
49	22.256	3193	3195	3198	rVB3	1468	1646	0.15%	0.016%
50	22.309	3202	3204	3207	rBV4	1432	1633	0.15%	0.016%
51	22.503	3235	3237	3238	rVB2	2685	1416	0.13%	0.014%
52	23.225	3359	3360	3362	rBV2	2591	1663	0.15%	0.016%
53	23.531	3405	3412	3420	rBV9	5129	13403	1.23%	0.133%
54	23.719	3442	3444	3448	rVB4	1682	1423	0.13%	0.014%
55	24.406	3554	3561	3567	rBV8	6214	14008	1.29%	0.139%
56	24.565	3584	3588	3591	rVV5	1623	2391	0.22%	0.024%
57	24.906	3644	3646	3649	rVV3	2313	1877	0.17%	0.019%
58	25.176	3679	3692	3706	rBV	358720	1061238	97.43%	10.510%
59	25.417	3721	3733	3748	rVB2	178725	549020	50.40%	5.437%
60	25.558	3755	3757	3761	rBV4	2362	3519	0.32%	0.035%
61	25.675	3776	3777	3779	rBV2	2066	1382	0.13%	0.014%
62	25.781	3791	3795	3798	rBV6	1873	2159	0.20%	0.021%
63	26.116	3851	3852	3854	rBV2	1533	1556	0.14%	0.015%
64	26.268	3876	3878	3880	rBV3	2427	1889	0.17%	0.019%
65	26.550	3924	3926	3929	rVB2	1898	1724	0.16%	0.017%
66	26.597	3933	3934	3938	rBV4	2202	2897	0.27%	0.029%
67	26.686	3940	3949	3952	rBV6	6905	16487	1.51%	0.163%
68	26.815	3969	3971	3973	rBV3	1887	1440	0.13%	0.014%
69	27.120	4021	4023	4028	rVB5	1742	2265	0.21%	0.022%
70	27.220	4038	4040	4045	rBV4	1767	2834	0.26%	0.028%
71	27.684	4116	4119	4120	rVB3	2060	1905	0.17%	0.019%
72	27.714	4120	4124	4126	rBV5	1915	2811	0.26%	0.028%
73	27.808	4138	4140	4143	rBV4	1431	1548	0.14%	0.015%
74	27.902	4153	4156	4157	rBV3	1707	2056	0.19%	0.020%
75	27.996	4170	4172	4173	rBV2	1919	1465	0.13%	0.015%
76	28.166	4197	4201	4202	rBV4	4384	5647	0.52%	0.056%

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG020322\
 Data File : BG052278.D
 Acq On : 3 Feb 2022 21:35
 Operator : CG/JU
 Sample : PB142431BL
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK431

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG013122.M
 Title : SVOA CALIBRATION

77	28.548	4264	4266	4270	rBV5	2426	3914	0.36%	0.039%
78	28.583	4270	4272	4275	rVB4	2109	1717	0.16%	0.017%
79	28.642	4280	4282	4285	rBV4	1494	1466	0.13%	0.015%
80	28.953	4334	4335	4338	rBV3	1796	1387	0.13%	0.014%
81	29.276	4388	4390	4395	rBV5	1894	2543	0.23%	0.025%
82	29.399	4410	4411	4414	rBV2	2137	1876	0.17%	0.019%
83	29.441	4416	4418	4420	rVB2	2118	1504	0.14%	0.015%
84	29.605	4443	4446	4448	rVB4	1519	1850	0.17%	0.018%
85	29.652	4452	4454	4458	rVV3	1672	2115	0.19%	0.021%
86	29.711	4461	4464	4467	rBV5	1920	2594	0.24%	0.026%
87	29.963	4505	4507	4509	rBV3	3149	3269	0.30%	0.032%
88	30.216	4548	4550	4552	rBV2	2365	2158	0.20%	0.021%
89	30.392	4578	4580	4581	rVB2	2583	1384	0.13%	0.014%
90	30.480	4592	4595	4597	rBV3	2215	2838	0.26%	0.028%
91	30.551	4605	4607	4610	rVB3	2349	1818	0.17%	0.018%
92	30.674	4626	4628	4632	rVV3	2446	2885	0.26%	0.029%
93	31.209	4717	4719	4723	rBV4	1332	1737	0.16%	0.017%
94	31.461	4760	4762	4764	rBV2	1944	1998	0.18%	0.020%
95	31.743	4809	4810	4812	rBV2	1817	1460	0.13%	0.014%
96	31.890	4831	4835	4838	rBV6	1692	2725	0.25%	0.027%
97	31.972	4847	4849	4852	rBV3	2502	1955	0.18%	0.019%
98	32.096	4867	4870	4871	rBV2	1997	1788	0.16%	0.018%
99	32.131	4871	4876	4877	rBV4	2326	3821	0.35%	0.038%
100	32.243	4893	4895	4897	rVB3	1664	1504	0.14%	0.015%




Sum of corrected areas: 10097280

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG020322\
Data File : BG052278.D
Acq On : 3 Feb 2022 21:35
Operator : CG/JU
Sample : PB142431BL
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK431

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG013122.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

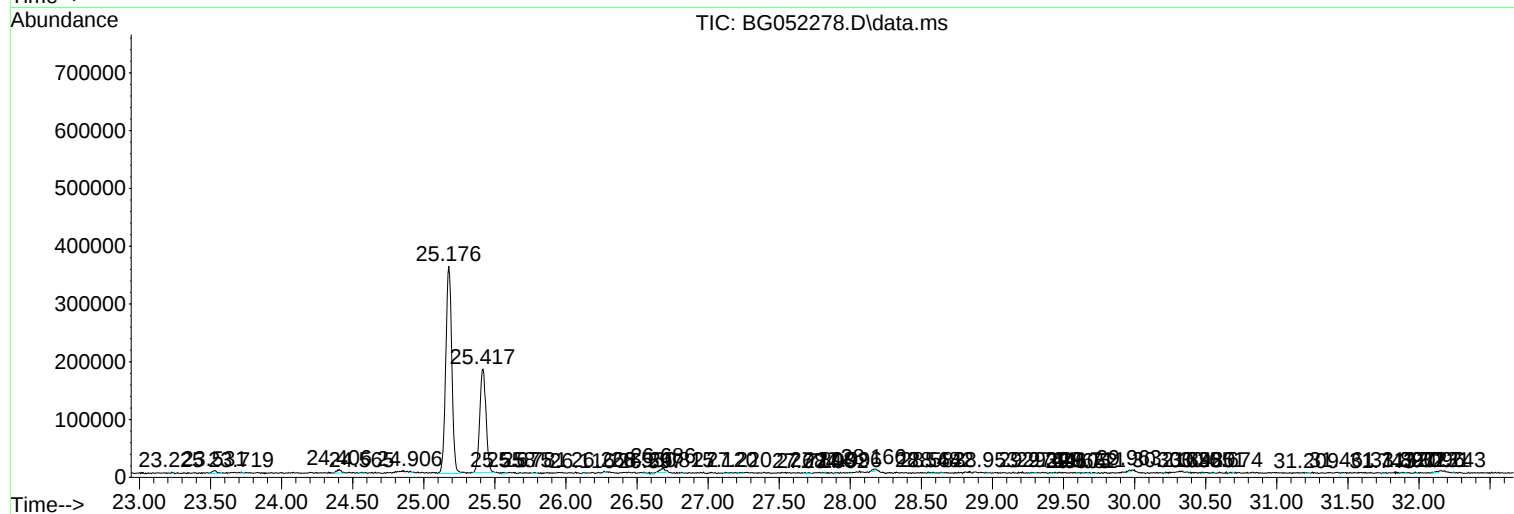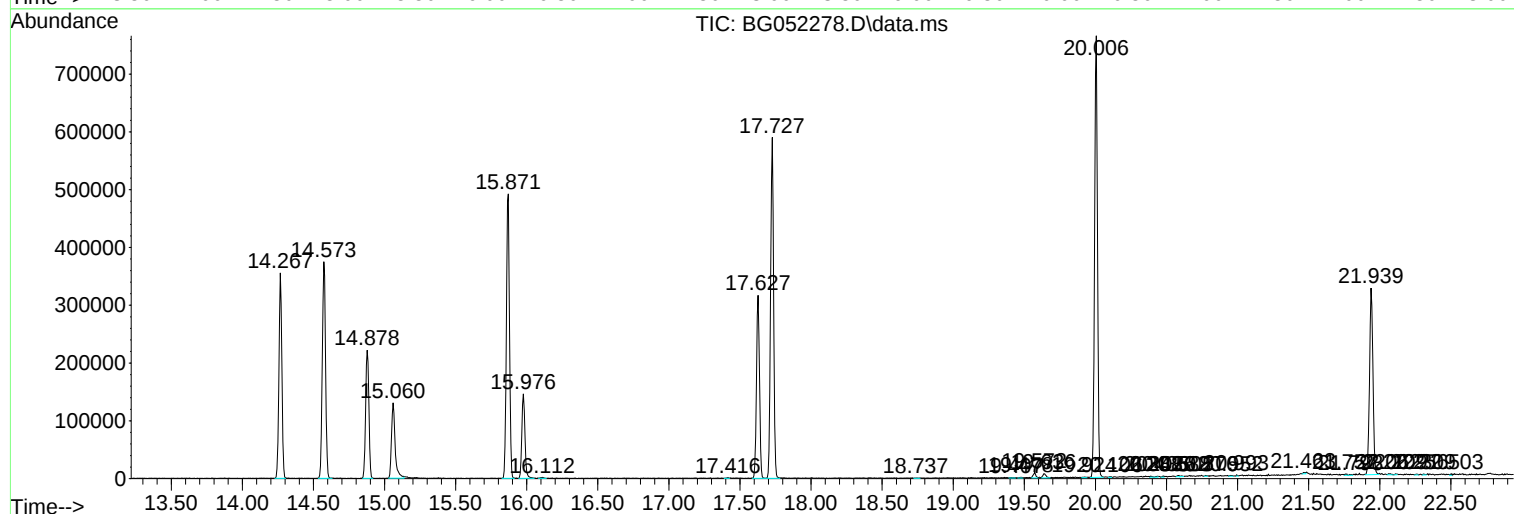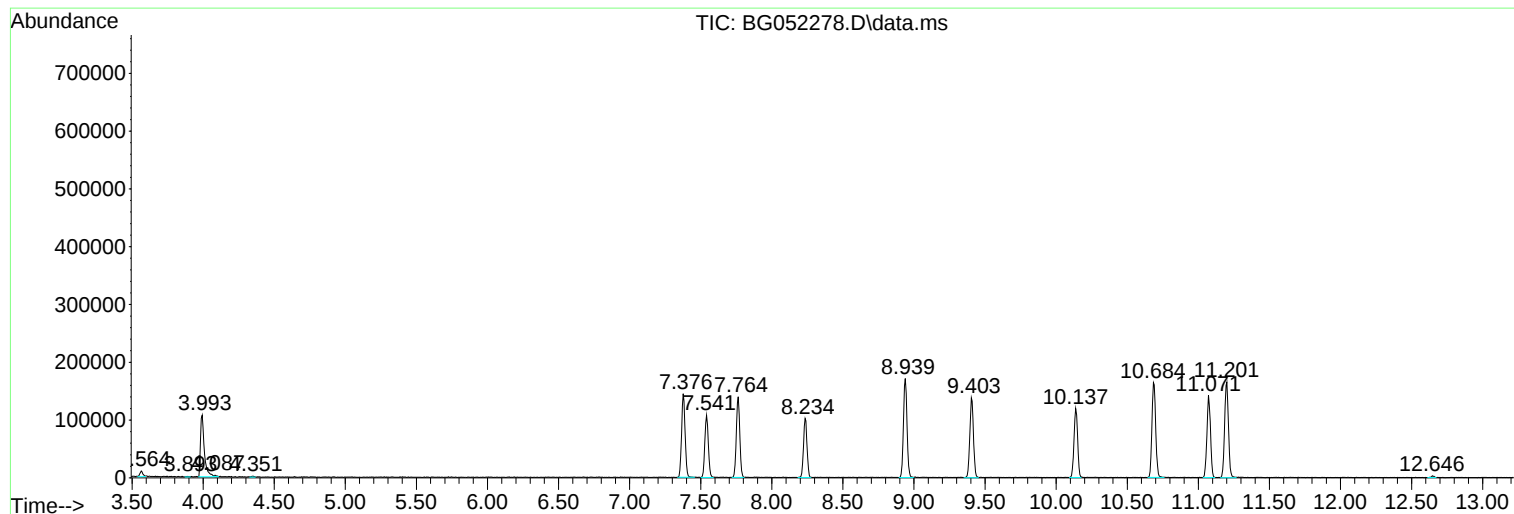

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG020322\
Data File : BG052278.D
Acq On : 3 Feb 2022 21:35
Operator : CG/JU
Sample : PB142431BL
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK431

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG013122.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG020322\
Data File : BG052278.D
Acq On : 3 Feb 2022 21:35
Operator : CG/JU
Sample : PB142431BL
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK431

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG013122.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc