

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG020322\
 Data File : BG052280.D
 Acq On : 3 Feb 2022 22:50
 Operator : CG/JU
 Sample : PB142414BL
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK414

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG013122.M
 Title : SVOA CALIBRATION

Signal : TIC: BG052280.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.564	8	13	17	rBV2	8299	13310	1.35%	0.138%
2	3.858	59	63	65	rBV2	1025	1422	0.14%	0.015%
3	3.993	81	86	100	rBV	102795	195859	19.89%	2.024%
4	4.345	142	146	152	rVB3	2702	4569	0.46%	0.047%
5	7.376	655	662	673	rVB	138430	239768	24.35%	2.478%
6	7.541	683	690	701	rVB	104257	174883	17.76%	1.807%
7	7.764	721	728	735	rVB	130476	226108	22.96%	2.337%
8	8.234	801	808	815	rVB	111830	189229	19.22%	1.956%
9	8.939	921	928	937	rBV	161803	280363	28.48%	2.898%
10	9.403	999	1007	1022	rBV	130829	241834	24.56%	2.499%
11	10.137	1124	1132	1143	rBV	113672	199723	20.28%	2.064%
12	10.684	1217	1225	1238	rBV	152918	282436	28.69%	2.919%
13	11.071	1284	1291	1300	rBV	146197	267180	27.14%	2.761%
14	11.195	1305	1312	1322	rBV	154483	281700	28.61%	2.911%
15	12.652	1555	1560	1564	rVB4	2056	3398	0.35%	0.035%
16	14.267	1828	1835	1842	rBV	328116	462866	47.01%	4.784%
17	14.573	1880	1887	1894	rBV	344675	545629	55.42%	5.639%
18	14.878	1932	1939	1948	rBV	246342	384967	39.10%	3.979%
19	15.060	1963	1970	1986	rBV2	112739	213993	21.73%	2.212%
20	15.160	1986	1987	1991	rVV3	1536	2001	0.20%	0.021%
21	15.865	2101	2107	2117	rVB	445739	677129	68.77%	6.998%
22	15.977	2120	2126	2135	rVV	138586	201663	20.48%	2.084%
23	16.035	2135	2136	2142	rVB2	1555	1774	0.18%	0.018%
24	17.627	2400	2407	2414	rBV	333781	507224	51.52%	5.242%
25	17.727	2417	2424	2435	rVV2	511459	809888	82.26%	8.370%
26	17.944	2456	2461	2466	rBV3	920	1908	0.19%	0.020%
27	19.566	2733	2737	2742	rBV4	6220	9128	0.93%	0.094%
28	19.642	2746	2750	2756	rVB	6168	8223	0.84%	0.085%
29	20.006	2805	2812	2821	rVV	699397	984592	100.00%	10.176%
30	20.353	2868	2871	2876	rBV3	1421	2161	0.22%	0.022%
31	20.535	2901	2902	2905	rVB2	1817	1535	0.16%	0.016%
32	20.570	2905	2908	2909	rBV3	1407	1396	0.14%	0.014%
33	20.582	2909	2910	2914	rBV3	1397	1498	0.15%	0.015%
34	20.688	2924	2928	2929	rBV5	1261	1594	0.16%	0.016%
35	20.741	2929	2937	2940	rBV5	2440	5019	0.51%	0.052%
36	20.917	2965	2967	2969	rBV3	1857	1450	0.15%	0.015%

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG020322\
 Data File : BG052280.D
 Acq On : 3 Feb 2022 22:50
 Operator : CG/JU
 Sample : PB142414BL
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK414

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG013122.M
 Title : SVOA CALIBRATION

37	21.328	3036	3037	3040	rBV3	1645	1977	0.20%	0.020%
38	21.475	3059	3062	3065	rBV5	3188	3005	0.31%	0.031%
39	21.545	3070	3074	3076	rBV3	2195	3763	0.38%	0.039%
40	21.739	3104	3107	3108	rVV3	2171	1709	0.17%	0.018%

41	21.822	3119	3121	3124	rVB4	2124	2376	0.24%	0.025%
42	21.939	3133	3141	3149	rBV	341337	563809	57.26%	5.827%
43	22.391	3216	3218	3220	rBV3	1171	1317	0.13%	0.014%
44	22.491	3233	3235	3238	rBV3	1349	1994	0.20%	0.021%
45	22.556	3245	3246	3250	rVB3	2196	2263	0.23%	0.023%

46	22.773	3281	3283	3287	rVB4	3209	4075	0.41%	0.042%
47	22.808	3287	3289	3291	rBV3	1431	1783	0.18%	0.018%
48	23.267	3363	3367	3368	rBV3	1788	1573	0.16%	0.016%
49	23.478	3400	3403	3404	rBV3	1820	1507	0.15%	0.016%
50	23.525	3406	3411	3412	rBV4	4597	5504	0.56%	0.057%

51	23.590	3420	3422	3424	rBV3	2244	1651	0.17%	0.017%
52	23.678	3434	3437	3438	rVB2	1701	1306	0.13%	0.013%
53	23.831	3462	3463	3466	rBV3	2103	1937	0.20%	0.020%
54	24.177	3520	3522	3524	rBV3	2589	2105	0.21%	0.022%
55	24.201	3524	3526	3527	rVV2	2318	1578	0.16%	0.016%

56	24.218	3527	3529	3533	rVB5	2255	2467	0.25%	0.025%
57	24.259	3533	3536	3537	rBV3	1440	1351	0.14%	0.014%
58	24.301	3539	3543	3544	rBV3	1762	2151	0.22%	0.022%
59	24.400	3556	3560	3566	rVB8	8458	13977	1.42%	0.144%
60	24.782	3624	3625	3628	rBV2	2166	1644	0.17%	0.017%

61	24.835	3632	3634	3636	rBV3	2054	1797	0.18%	0.019%
62	24.929	3649	3650	3652	rBV2	1563	1428	0.15%	0.015%
63	25.041	3666	3669	3670	rBV3	1810	1888	0.19%	0.020%
64	25.182	3680	3693	3704	rVV	314624	950798	96.57%	9.826%
65	25.417	3721	3733	3746	rVV4	183220	587165	59.64%	6.068%

66	25.605	3762	3765	3767	rVB4	2329	2091	0.21%	0.022%
67	25.628	3767	3769	3771	rBV3	1345	1384	0.14%	0.014%
68	26.221	3868	3870	3873	rBV3	1819	1764	0.18%	0.018%
69	26.427	3902	3905	3908	rBV4	1643	1648	0.17%	0.017%
70	26.668	3942	3946	3948	rBV5	6482	8437	0.86%	0.087%

71	26.968	3996	3997	3999	rBV2	2091	1498	0.15%	0.015%
72	27.044	4008	4010	4013	rVB4	1347	1432	0.15%	0.015%
73	27.150	4026	4028	4029	rBV2	2134	2027	0.21%	0.021%
74	27.167	4029	4031	4032	rVV	2498	1714	0.17%	0.018%
75	27.179	4032	4033	4037	rVB4	2120	2083	0.21%	0.022%

76	27.332	4058	4059	4062	rVV2	2081	1430	0.15%	0.015%
----	--------	------	------	------	------	------	------	-------	--------

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG020322\
 Data File : BG052280.D
 Acq On : 3 Feb 2022 22:50
 Operator : CG/JU
 Sample : PB142414BL
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK414

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG013122.M
 Title : SVOA CALIBRATION

77	27.596	4103	4104	4108	rVV3	1675	1314	0.13%	0.014%
78	27.743	4127	4129	4133	rBV4	1661	1474	0.15%	0.015%
79	27.954	4163	4165	4168	rVB4	1542	1454	0.15%	0.015%
80	28.001	4171	4173	4175	rBV2	1693	1720	0.17%	0.018%
81	28.125	4193	4194	4195	rBV	2938	1587	0.16%	0.016%
82	28.166	4195	4201	4202	rVV4	4885	8480	0.86%	0.088%
83	28.283	4219	4221	4224	rVB3	1686	1675	0.17%	0.017%
84	29.006	4341	4344	4345	rBV3	2312	1827	0.19%	0.019%
85	29.123	4361	4364	4366	rBV3	1388	1934	0.20%	0.020%
86	29.229	4380	4382	4384	rBV3	1668	1402	0.14%	0.014%
87	29.746	4469	4470	4475	rBV5	1910	2044	0.21%	0.021%
88	29.958	4502	4506	4508	rBV5	3947	5870	0.60%	0.061%
89	30.063	4522	4524	4526	rBV2	1341	1440	0.15%	0.015%
90	30.257	4555	4557	4560	rVV3	1484	1749	0.18%	0.018%
91	30.610	4615	4617	4619	rBV2	1759	1838	0.19%	0.019%
92	30.698	4630	4632	4636	rVB6	2166	2642	0.27%	0.027%
93	30.733	4636	4638	4641	rBV3	1600	2140	0.22%	0.022%
94	30.798	4648	4649	4651	rBV2	2065	1757	0.18%	0.018%
95	31.608	4785	4787	4791	rBV4	2368	2689	0.27%	0.028%
96	31.990	4851	4852	4855	rBV3	1762	1937	0.20%	0.020%
97	32.125	4873	4875	4876	rBV	3275	1795	0.18%	0.019%
98	32.331	4908	4910	4911	rBV2	1463	1447	0.15%	0.015%
99	32.472	4932	4934	4936	rBV2	1411	1438	0.15%	0.015%
100	32.630	4959	4961	4963	rBV2	1525	1421	0.14%	0.015%




Sum of corrected areas: 9675900

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG020322\
Data File : BG052280.D
Acq On : 3 Feb 2022 22:50
Operator : CG/JU
Sample : PB142414BL
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK414

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG013122.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

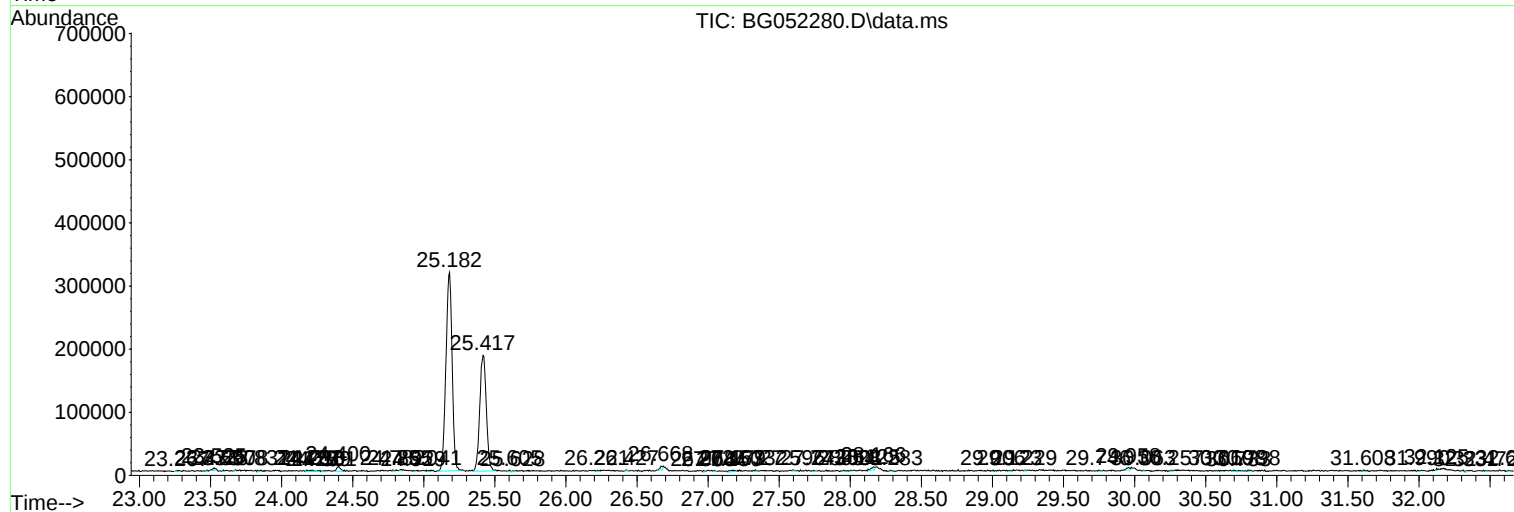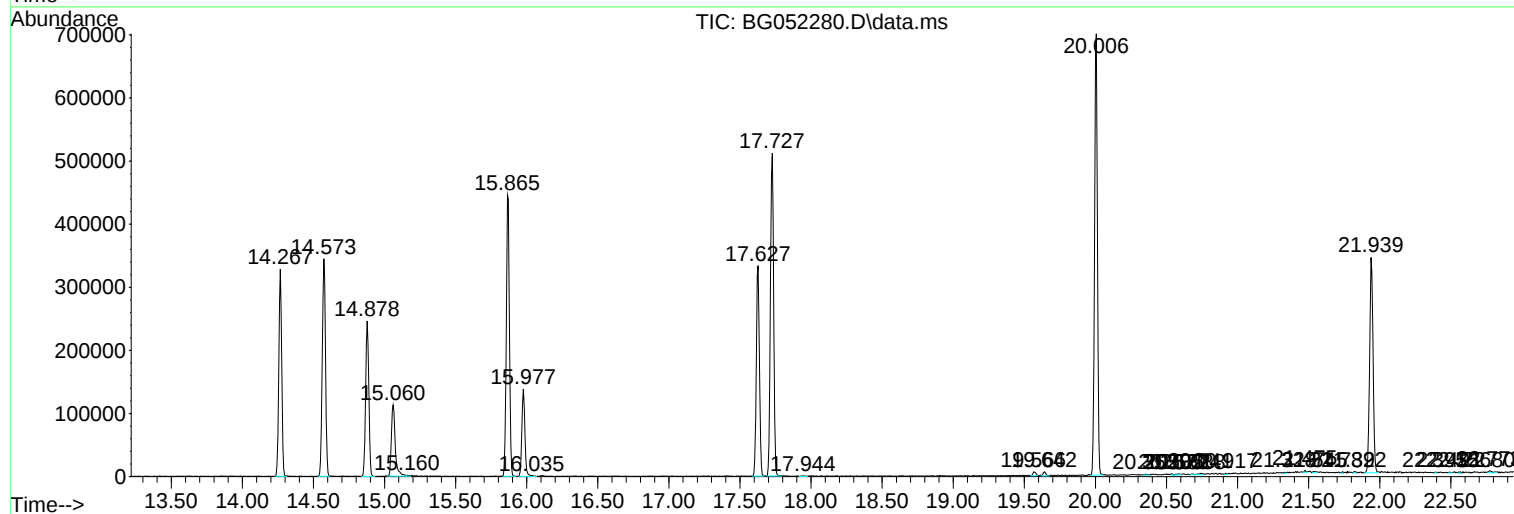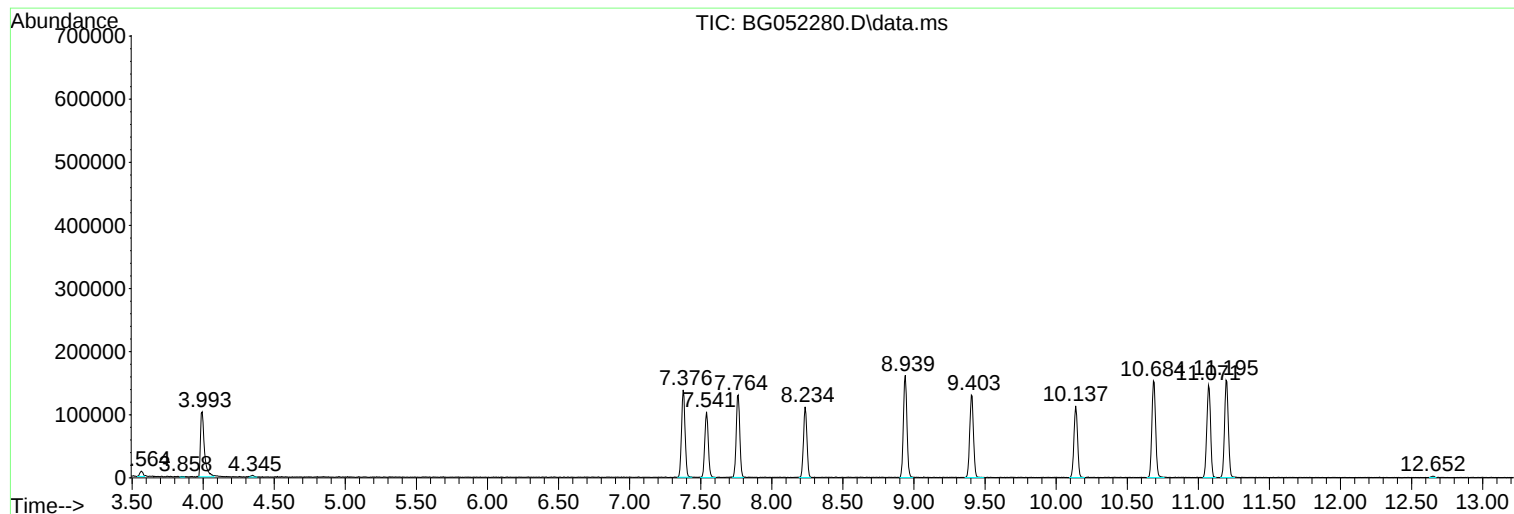

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG020322\
Data File : BG052280.D
Acq On : 3 Feb 2022 22:50
Operator : CG/JU
Sample : PB142414BL
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK414

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG013122.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG020322\
Data File : BG052280.D
Acq On : 3 Feb 2022 22:50
Operator : CG/JU
Sample : PB142414BL
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK414

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG013122.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc