

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG020322\
 Data File : BG052287.D
 Acq On : 4 Feb 2022 3:14
 Operator : CG/JU
 Sample : N1325-16
 Misc :
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 TEX-2

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG013122.M
 Title : SVOA CALIBRATION

Signal : TIC: BG052287.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.543	5	9	10	rBV2	5881	7079	0.69%	0.131%
2	3.561	10	12	16	rVV3	5656	7610	0.74%	0.141%
3	3.602	16	19	23	rVV4	3787	5080	0.49%	0.094%
4	3.795	49	52	57	rVB5	1129	2184	0.21%	0.040%
5	4.001	84	87	93	rBV2	13521	21891	2.12%	0.404%
6	4.894	233	239	252	rVB	601784	1031822	100.00%	19.062%
7	7.379	655	662	668	rBV3	16175	25642	2.49%	0.474%
8	7.543	681	690	696	rBV2	29910	52813	5.12%	0.976%
9	7.767	720	728	735	rVV2	29640	52555	5.09%	0.971%
10	8.237	801	808	815	rVB2	95630	164371	15.93%	3.037%
11	8.941	921	928	935	rBV2	24657	43517	4.22%	0.804%
12	9.406	999	1007	1015	rBV2	39755	69881	6.77%	1.291%
13	10.140	1126	1132	1139	rVV2	28463	51807	5.02%	0.957%
14	10.686	1219	1225	1234	rVV	37929	70720	6.85%	1.306%
15	11.074	1283	1291	1299	rVB	128591	232328	22.52%	4.292%
16	11.197	1302	1312	1319	rVV	37219	70231	6.81%	1.297%
17	14.264	1829	1834	1843	rBV	100061	139428	13.51%	2.576%
18	14.575	1879	1887	1895	rVB	108034	169125	16.39%	3.124%
19	14.880	1932	1939	1947	rVB	218458	334822	32.45%	6.185%
20	15.068	1966	1971	1980	rBV2	6125	13892	1.35%	0.257%
21	15.867	2100	2107	2116	rBV	150651	224040	21.71%	4.139%
22	15.979	2120	2126	2134	rBV3	26991	38804	3.76%	0.717%
23	17.630	2400	2407	2413	rBV	289955	438588	42.51%	8.102%
24	17.730	2417	2424	2430	rBV	173427	257440	24.95%	4.756%
25	19.369	2700	2703	2706	rBV4	1364	2020	0.20%	0.037%
26	19.574	2735	2738	2741	rVB5	1924	2529	0.25%	0.047%
27	19.645	2746	2750	2753	rBV3	2351	2954	0.29%	0.055%
28	19.885	2788	2791	2794	rBV4	1299	2107	0.20%	0.039%
29	20.003	2803	2811	2820	rBV	221534	322539	31.26%	5.958%
30	20.115	2827	2830	2834	rVB4	1660	2105	0.20%	0.039%
31	20.185	2837	2842	2843	rVB5	1996	1832	0.18%	0.034%
32	20.344	2866	2869	2872	rBV4	1730	2546	0.25%	0.047%
33	20.432	2881	2884	2886	rBV3	2013	2728	0.26%	0.050%
34	20.690	2924	2928	2933	rVV6	1640	2822	0.27%	0.052%
35	20.755	2936	2939	2943	rBV4	1911	2707	0.26%	0.050%
36	20.784	2943	2944	2948	rVB4	1447	1693	0.16%	0.031%

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG020322\
 Data File : BG052287.D
 Acq On : 4 Feb 2022 3:14
 Operator : CG/JU
 Sample : N1325-16
 Misc :
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 TEX-2

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG013122.M
 Title : SVOA CALIBRATION

37	20.820	2948	2950	2953	rBV3	1352	1761	0.17%	0.033%
38	20.872	2957	2959	2960	rBV	2414	1774	0.17%	0.033%
39	20.949	2969	2972	2973	rVV3	1791	2021	0.20%	0.037%
40	20.972	2974	2976	2978	rVV2	2049	1680	0.16%	0.031%
41	21.002	2979	2981	2983	rVB3	2005	1687	0.16%	0.031%
42	21.219	3012	3018	3019	rBV4	2614	4416	0.43%	0.082%
43	21.331	3027	3037	3038	rBV6	15355	37008	3.59%	0.684%
44	21.425	3042	3053	3054	rBV5	29569	79445	7.70%	1.468%
45	21.942	3135	3141	3149	rVB2	268514	455519	44.15%	8.415%
46	22.100	3165	3168	3169	rBV3	3614	4182	0.41%	0.077%
47	22.776	3280	3283	3284	rBV2	4258	4888	0.47%	0.090%
48	22.881	3299	3301	3305	rVV5	2854	3796	0.37%	0.070%
49	23.146	3344	3346	3349	rBV4	1942	2330	0.23%	0.043%
50	23.193	3352	3354	3357	rBV3	2679	2744	0.27%	0.051%
51	23.445	3393	3397	3398	rBV4	3072	3678	0.36%	0.068%
52	23.522	3406	3410	3416	rVB8	7116	13771	1.33%	0.254%
53	24.009	3491	3493	3496	rBV4	2109	2133	0.21%	0.039%
54	24.227	3528	3530	3533	rBV4	2178	2161	0.21%	0.040%
55	24.274	3536	3538	3540	rVB3	2791	1758	0.17%	0.032%
56	24.397	3557	3559	3566	rVB6	8354	14310	1.39%	0.264%
57	24.808	3625	3629	3631	rBV5	3515	5063	0.49%	0.094%
58	25.020	3663	3665	3668	rVB4	1946	2018	0.20%	0.037%
59	25.049	3668	3670	3672	rBV2	2050	2047	0.20%	0.038%
60	25.178	3682	3692	3701	rBV2	98401	273511	26.51%	5.053%
61	25.302	3709	3713	3716	rBV5	2190	2614	0.25%	0.048%
62	25.419	3720	3733	3743	rVV2	158660	484377	46.94%	8.948%
63	25.519	3747	3750	3751	rBV3	2395	1757	0.17%	0.032%
64	25.631	3768	3769	3772	rBV3	2322	2338	0.23%	0.043%
65	25.778	3792	3794	3795	rBV2	2856	2335	0.23%	0.043%
66	25.954	3822	3824	3828	rBV5	1848	3237	0.31%	0.060%
67	26.212	3866	3868	3869	rBV2	3164	1712	0.17%	0.032%
68	26.682	3942	3948	3957	rVB9	9731	30701	2.98%	0.567%
69	26.876	3979	3981	3984	rBV3	2180	2298	0.22%	0.042%
70	26.911	3985	3987	3992	rVV5	1904	2674	0.26%	0.049%
71	26.970	3995	3997	4000	rVB3	2056	2111	0.20%	0.039%
72	27.058	4009	4012	4015	rBV4	3121	3955	0.38%	0.073%
73	27.123	4022	4023	4027	rVB4	2261	1831	0.18%	0.034%
74	27.510	4088	4089	4092	rVV3	2270	1904	0.18%	0.035%
75	27.552	4095	4096	4101	rBV4	2000	3214	0.31%	0.059%
76	27.728	4124	4126	4128	rBV3	2447	2067	0.20%	0.038%

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG020322\
 Data File : BG052287.D
 Acq On : 4 Feb 2022 3:14
 Operator : CG/JU
 Sample : N1325-16
 Misc :
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 TEX-2

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG013122.M
 Title : SVOA CALIBRATION

77	28.145	4193	4197	4198	rBV4	3881	4567	0.44%	0.084%
78	28.174	4198	4202	4203	rVV4	4080	5935	0.58%	0.110%
79	28.427	4243	4245	4247	rBV3	2518	2150	0.21%	0.040%
80	28.491	4253	4256	4258	rVB3	2468	3052	0.30%	0.056%
81	28.562	4267	4268	4273	rVB4	3168	2525	0.24%	0.047%
82	28.738	4296	4298	4301	rBV4	1534	1788	0.17%	0.033%
83	28.815	4309	4311	4313	rBV3	1875	2534	0.25%	0.047%
84	28.850	4316	4317	4320	rBV2	2146	2197	0.21%	0.041%
85	29.026	4345	4347	4348	rBV2	2261	1780	0.17%	0.033%
86	29.050	4350	4351	4353	rBV2	2963	2425	0.24%	0.045%
87	29.144	4364	4367	4368	rBV3	3406	3851	0.37%	0.071%
88	29.837	4483	4485	4488	rBV3	3686	2956	0.29%	0.055%
89	30.465	4590	4592	4593	rBV2	2568	2323	0.23%	0.043%
90	30.501	4596	4598	4601	rVB4	3038	2509	0.24%	0.046%
91	30.741	4638	4639	4642	rBV3	3092	2186	0.21%	0.040%
92	30.941	4671	4673	4676	rBV4	2127	2346	0.23%	0.043%
93	30.994	4680	4682	4685	rBV4	2010	2144	0.21%	0.040%
94	31.023	4685	4687	4689	rVB4	2439	1817	0.18%	0.034%
95	31.194	4714	4716	4719	rBV3	3106	3667	0.36%	0.068%
96	31.223	4719	4721	4722	rBV2	2998	1856	0.18%	0.034%
97	31.382	4745	4748	4749	rBV3	2717	3047	0.30%	0.056%
98	31.399	4749	4751	4752	rVB2	3306	1864	0.18%	0.034%
99	31.863	4828	4830	4834	rBV5	2978	4481	0.43%	0.083%
100	32.316	4906	4907	4910	rBV3	2330	2032	0.20%	0.038%




Sum of corrected areas: 5413110

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG020322\
Data File : BG052287.D
Acq On : 4 Feb 2022 3:14
Operator : CG/JU
Sample : N1325-16
Misc :
ALS Vial : 27 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
TEX-2

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG013122.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

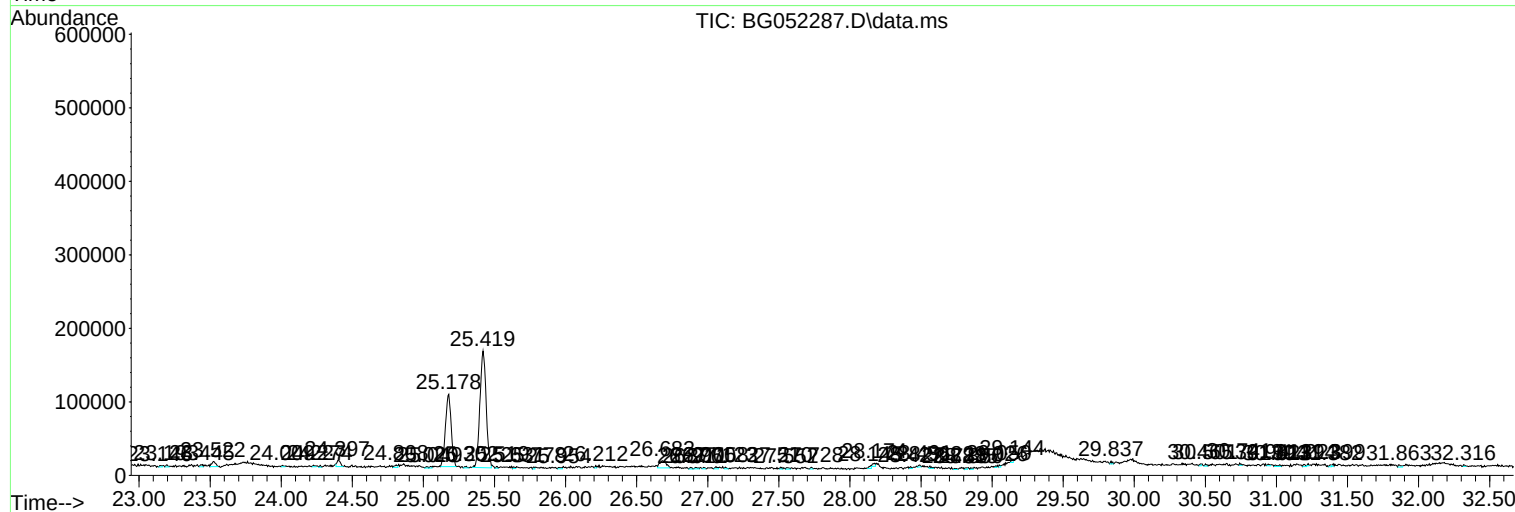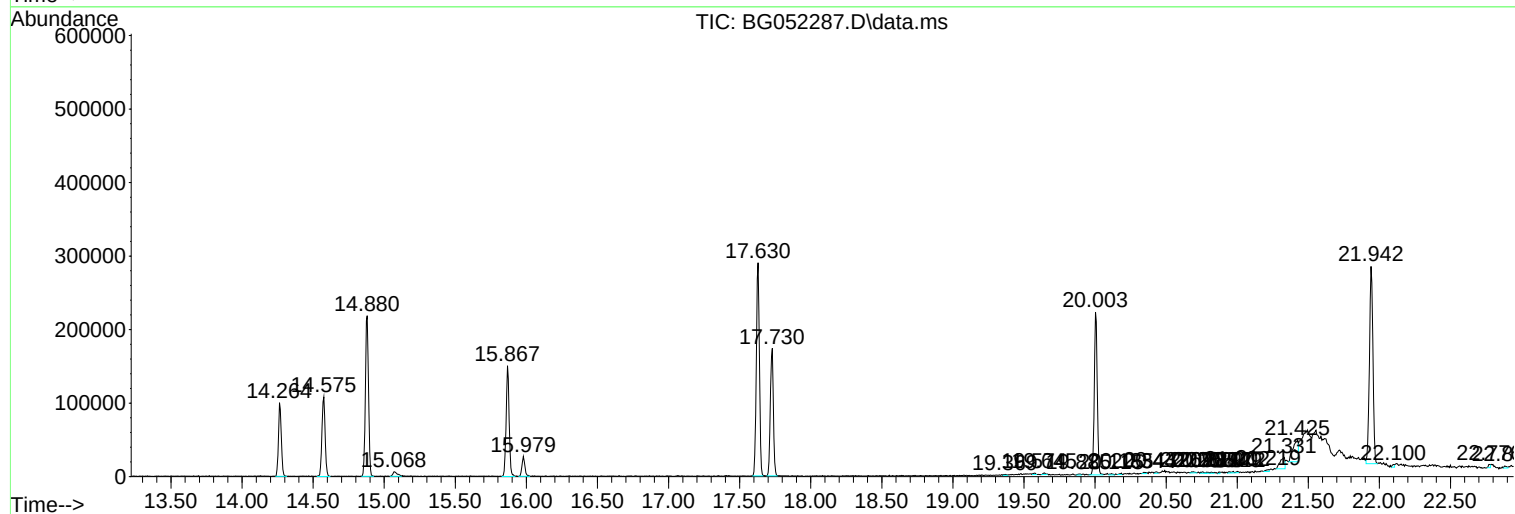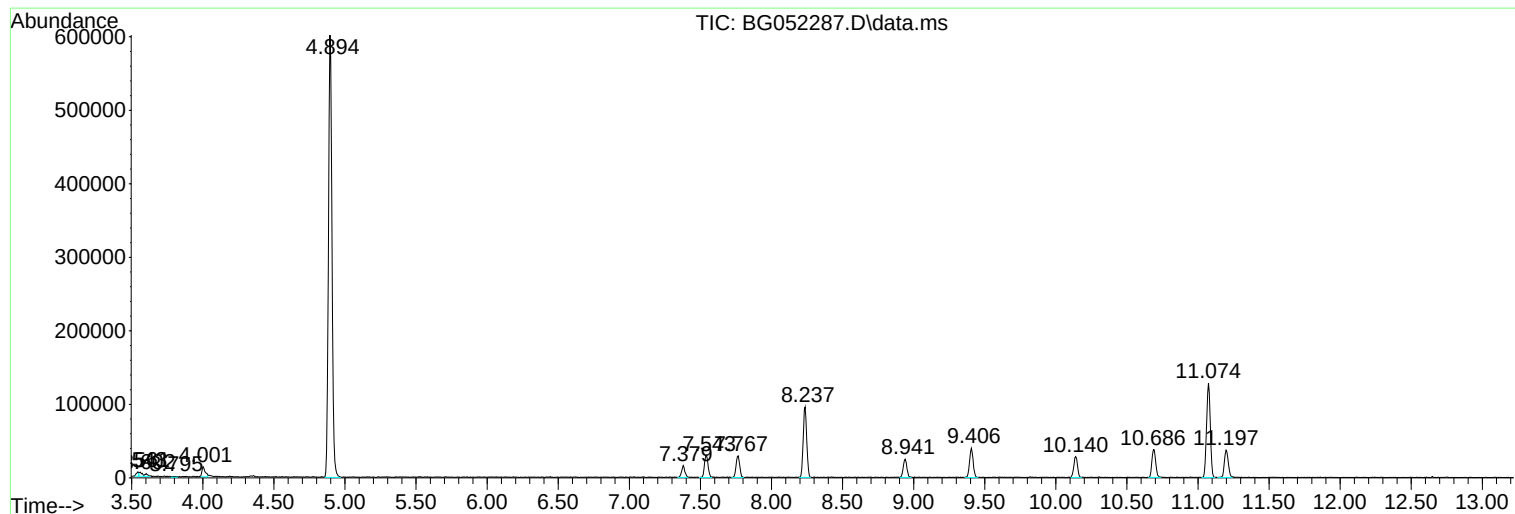

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG020322\
Data File : BG052287.D
Acq On : 4 Feb 2022 3:14
Operator : CG/JU
Sample : N1325-16
Misc :
ALS Vial : 27 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
TEX-2










Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG013122.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 2 unknown-01 Concentration Rank 2

R.T.	EstConc	Area	Relative to ISTD	R.T.
21.425	3.49 ng/ul	79445	Chrysene-d12	21.942

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Heptasiloxane, hexadecamethyl-	532	C16H48O6Si7	000541-01-5	47
2			1,1,1,3,3,5,5,7,7,9,9,11,11,13,1...	680	C20H60O8Si9	002652-13-3	38
3			Cyclononasiloxane, octadecamethyl-	666	C18H54O9Si9	000556-71-8	38
4			Hexasiloxane, tetradecamethyl-	458	C14H42O5Si6	000107-52-8	37
5			1,1,1,3,3,5,5,7,7,9,9,11,11,13,1...	606	C18H54O7Si8	000556-69-4	22

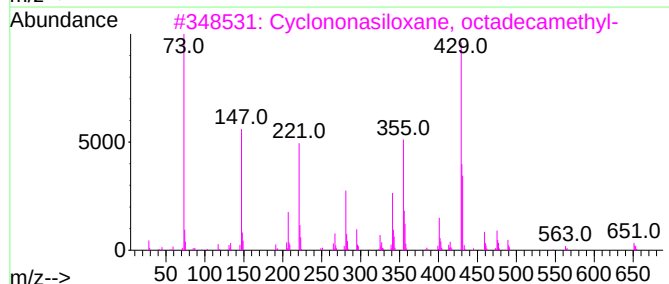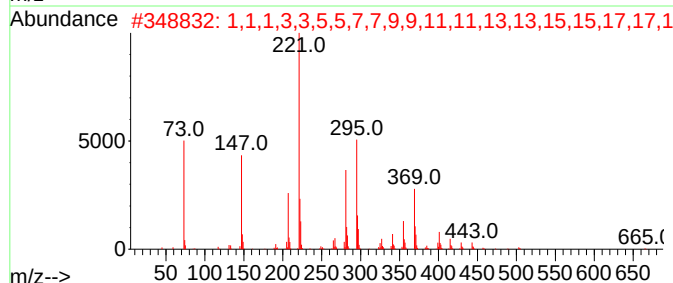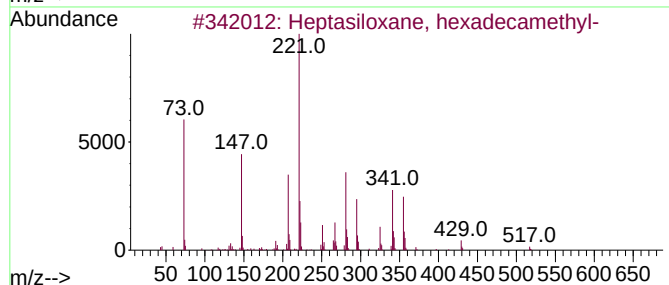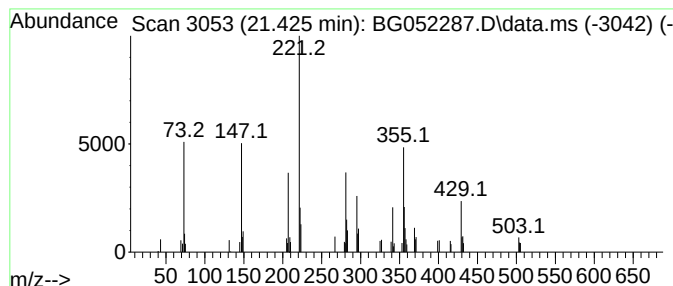

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG020322\
Data File : BG052287.D
Acq On : 4 Feb 2022 3:14
Operator : CG/JU
Sample : N1325-16
Misc :
ALS Vial : 27 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
TEX-2

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG013122.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
unknown-01	21.425	3.5	ng/u1	79445	5	21.942	455519	20.0