

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG020322\
 Data File : BG052294.D
 Acq On : 4 Feb 2022 10:16
 Operator : CG/JU
 Sample : PB142414BL
 Misc :
 ALS Vial : 35 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK414

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG013122.M
 Title : SVOA CALIBRATION

Signal : TIC: BG052294.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.574	9	14	22	rVB4	9167	16769	1.56%	0.157%
2	4.003	82	87	101	rBV	116865	220778	20.48%	2.071%
3	4.355	143	147	154	rVB4	2413	4320	0.40%	0.041%
4	7.398	658	665	672	rBV	154873	276118	25.61%	2.590%
5	7.557	685	692	701	rBV	115706	201440	18.69%	1.889%
6	7.780	723	730	740	rBV2	150356	262439	24.34%	2.461%
7	8.256	804	811	818	rVB	112443	193887	17.99%	1.819%
8	8.955	923	930	938	rBV	186088	326294	30.27%	3.060%
9	9.425	1003	1010	1019	rBV	151713	267569	24.82%	2.510%
10	10.153	1127	1134	1143	rBV	127319	230227	21.36%	2.159%
11	10.705	1221	1228	1239	rBV	187447	333402	30.93%	3.127%
12	11.087	1286	1293	1302	rBV	155266	269993	25.04%	2.532%
13	11.217	1307	1315	1325	rVB	179456	333608	30.95%	3.129%
14	12.667	1556	1562	1570	rBV3	3333	6214	0.58%	0.058%
15	14.277	1830	1836	1846	rVB	366780	541269	50.21%	5.077%
16	14.583	1881	1888	1896	rBV	406315	642957	59.64%	6.030%
17	14.888	1933	1940	1947	rBV	245033	384849	35.70%	3.610%
18	15.070	1965	1971	1984	rBV	126134	228668	21.21%	2.145%
19	15.246	1998	2001	2005	rVB2	1063	1555	0.14%	0.015%
20	15.881	2102	2109	2118	rVB	511599	793326	73.59%	7.441%
21	15.987	2121	2127	2139	rBV	134375	207709	19.27%	1.948%
22	16.116	2146	2149	2153	rVB3	2120	2328	0.22%	0.022%
23	17.308	2348	2352	2355	rBV2	1090	1554	0.14%	0.015%
24	17.426	2367	2372	2377	rBV2	1360	2197	0.20%	0.021%
25	17.637	2401	2408	2418	rBV	326854	486385	45.12%	4.562%
26	17.737	2418	2425	2437	rBV	596197	908428	84.27%	8.520%
27	19.300	2689	2691	2695	rVV3	1124	1589	0.15%	0.015%
28	19.364	2697	2702	2703	rVV3	1412	2196	0.20%	0.021%
29	19.576	2734	2738	2746	rBV3	7652	10121	0.94%	0.095%
30	19.646	2747	2750	2756	rVB2	7815	10327	0.96%	0.097%
31	19.875	2785	2789	2793	rVB3	1069	1776	0.16%	0.017%
32	20.010	2806	2812	2819	rVV	741442	1078042	100.00%	10.111%
33	20.663	2920	2923	2927	rVV3	2155	3258	0.30%	0.031%
34	20.762	2939	2940	2943	rBV3	2067	1920	0.18%	0.018%
35	21.156	3006	3007	3009	rBV2	1761	1827	0.17%	0.017%
36	21.221	3016	3018	3022	rBV3	1292	1783	0.17%	0.017%

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG020322\
 Data File : BG052294.D
 Acq On : 4 Feb 2022 10:16
 Operator : CG/JU
 Sample : PB142414BL
 Misc :
 ALS Vial : 35 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK414

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG013122.M
 Title : SVOA CALIBRATION

37	21.444	3054	3056	3058	rBV3	3028	3333	0.31%	0.031%
38	21.467	3058	3060	3063	rVV4	2780	4159	0.39%	0.039%
39	21.555	3073	3075	3076	rVB2	2850	1685	0.16%	0.016%
40	21.644	3088	3090	3093	rBV4	1828	1625	0.15%	0.015%
41	21.949	3135	3142	3153	rBV	311100	534209	49.55%	5.010%
42	22.125	3171	3172	3176	rVB4	2593	2414	0.22%	0.023%
43	22.666	3261	3264	3266	rBV3	2113	2545	0.24%	0.024%
44	22.713	3270	3272	3274	rVB2	2651	1704	0.16%	0.016%
45	22.760	3278	3280	3281	rVV	3202	2570	0.24%	0.024%
46	22.783	3281	3284	3291	rVB6	5425	8498	0.79%	0.080%
47	23.089	3335	3336	3339	rBV3	2655	2170	0.20%	0.020%
48	23.153	3346	3347	3349	rBV2	2683	1868	0.17%	0.018%
49	23.535	3409	3412	3419	rVB8	7672	14516	1.35%	0.136%
50	23.711	3438	3442	3447	rVV5	3995	6960	0.65%	0.065%
51	23.823	3459	3461	3463	rBV2	2005	1593	0.15%	0.015%
52	23.864	3466	3468	3469	rVB	2356	1568	0.15%	0.015%
53	23.882	3469	3471	3473	rBV2	1903	2044	0.19%	0.019%
54	24.422	3556	3563	3570	rVB3	12130	27662	2.57%	0.259%
55	24.857	3634	3637	3638	rBV2	3525	2870	0.27%	0.027%
56	25.192	3682	3694	3711	rVB2	346048	1021260	94.73%	9.579%
57	25.433	3723	3735	3749	rBV2	172487	566297	52.53%	5.311%
58	25.568	3756	3758	3761	rBV3	2264	2194	0.20%	0.021%
59	26.549	3923	3925	3926	rBV2	1919	1601	0.15%	0.015%
60	26.701	3942	3951	3961	rVB7	12949	42207	3.92%	0.396%
61	26.960	3993	3995	3997	rVB3	2540	1830	0.17%	0.017%
62	27.107	4018	4020	4022	rVB3	2012	1622	0.15%	0.015%
63	27.136	4022	4025	4026	rBV3	2833	1980	0.18%	0.019%
64	27.859	4146	4148	4152	rVB4	1714	1593	0.15%	0.015%
65	28.023	4173	4176	4177	rBV2	2010	2096	0.19%	0.020%
66	28.076	4182	4185	4187	rVV3	3788	4335	0.40%	0.041%
67	28.111	4189	4191	4193	rVB3	2825	1898	0.18%	0.018%
68	28.199	4196	4206	4212	rBV8	12128	39004	3.62%	0.366%
69	28.311	4224	4225	4231	rBV5	1801	2520	0.23%	0.024%
70	28.352	4231	4232	4235	rVB3	2636	2433	0.23%	0.023%
71	28.434	4244	4246	4247	rBV2	2597	1883	0.17%	0.018%
72	28.564	4267	4268	4270	rBV	2165	2006	0.19%	0.019%
73	28.646	4280	4282	4283	rBV2	2715	1631	0.15%	0.015%
74	28.922	4327	4329	4332	rVB4	1997	1923	0.18%	0.018%
75	28.963	4332	4336	4338	rVB4	1888	1913	0.18%	0.018%
76	29.010	4342	4344	4345	rBV2	2585	2188	0.20%	0.021%

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG020322\
 Data File : BG052294.D
 Acq On : 4 Feb 2022 10:16
 Operator : CG/JU
 Sample : PB142414BL
 Misc :
 ALS Vial : 35 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK414

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 0.1 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG013122.M
 Title : SVOA CALIBRATION

77	29.345	4399	4401	4406	rBV4	3745	5443	0.50%	0.051%
78	29.392	4406	4409	4410	rBV3	1727	1751	0.16%	0.016%
79	29.492	4424	4426	4429	rVB2	2209	2029	0.19%	0.019%
80	29.727	4464	4466	4468	rVB3	2297	1507	0.14%	0.014%
81	29.750	4468	4470	4471	rVB	3770	1814	0.17%	0.017%
82	29.768	4471	4473	4475	rBV3	1436	1515	0.14%	0.014%
83	29.879	4491	4492	4494	rBV	2043	1578	0.15%	0.015%
84	29.950	4502	4504	4505	rBV2	2902	2005	0.19%	0.019%
85	29.973	4505	4508	4509	rVV3	4803	5348	0.50%	0.050%
86	29.997	4509	4512	4521	rVB8	6911	19506	1.81%	0.183%
87	30.138	4534	4536	4542	rVB7	2407	2708	0.25%	0.025%
88	30.314	4565	4566	4568	rBV2	3237	2547	0.24%	0.024%
89	30.778	4644	4645	4648	rVB3	2684	1980	0.18%	0.019%
90	31.095	4697	4699	4704	rVB4	1956	3052	0.28%	0.029%
91	31.166	4710	4711	4713	rBV2	2138	1655	0.15%	0.016%
92	31.231	4719	4722	4724	rBV4	2179	2731	0.25%	0.026%
93	31.248	4724	4725	4729	rVV4	2117	1658	0.15%	0.016%
94	31.377	4745	4747	4748	rBV2	2542	1748	0.16%	0.016%
95	31.789	4813	4817	4819	rVV4	2248	2843	0.26%	0.027%
96	31.847	4825	4827	4830	rVB4	2652	2740	0.25%	0.026%
97	31.883	4830	4833	4834	rBV2	2350	2407	0.22%	0.023%
98	32.165	4877	4881	4882	rBV3	2902	4155	0.39%	0.039%
99	32.382	4916	4918	4921	rBV3	2520	1978	0.18%	0.019%
100	32.617	4957	4958	4961	rVB3	2200	1636	0.15%	0.015%




Sum of corrected areas: 10661863

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG020322\
Data File : BG052294.D
Acq On : 4 Feb 2022 10:16
Operator : CG/JU
Sample : PB142414BL
Misc :
ALS Vial : 35 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK414

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG013122.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

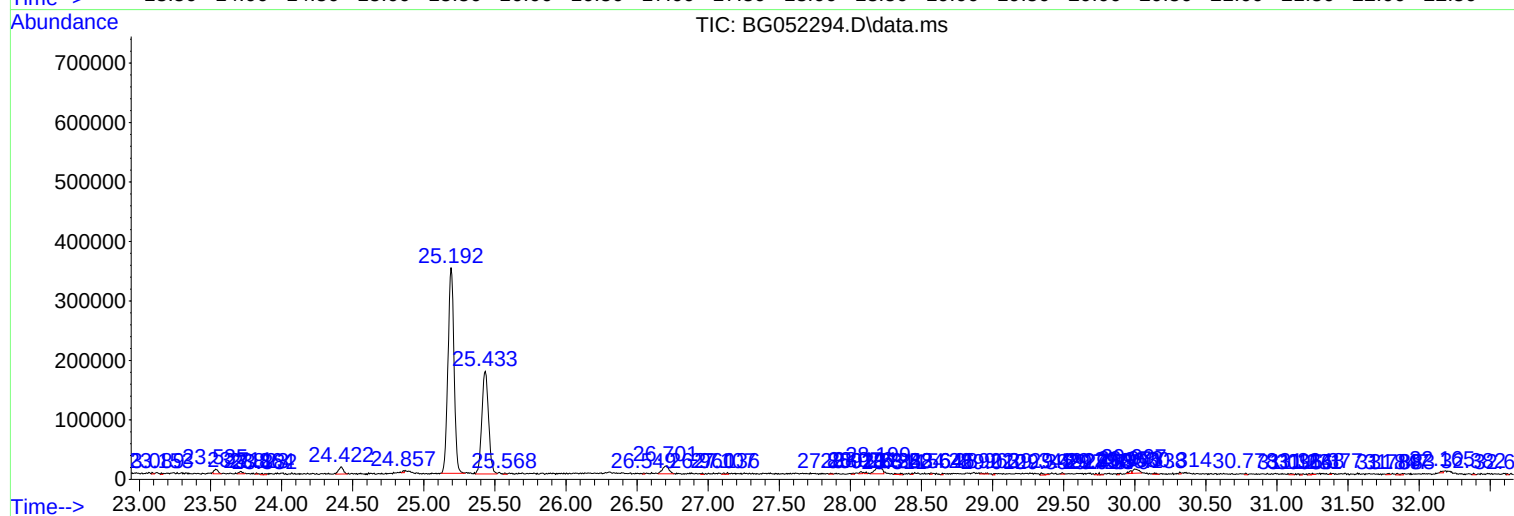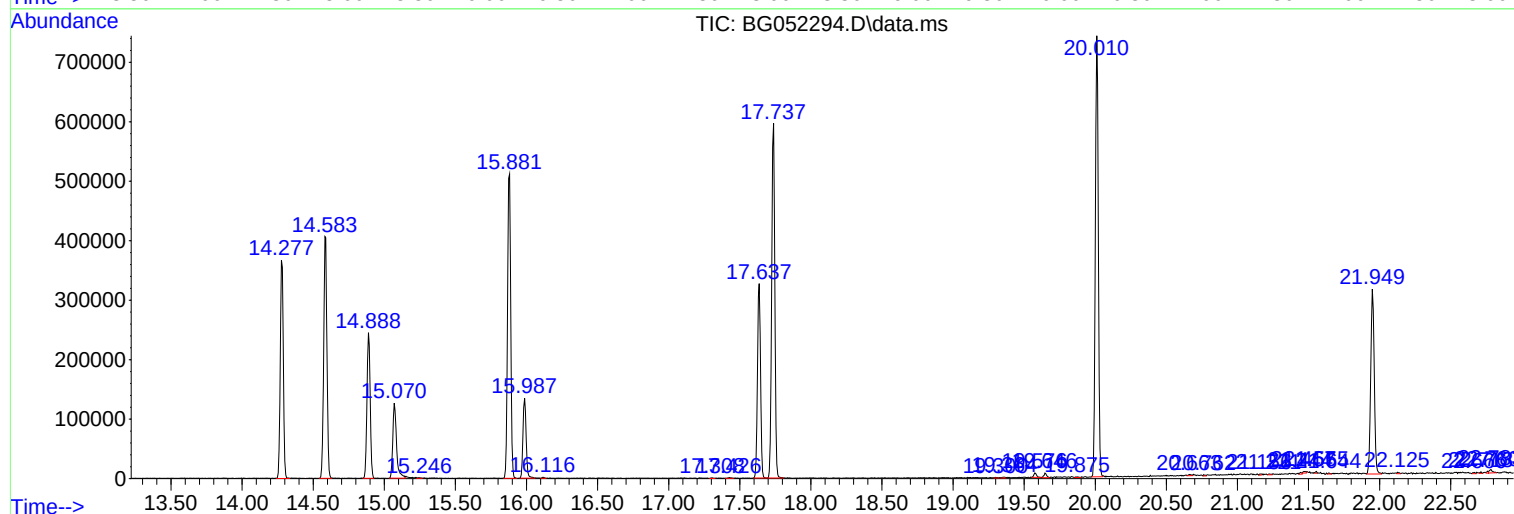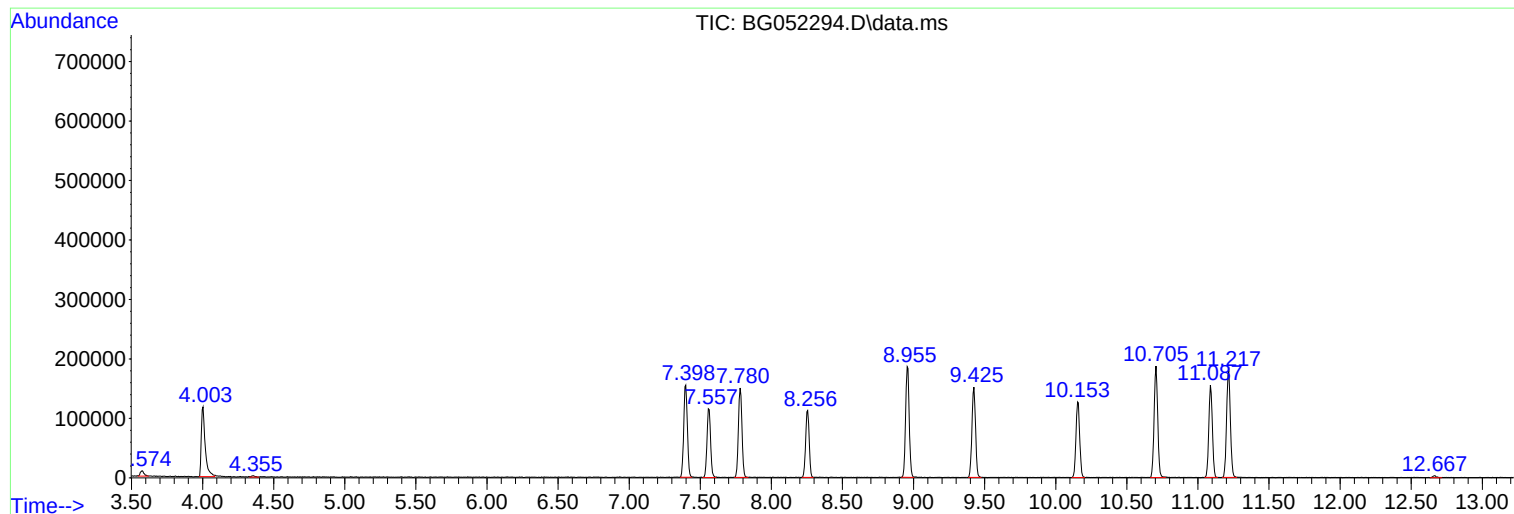

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG020322\
Data File : BG052294.D
Acq On : 4 Feb 2022 10:16
Operator : CG/JU
Sample : PB142414BL
Misc :
ALS Vial : 35 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK414

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG013122.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG020322\
Data File : BG052294.D
Acq On : 4 Feb 2022 10:16
Operator : CG/JU
Sample : PB142414BL
Misc :
ALS Vial : 35 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK414

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG013122.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc