

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG020322\
 Data File : BG052297.D
 Acq On : 4 Feb 2022 12:16
 Operator : CG/JU
 Sample : N1328-18DL 10X
 Misc :
 ALS Vial : 38 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 C0HN7DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG013122.M
 Title : SVOA CALIBRATION

Signal : TIC: BG052297.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.541	3	9	17	rBV	489568	947992	98.57%	18.186%
2	4.028	90	92	95	rBV4	1447	1525	0.16%	0.029%
3	4.134	109	110	115	rBV2	1038	1130	0.12%	0.022%
4	4.345	143	146	149	rBV5	2136	2617	0.27%	0.050%
5	4.721	206	210	212	rVB2	1168	1480	0.15%	0.028%
6	4.898	232	240	252	rVV	552091	961785	100.00%	18.451%
7	4.997	256	257	263	rBV2	984	1404	0.15%	0.027%
8	5.456	332	335	339	rVB2	973	1213	0.13%	0.023%
9	5.514	339	345	346	rBV	1179	2113	0.22%	0.041%
10	6.707	545	548	551	rBV2	1187	1236	0.13%	0.024%
11	7.382	658	663	671	rBV4	2756	5833	0.61%	0.112%
12	7.541	684	690	697	rVB	12837	22751	2.37%	0.436%
13	7.764	723	728	734	rVB2	11240	18896	1.96%	0.363%
14	8.234	801	808	815	rVB	112994	196242	20.40%	3.765%
15	8.810	904	906	911	rBV2	635	1167	0.12%	0.022%
16	8.945	923	929	935	rVB3	8723	13991	1.45%	0.268%
17	9.409	1001	1008	1014	rBV3	15857	27900	2.90%	0.535%
18	10.137	1127	1132	1139	rVB4	10266	18315	1.90%	0.351%
19	10.690	1218	1226	1234	rBV	13771	24863	2.59%	0.477%
20	11.072	1284	1291	1299	rBV	153562	274344	28.52%	5.263%
21	11.201	1306	1313	1319	rBV2	12287	22339	2.32%	0.429%
22	14.267	1829	1835	1842	rBV	37728	53929	5.61%	1.035%
23	14.508	1873	1876	1878	rBV2	1276	1203	0.13%	0.023%
24	14.573	1880	1887	1893	rVB2	41864	65670	6.83%	1.260%
25	14.878	1931	1939	1946	rBV	265735	400507	41.64%	7.683%
26	15.865	2102	2107	2114	rVB	55925	86307	8.97%	1.656%
27	15.983	2122	2127	2134	rBV4	4805	7529	0.78%	0.144%
28	17.410	2364	2370	2377	rBV3	1362	3110	0.32%	0.060%
29	17.627	2400	2407	2414	rBV	342108	512839	53.32%	9.838%
30	17.721	2418	2423	2431	rVV	65640	103871	10.80%	1.993%
31	18.467	2548	2550	2554	rBV2	897	1277	0.13%	0.024%
32	19.096	2655	2657	2660	rVB3	1166	1084	0.11%	0.021%
33	19.337	2692	2698	2701	rBV3	1009	1557	0.16%	0.030%
34	19.431	2713	2714	2718	rBV2	1089	1409	0.15%	0.027%
35	19.478	2720	2722	2726	rBV3	1001	1316	0.14%	0.025%
36	19.619	2744	2746	2749	rBV2	1311	1913	0.20%	0.037%

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG020322\
 Data File : BG052297.D
 Acq On : 4 Feb 2022 12:16
 Operator : CG/JU
 Sample : N1328-18DL 10X
 Misc :
 ALS Vial : 38 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 C0HN7DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG013122.M
 Title : SVOA CALIBRATION

37	19.642	2749	2750	2755	rVB3	1615	1511	0.16%	0.029%
38	20.006	2806	2812	2818	rBV	87620	125602	13.06%	2.410%
39	20.318	2862	2865	2867	rBV2	1286	1637	0.17%	0.031%
40	20.547	2902	2904	2906	rBV2	1717	1296	0.13%	0.025%
41	20.570	2906	2908	2909	rVV2	2781	1543	0.16%	0.030%
42	20.612	2913	2915	2918	rBV4	1239	1091	0.11%	0.021%
43	21.058	2989	2991	2992	rBV	2262	1381	0.14%	0.026%
44	21.945	3135	3142	3150	rVB2	322351	564497	58.69%	10.829%
45	22.344	3208	3210	3211	rBV2	2366	1418	0.15%	0.027%
46	23.096	3336	3338	3341	rBV3	2604	2872	0.30%	0.055%
47	25.176	3684	3692	3701	rBV2	36928	105572	10.98%	2.025%
48	25.423	3722	3734	3745	rBV3	194505	594468	61.81%	11.404%
49	25.893	3812	3814	3817	rBV3	2335	1843	0.19%	0.035%
50	26.656	3942	3944	3945	rBV2	4665	3906	0.41%	0.075%
51	26.674	3945	3947	3950	rVV3	5884	7617	0.79%	0.146%
52	27.438	4075	4077	4078	rBV2	2763	1663	0.17%	0.032%
53	27.908	4155	4157	4159	rBV2	2342	2115	0.22%	0.041%




Sum of corrected areas: 5212689

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG020322\
Data File : BG052297.D
Acq On : 4 Feb 2022 12:16
Operator : CG/JU
Sample : N1328-18DL 10X
Misc :
ALS Vial : 38 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
C0HN7DL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG013122.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

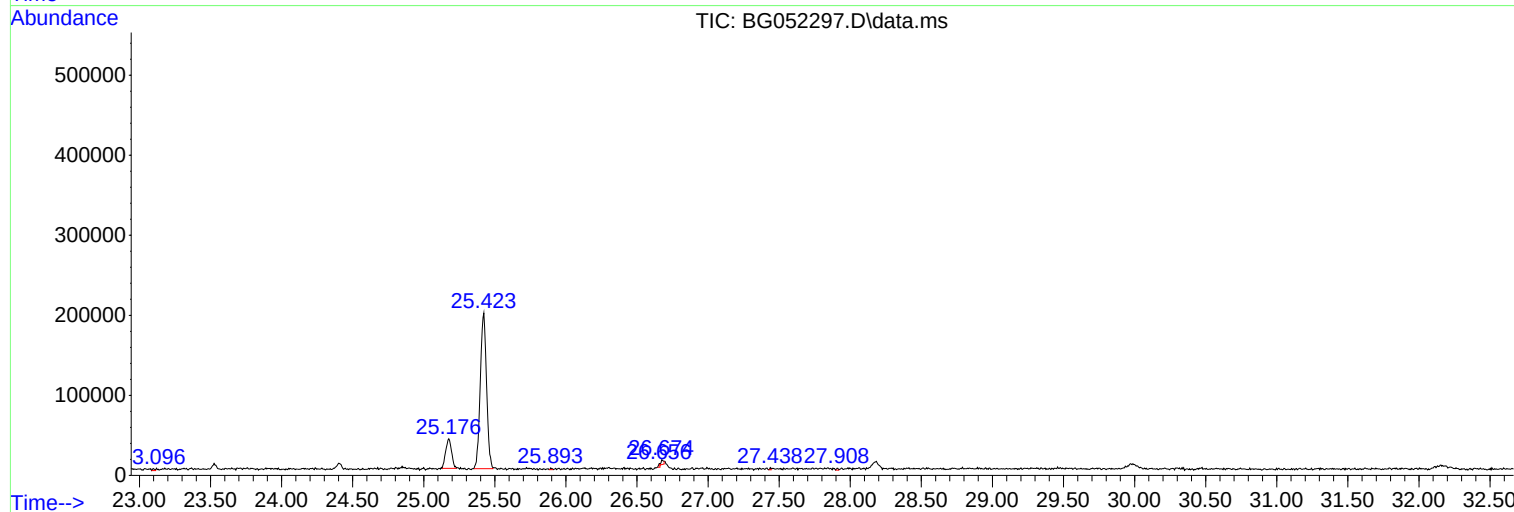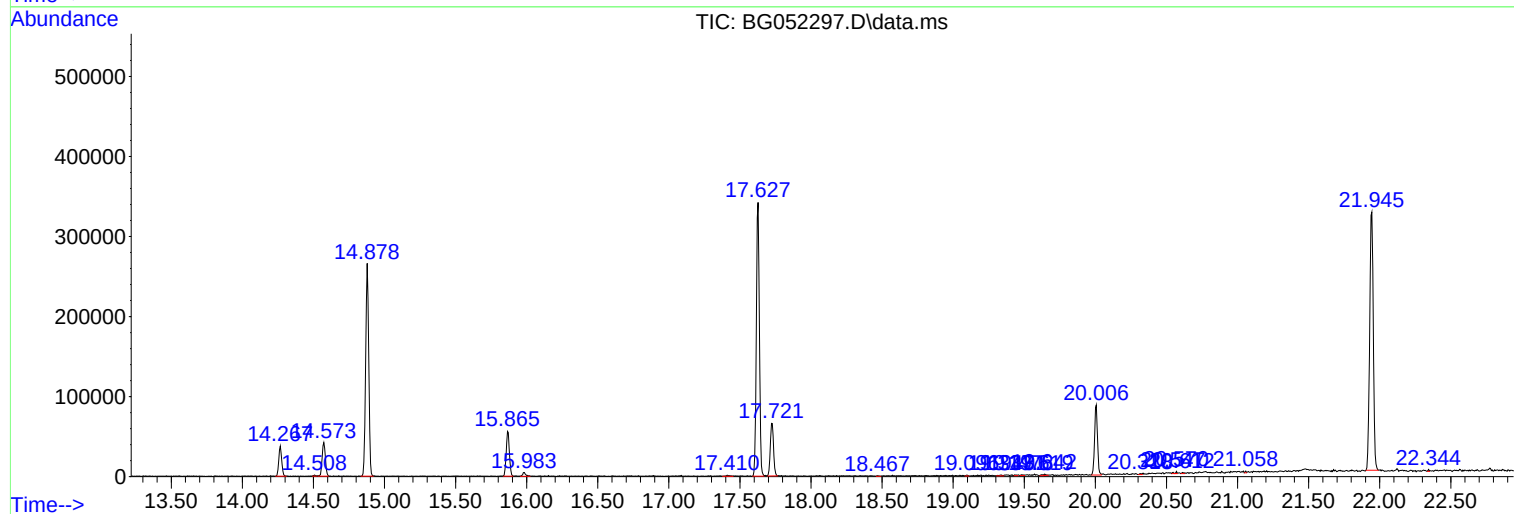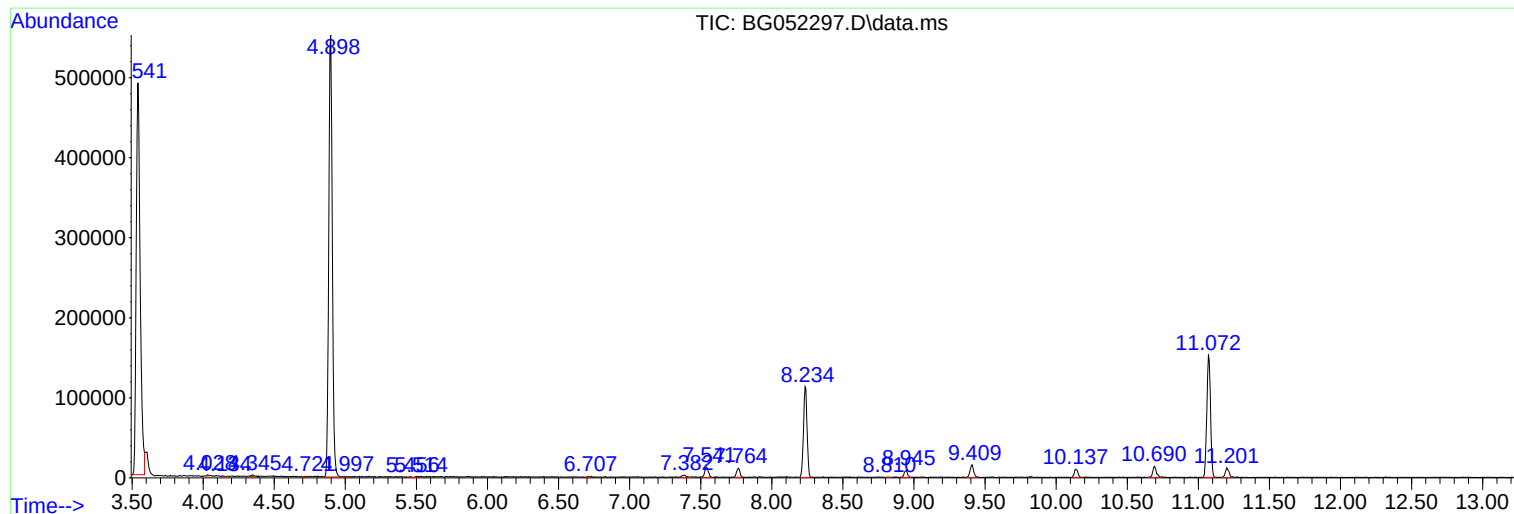

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG020322\
Data File : BG052297.D
Acq On : 4 Feb 2022 12:16
Operator : CG/JU
Sample : N1328-18DL 10X
Misc :
ALS Vial : 38 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
C0HN7DL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG013122.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG020322\
Data File : BG052297.D
Acq On : 4 Feb 2022 12:16
Operator : CG/JU
Sample : N1328-18DL 10X
Misc :
ALS Vial : 38 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
C0HN7DL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG013122.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
