
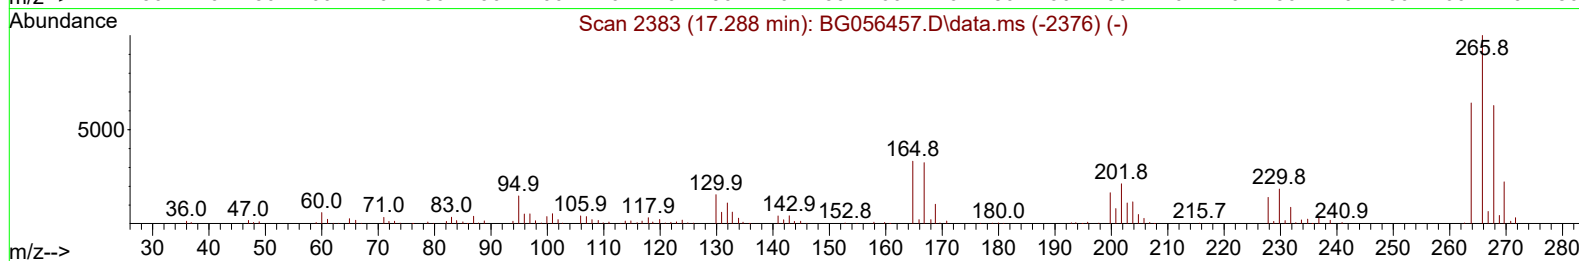
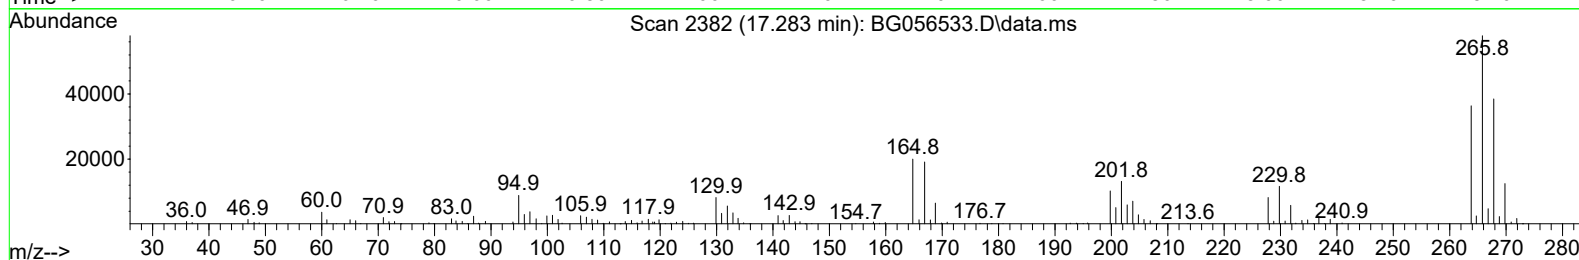


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG020323\
Data File : BG056533.D
Acq On : 3 Feb 2023 10:55
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Feb 04 04:31:10 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG012723.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Feb 01 01:15:52 2023
Response via : Initial Calibration

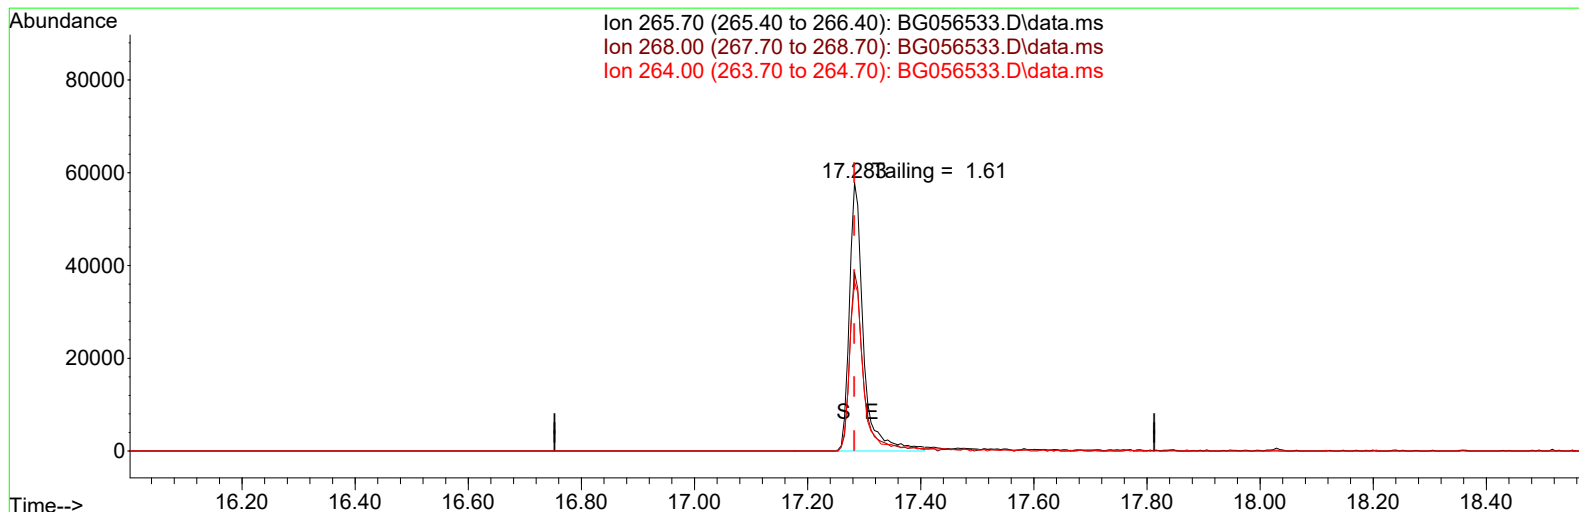

TIC: BG056533.D\data.ms

(70) Pentachlorophenol (C)




17.283min (+ 0.000) 19595.48 ng

response 101985

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.80	66.46
264.00	64.20	67.27
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG020323\
Data File : BG056533.D
Acq On : 3 Feb 2023 10:55
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Feb 04 04:31:10 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG012723.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Feb 01 01:15:52 2023
Response via : Initial Calibration

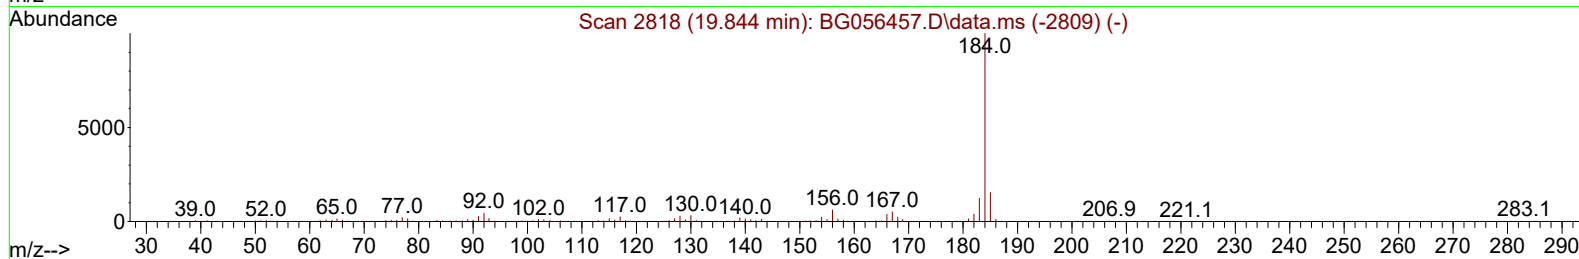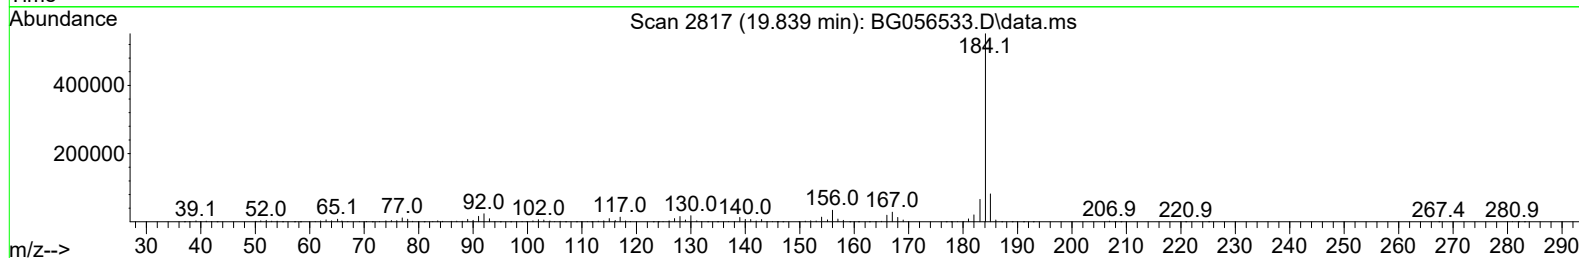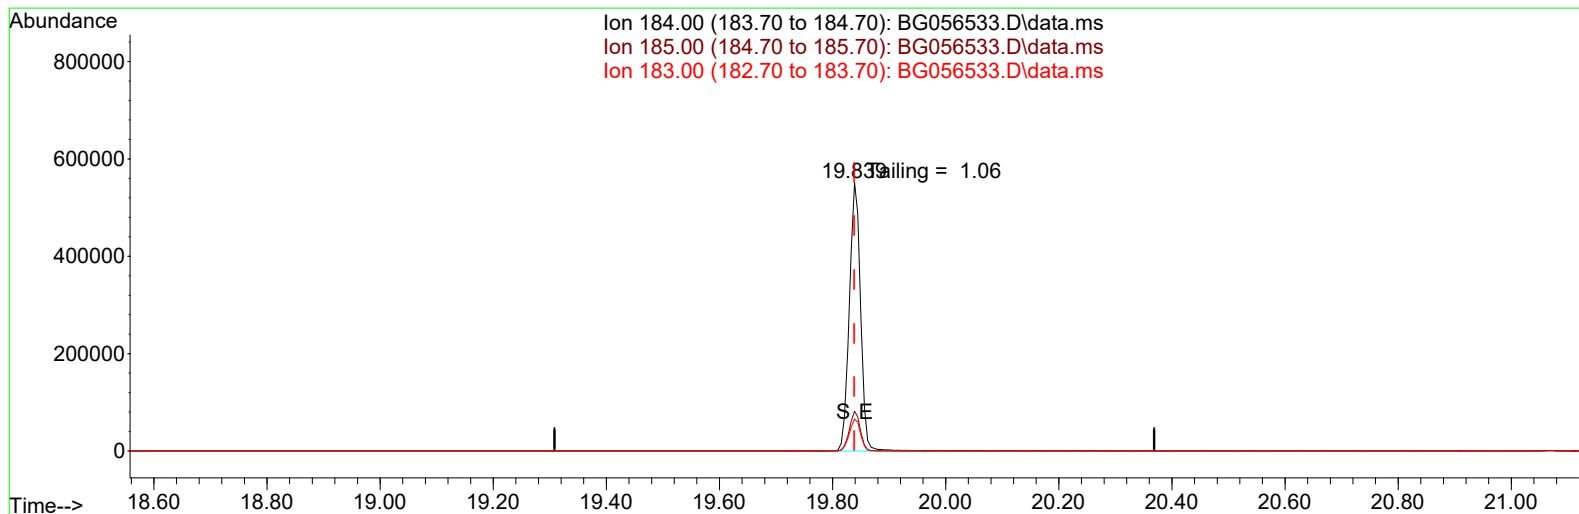

TIC: BG056533.D\data.ms

(77) Benzidine**19.839min (+ 0.000) 477744.32 ng****response 762772**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.40	14.80
183.00	12.30	11.91
0.00	0.00	0.00