
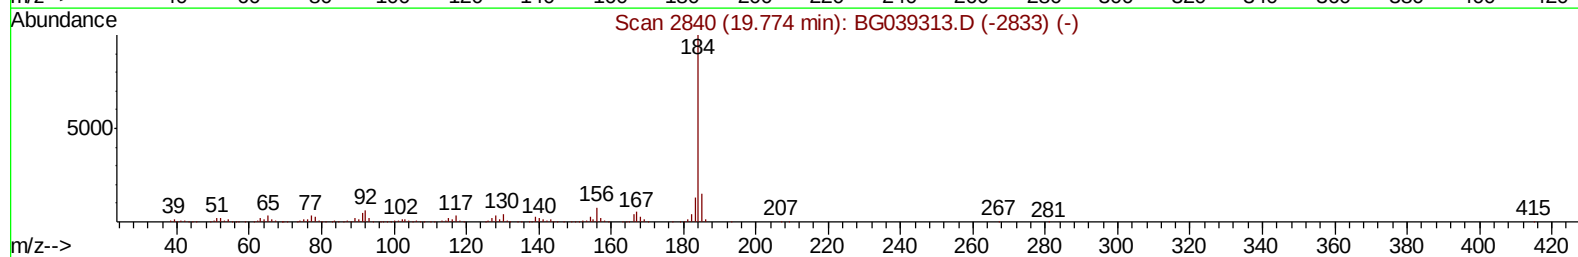
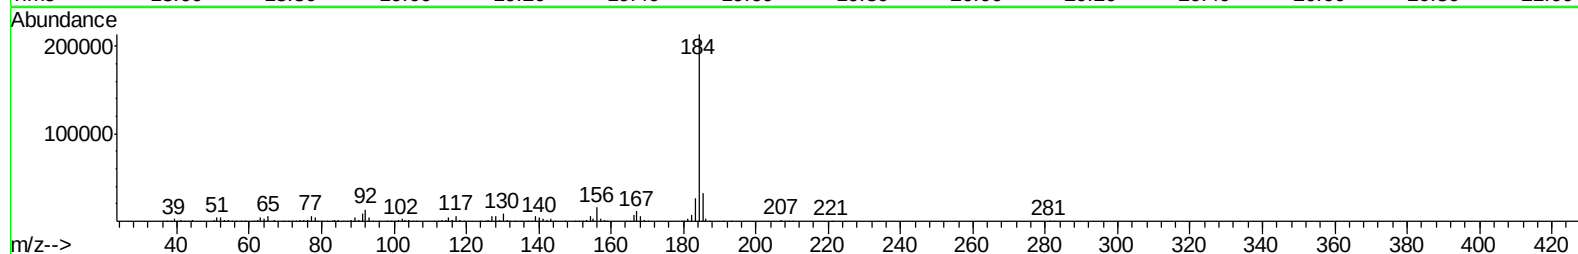


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG020519\
 Data File : BG039357.D
 Acq On : 5 Feb 2019 15:18
 Operator : JU/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Feb 05 23:43:50 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG012919.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Jan 29 15:41:51 2019
 Response via : Initial Calibration

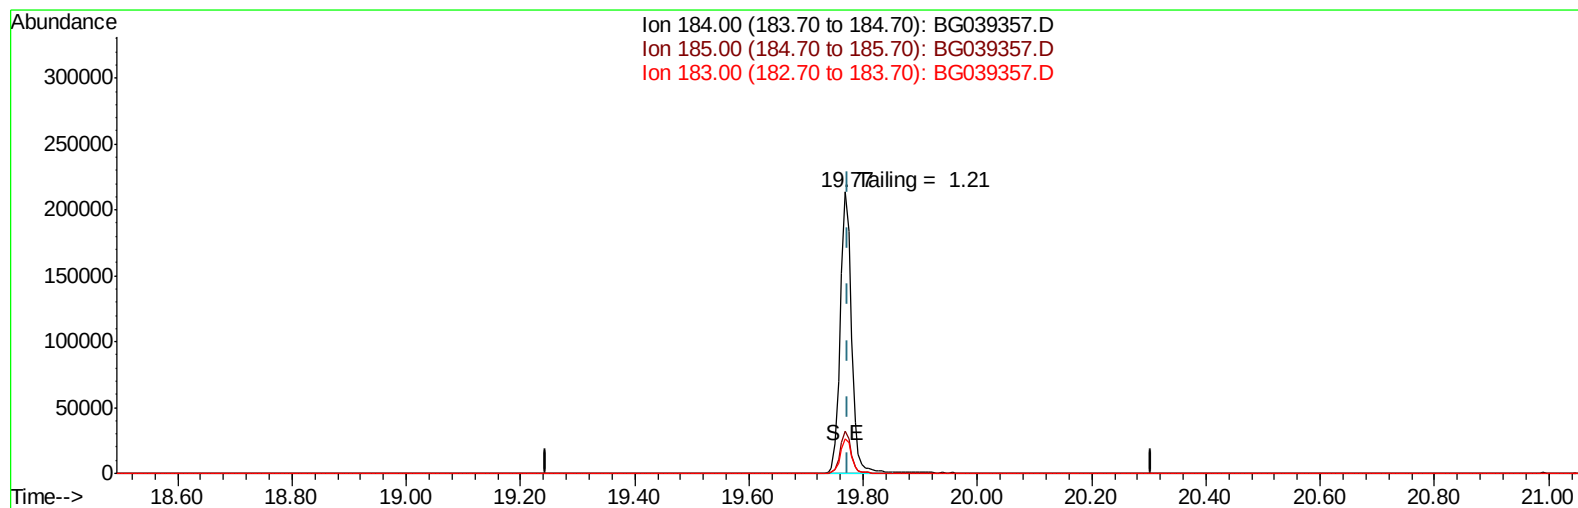

TIC: BG039357.D

(77) Benzidine




19.768min (-0.006) 0.00ng

response 291803

Ion	Exp%	Act%
184.00	100	100
185.00	15.20	14.82
183.00	13.20	12.21
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG020519\
Data File : BG039357.D
Acq On : 5 Feb 2019 15:18
Operator : JU/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Feb 05 23:43:50 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG012919.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jan 29 15:41:51 2019
Response via : Initial Calibration

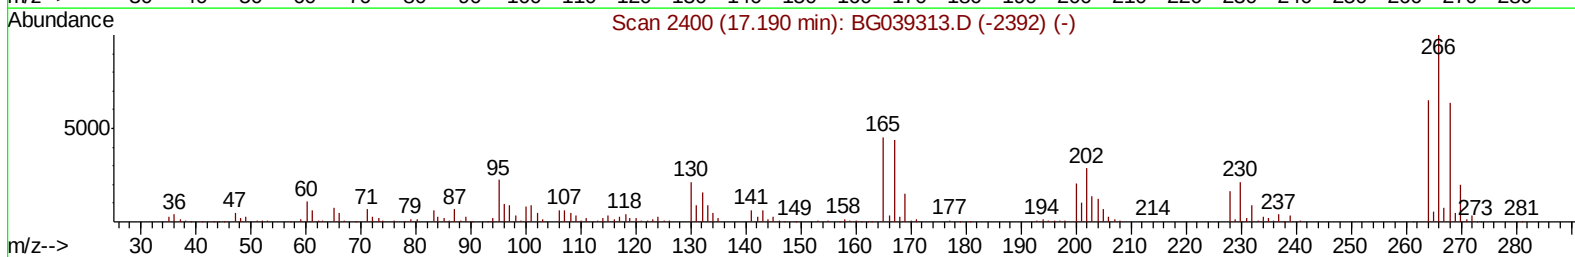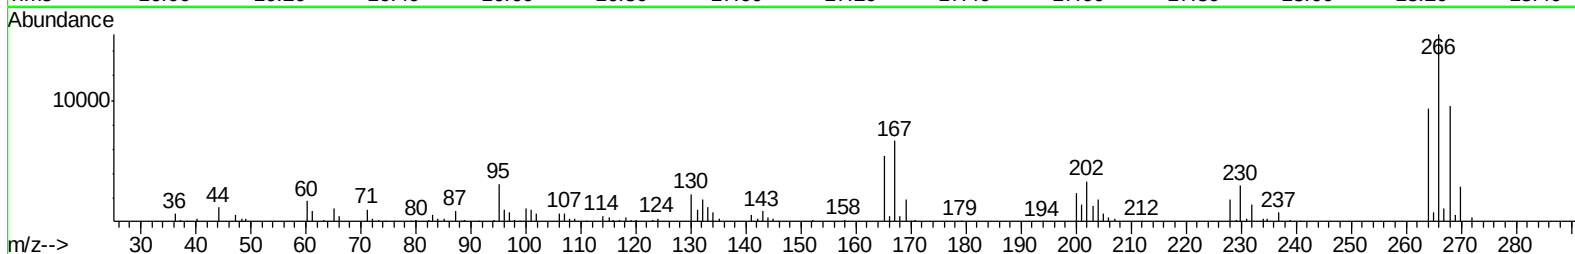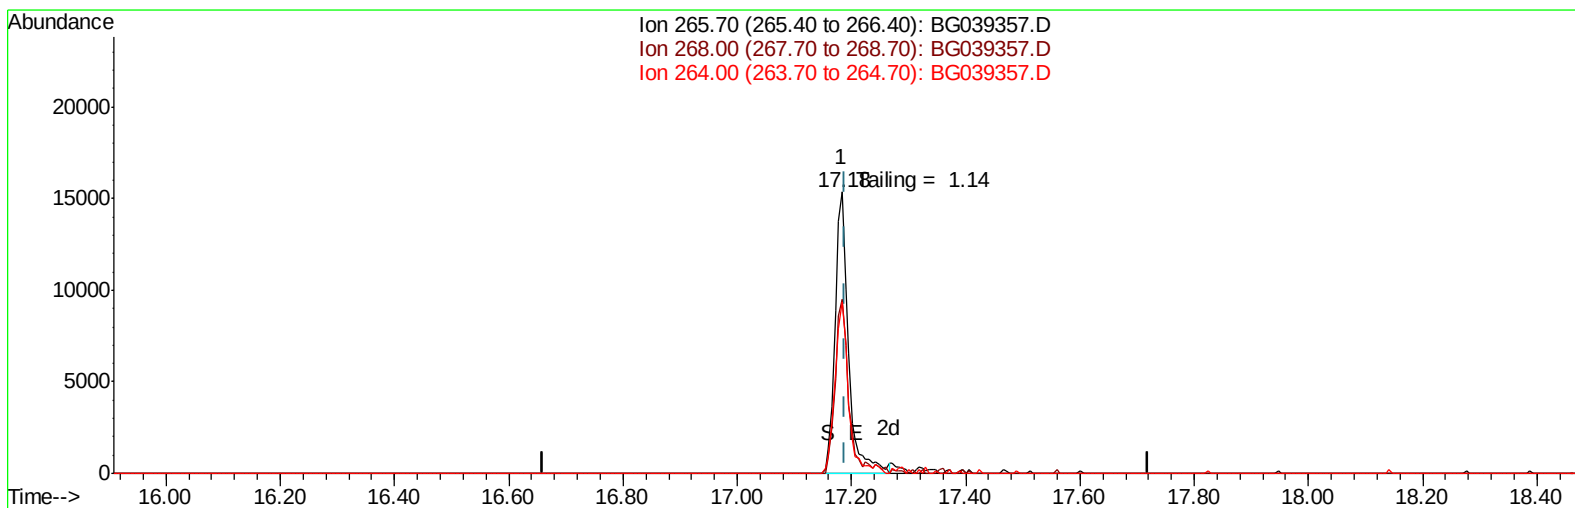

TIC: BG039357.D

(70) Pentachlorophenol (C)

17.183min (-0.006) 0.00ng

response 24796

Ion	Exp%	Act%
265.70	100	100
268.00	63.90	61.83
264.00	65.10	61.00
0.00	0.00	0.00