


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG020519\
 Data File : BG039357.D
 Acq On : 5 Feb 2019 15:18
 Operator : JU/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG012919.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Jan 29 15:41:51 2019

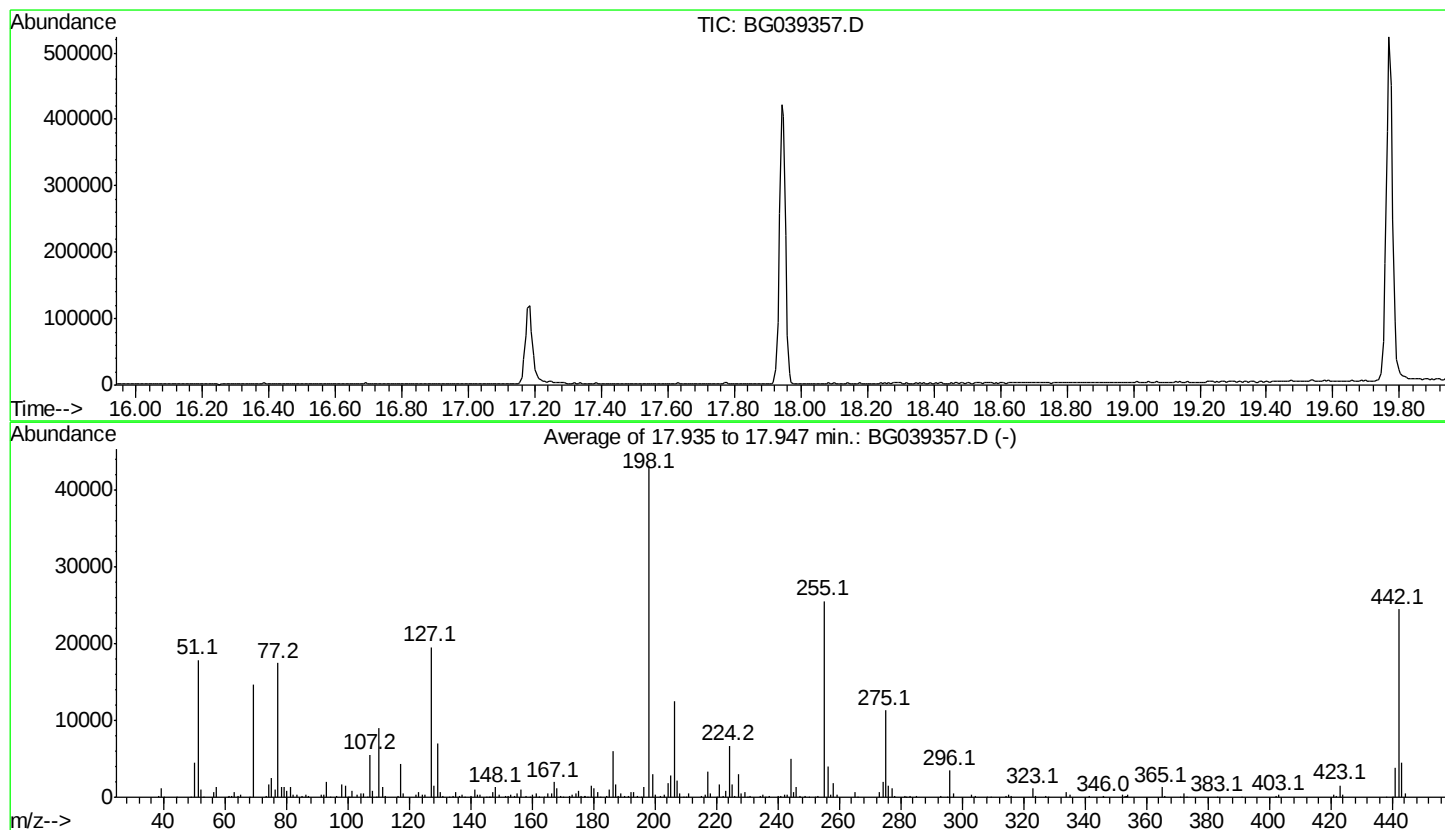

AutoFind: Scans 2527, 2528, 2529; Background Corrected with Scan 2521

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	41.4	17875	PASS
68	69	0.00	2	0.5	68	PASS
69	198	0.00	100	34.1	14707	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	45.2	19507	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	43160	PASS
199	198	5	9	6.8	2935	PASS
275	198	10	60	26.1	11276	PASS
365	198	1	100	3.0	1311	PASS
441	198	0.01	100	8.9	3843	PASS
442	198	50	100	56.7	24457	PASS
443	442	15	24	18.2	4445	PASS