

Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG020619\  
 Data File : BG039375.D  
 Acq On : 6 Feb 2019 17:56  
 Operator : JU/SJ  
 Sample : PB116873BL  
 Misc :  
 ALS Vial : 10 Sample Multiplier: 1

Instrument :  
 BNA\_G  
 ClientSampleId :  
 PB116873BL

Quant Time: Feb 07 01:24:44 2019  
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG012919.M  
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
 QLast Update : Tue Jan 29 15:41:51 2019  
 Response via : Initial Calibration

| Internal Standards          | R.T.  | QIon | Response | Conc   | Units | Dev(Min) |
|-----------------------------|-------|------|----------|--------|-------|----------|
| 1) 1,4-Dichlorobenzene-d4   | 8.18  | 152  | 54546    | 20.00  | ng    | 0.00     |
| 21) Naphthalene-d8          | 11.00 | 136  | 231808   | 20.00  | ng    | -0.01    |
| 39) Acenaphthene-d10        | 14.80 | 164  | 147704   | 20.00  | ng    | -0.01    |
| 64) Phenanthrene-d10        | 17.54 | 188  | 370901   | 20.00  | ng    | -0.01    |
| 76) Chrysene-d12            | 21.84 | 240  | 416947   | 20.00  | ng    | -0.01    |
| 87) Perylene-d12            | 25.22 | 264  | 414705   | 20.00  | ng    | -0.02    |
| System Monitoring Compounds |       |      |          |        |       |          |
| 5) 2-Fluorophenol           | 5.72  | 112  | 508391   | 159.52 | ng    | 0.00     |
| 7) Phenol-d6                | 7.31  | 99   | 710358   | 151.42 | ng    | 0.00     |
| 23) Nitrobenzene-d5         | 9.35  | 82   | 411150   | 110.80 | ng    | -0.01    |
| 42) 2,4,6-Tribromophenol    | 16.28 | 330  | 269829   | 169.65 | ng    | 0.00     |
| 45) 2-Fluorobiphenyl        | 13.43 | 172  | 1024444  | 99.50  | ng    | 0.00     |
| 79) Terphenyl-d14           | 20.14 | 244  | 1690466  | 85.82  | ng    | -0.01    |


Target Compounds Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG020619\  
Data File : BG039375.D  
Acq On : 6 Feb 2019 17:56  
Operator : JU/SJ  
Sample : PB116873BL  
Misc :  
ALS Vial : 10 Sample Multiplier: 1

Instrument :  
BNA\_G  
ClientSampleId :  
PB116873BL

Quant Time: Feb 07 01:24:44 2019  
Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG012919.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Tue Jan 29 15:41:51 2019  
Response via : Initial Calibration

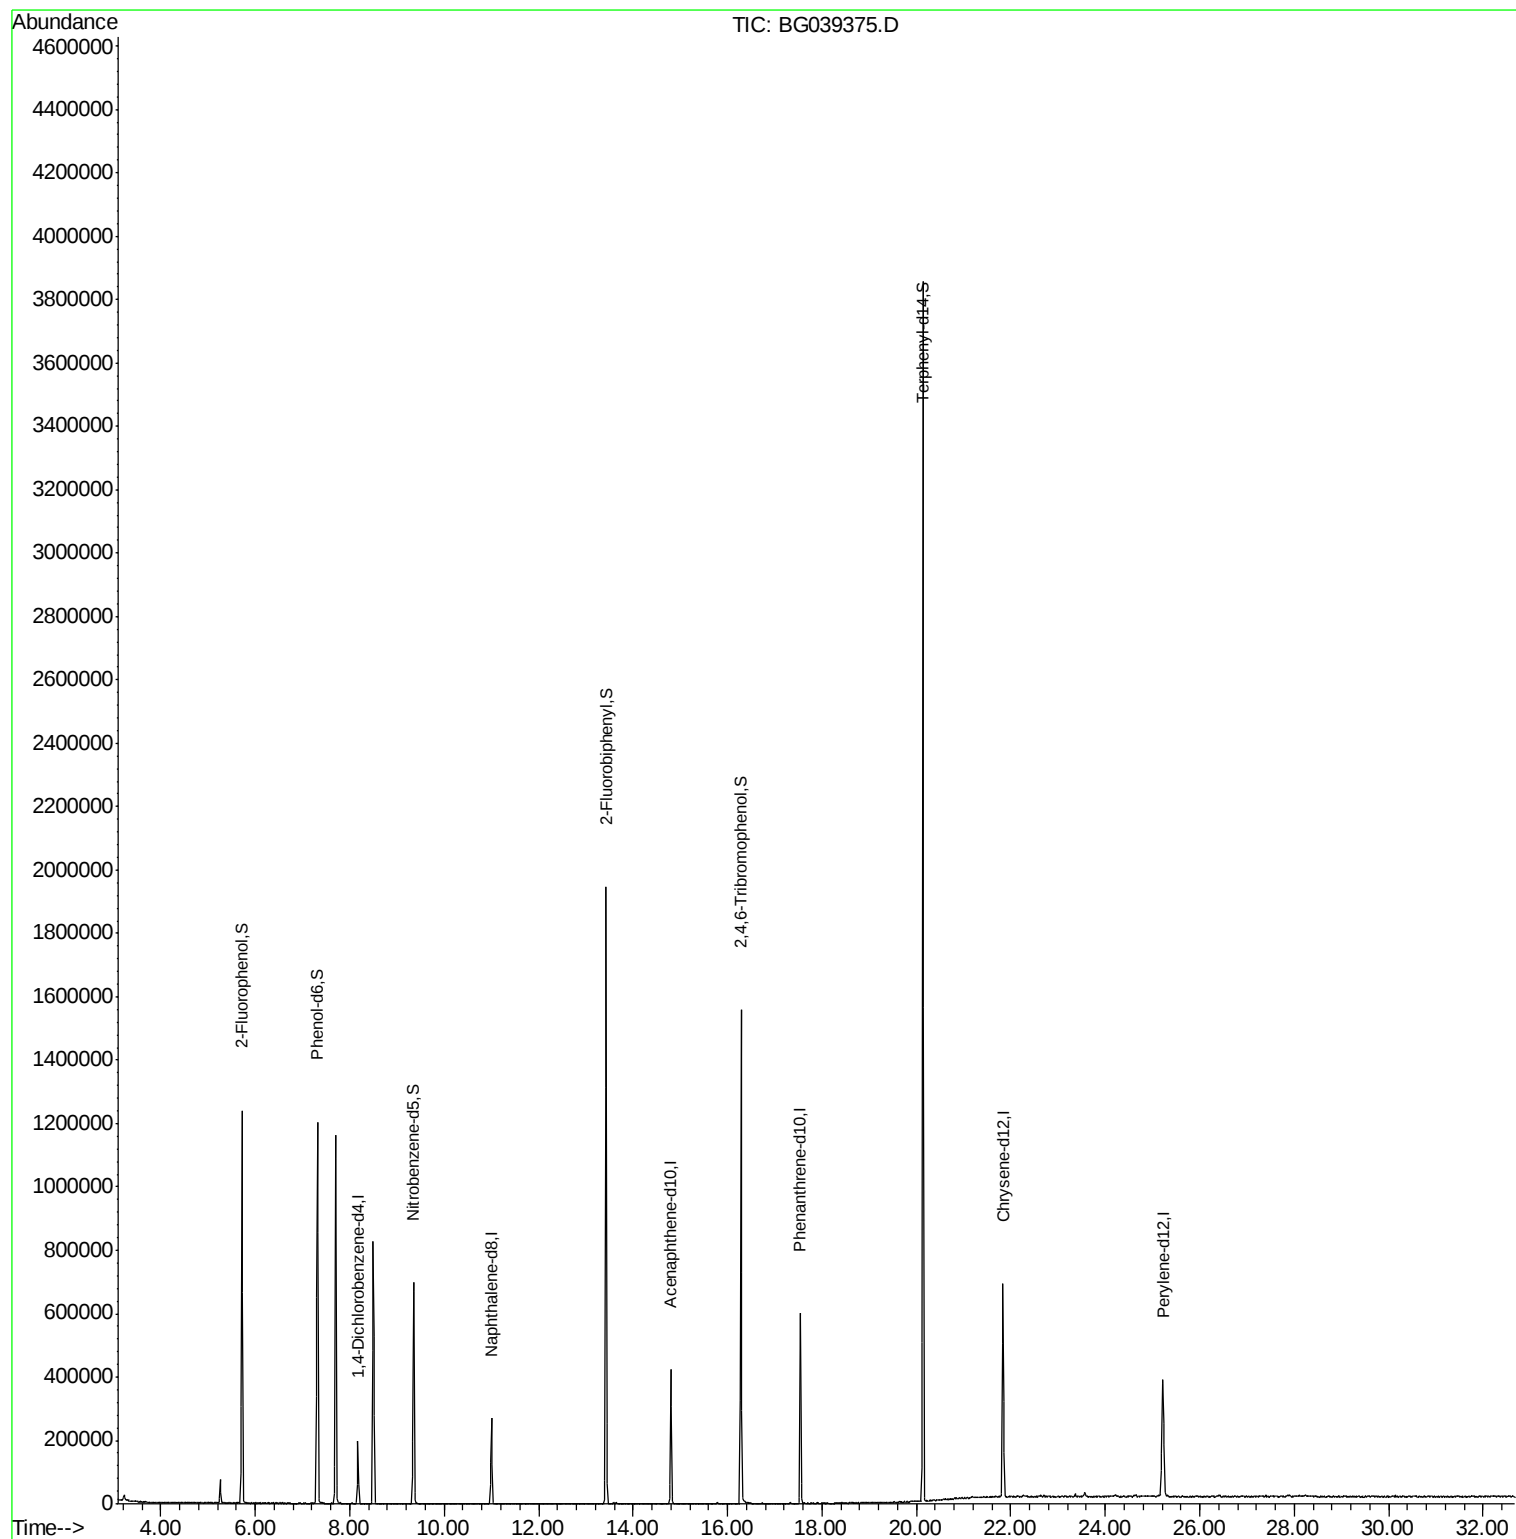




#1




1,4-Dichlorobenzene-d4  
Concen: 20.000 ng  
RT: 8.18 min Scan# 866  
Delta R.T. -0.01 min  
Lab File: BG039375.D  
Acq: 6 Feb 2019 17:56

Instrument :  
BNA\_G  
ClientSampleId :  
PB116873BL

Tot Ion:152 Resp: 54546  
Ion Ratio Lower Upper  
152 100  
150 157.1 123.7 185.5  
115 60.3 45.9 68.9

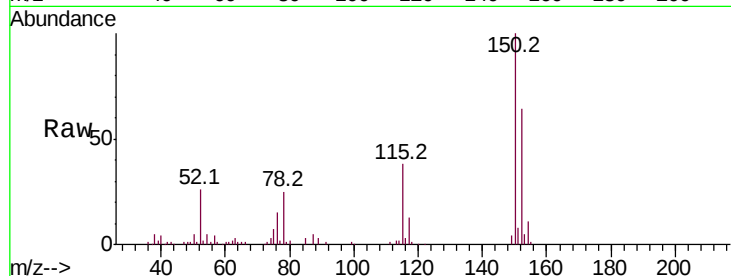


Abundance Ion 152.00 (151.70 to 152.70): E  
Ion 150.00 (149.70 to 150.70): E  
Ion 115.00 (114.70 to 115.70): E

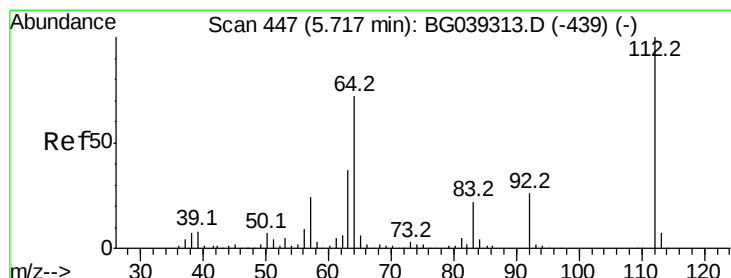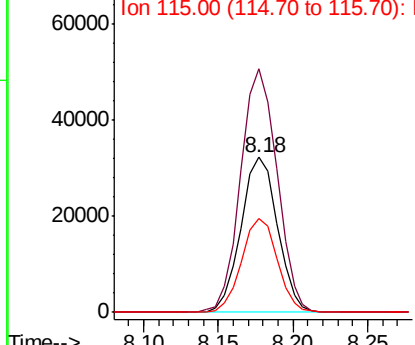



#5

2-Fluorophenol  
Concen: 159.520 ng  
RT: 5.72 min Scan# 447  
Delta R.T. -0.00 min  
Lab File: BG039375.D  
Acq: 6 Feb 2019 17:56

Tgt Ion:112 Resp: 508391  
Ion Ratio Lower Upper  
112 100  
64 70.2 57.8 86.8  
63 36.8 29.8 44.6

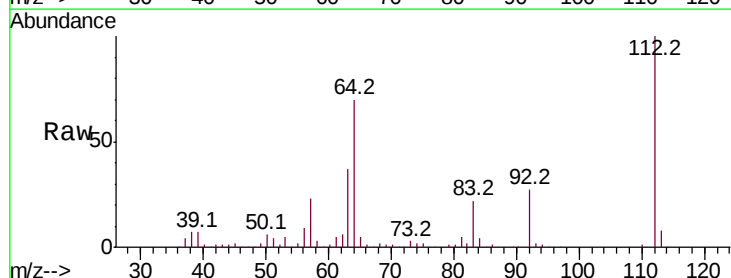

Abundance Ion 112.00 (111.70 to 112.70): E  
Ion 64.00 (63.70 to 64.70): BGC  
Ion 63.00 (62.70 to 63.70): BGC

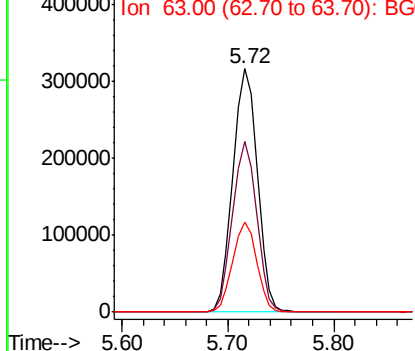



#7

Phenol-d6

Concen: 151.424 ng

RT: 7.31 min Scan# 719

Delta R.T. -0.01 min

Lab File: BG039375.D

Acq: 6 Feb 2019 17:56

Instrument :

BNA\_G

ClientSampleId :

PB116873BL


Tot Ion: 99 Resp: 710358

Ion Ratio Lower Upper




99 100

42 20.4 18.2 27.2

71 36.5 28.0 42.0

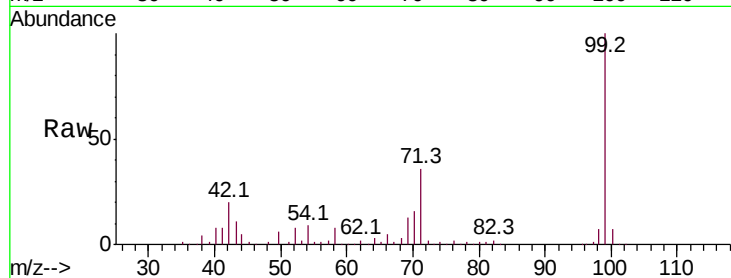

Abundance Ion 99.00 (98.70 to 99.70): BGC  
Ion 42.00 (41.70 to 42.70): BGC  
Ion 71.00 (70.70 to 71.70): BGC

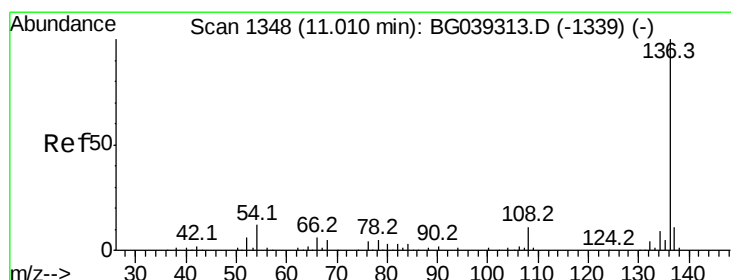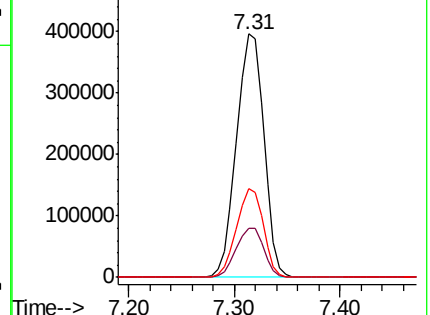

#21

Naphthalene-d8

Concen: 20.000 ng

RT: 11.00 min Scan# 1346

Delta R.T. -0.01 min

Lab File: BG039375.D

Acq: 6 Feb 2019 17:56

Tgt Ion: 136 Resp: 231808


Ion Ratio Lower Upper

136 100



137 11.4 9.1 13.7


54 10.5 9.4 14.2

68 5.7 4.2 6.4

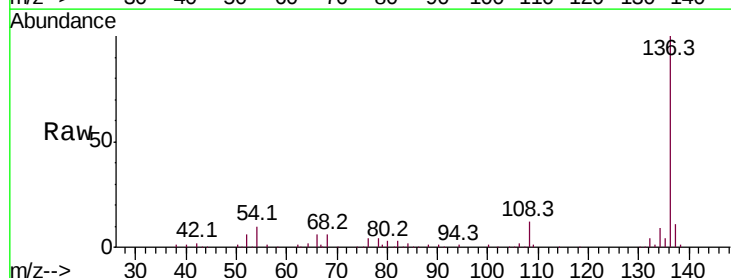

Abundance Ion 136.00 (135.70 to 136.70): BGC  
Ion 137.00 (136.70 to 137.70): BGC  
Ion 54.00 (53.70 to 54.70): BGC  
Ion 68.00 (67.70 to 68.70): BGC



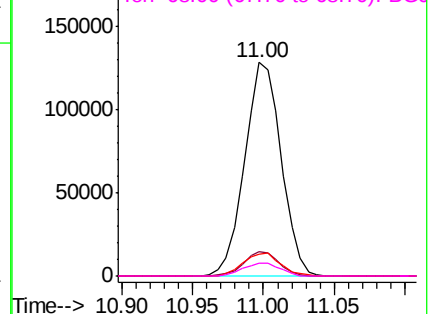





#23  
Nitrobenzene-d5  
Concen: 110.804 ng  
RT: 9.35 min Scan# 1066  
Delta R.T. -0.01 min  
Lab File: BG039375.D  
Acq: 6 Feb 2019 17:56




Instrument :  
BNA\_G  
ClientSampleId :  
PB116873BL


Tot Ion: 82 Resp: 411150  
Ion Ratio Lower Upper  
82 100  
128 42.4 31.3 46.9  
54 57.7 50.9 76.3

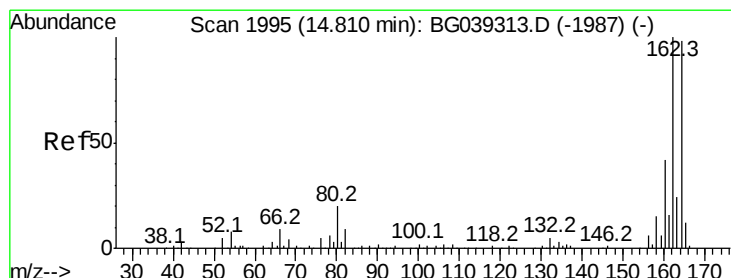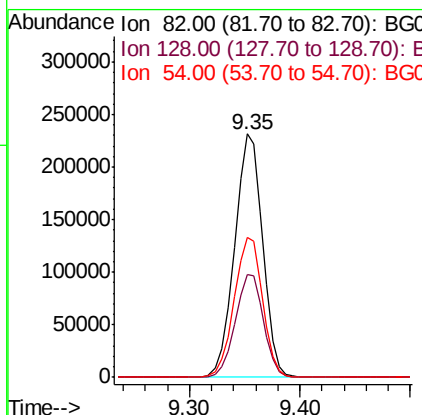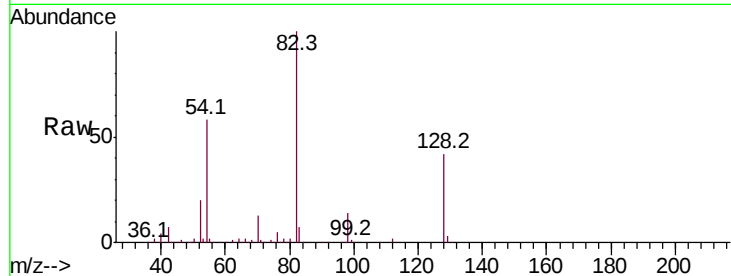

#39  
Acenaphthene-d10  
Concen: 20.000 ng  
RT: 14.80 min Scan# 1993  
Delta R.T. -0.01 min  
Lab File: BG039375.D  
Acq: 6 Feb 2019 17:56

Tgt Ion: 164 Resp: 147704  
Ion Ratio Lower Upper  
164 100  
162 104.2 81.6 122.4  
160 43.9 34.2 51.2

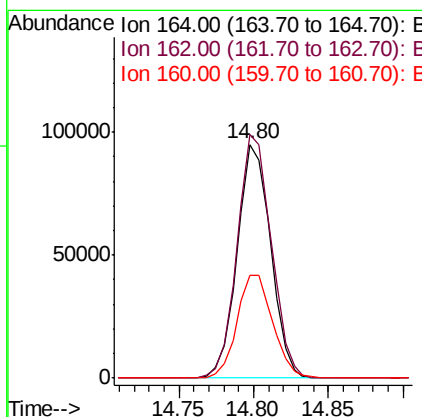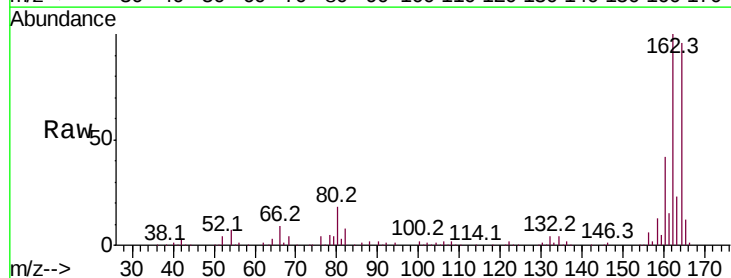



#42

2,4,6-Tribromophenol

Concen: 169.648 ng

RT: 16.28 min Scan# 2246

Delta R.T. -0.01 min

Lab File: BG039375.D

Acq: 6 Feb 2019 17:56

Instrument :

BNA\_G

ClientSampleId :

PB116873BL


Tot Ion:330 Resp: 269829

Ion Ratio Lower Upper

330 100

332 95.3 75.7 113.5




141 39.6 35.6 53.4

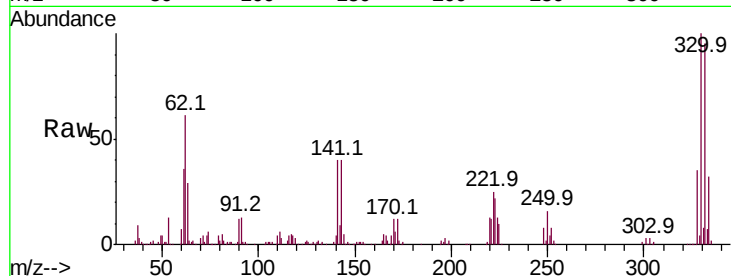

Abundance Ion 329.80 (329.50 to 330.50): E

Ion 331.80 (331.50 to 332.50): E

Ion 141.00 (140.70 to 141.70): E

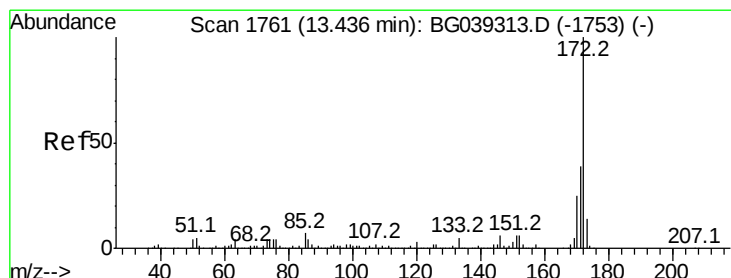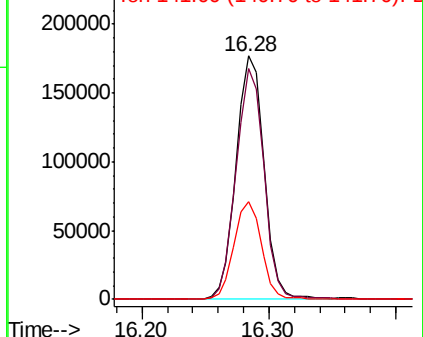

#45

2-Fluorobiphenyl

Concen: 99.497 ng

RT: 13.43 min Scan# 1760

Delta R.T. -0.01 min

Lab File: BG039375.D

Acq: 6 Feb 2019 17:56


Tgt Ion:172 Resp: 1024444

Ion Ratio Lower Upper

172 100

171 38.6 30.8 46.2



170 25.3 20.2 30.4

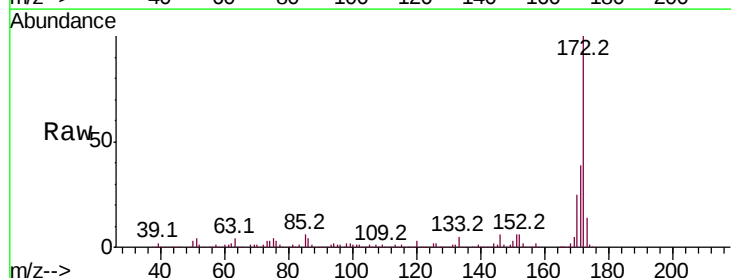


Abundance Ion 172.00 (171.70 to 172.70): E

Ion 171.00 (170.70 to 171.70): E

Ion 170.00 (169.70 to 170.70): E

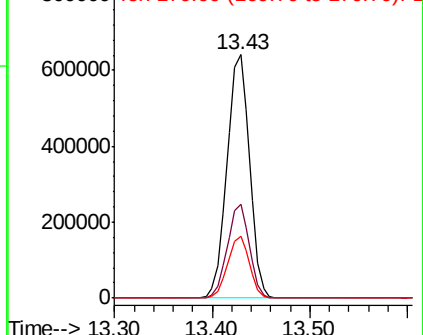

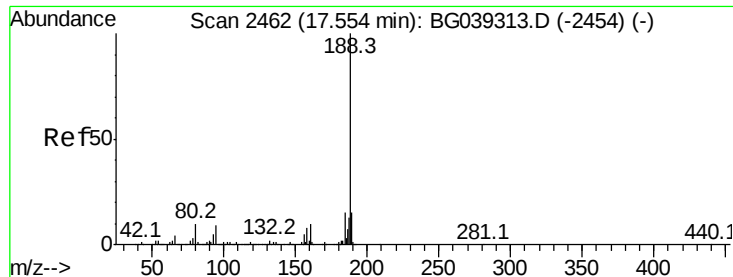

#64

Phenanthrene-d10

Concen: 20.000 ng

RT: 17.54 min Scan# 2460

Delta R.T. -0.01 min

Lab File: BG039375.D

Acq: 6 Feb 2019 17:56

Instrument :

BNA\_G

ClientSampleId :

PB116873BL


Tot Ion:188 Resp: 370901

Ion Ratio Lower Upper

188 100

94 8.9 6.9 10.3




80 9.1 8.1 12.1

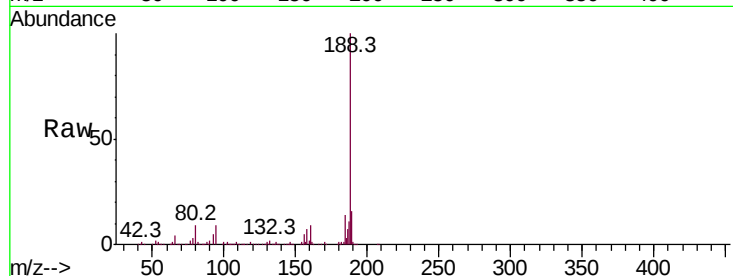

Abundance Ion 188.00 (187.70 to 188.70): E

Ion 94.00 (93.70 to 94.70): BGC

Ion 80.00 (79.70 to 80.70): BGC

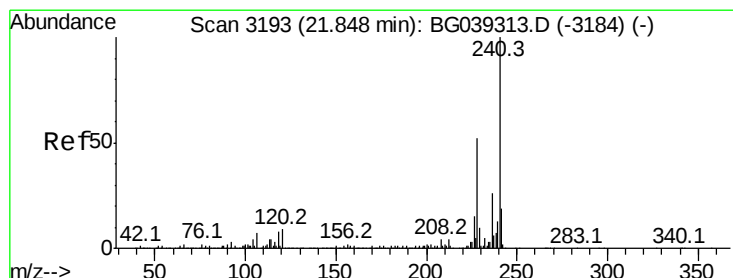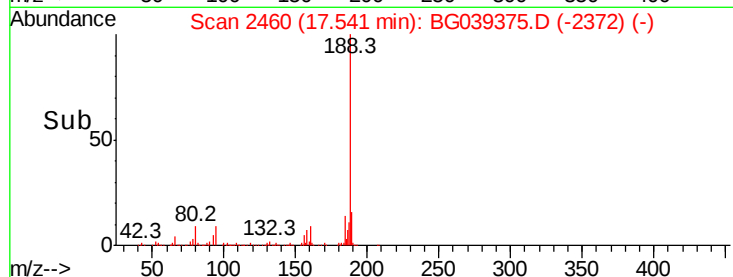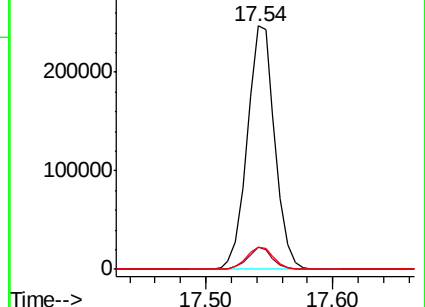

#76

Chrysene-d12

Concen: 20.000 ng

RT: 21.84 min Scan# 3191

Delta R.T. -0.01 min

Lab File: BG039375.D

Acq: 6 Feb 2019 17:56


Tgt Ion:240 Resp: 416947

Ion Ratio Lower Upper

240 100

120 8.3 7.0 10.6



236 25.5 21.0 31.4

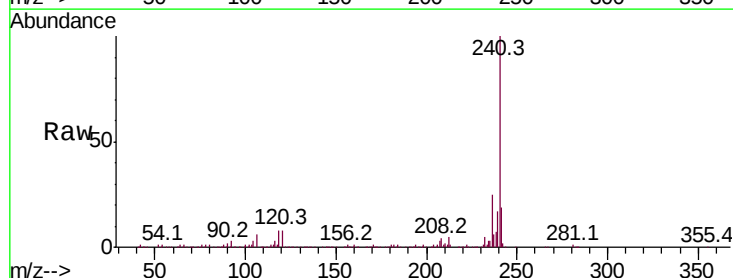


Abundance Ion 240.00 (239.70 to 240.70): E

Ion 120.00 (119.70 to 120.70): E

Ion 236.00 (235.70 to 236.70): E

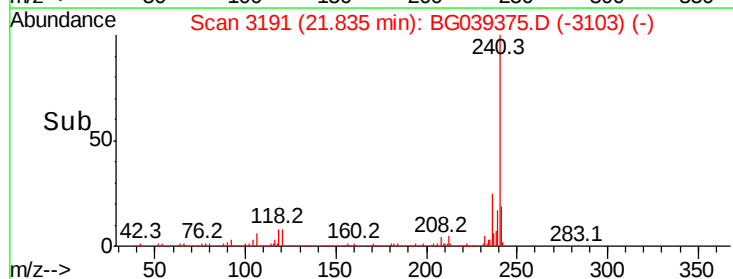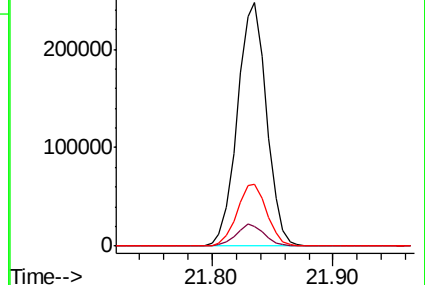




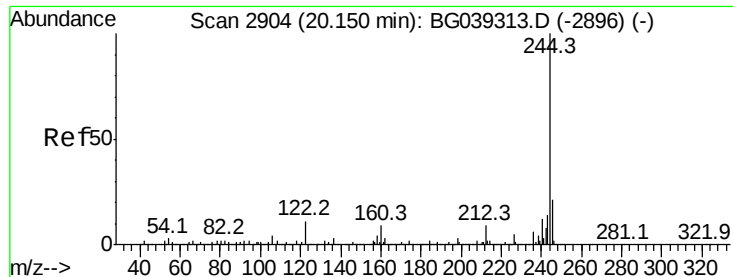


#79  
 Terphenyl-d14  
 Concen: 85.819 ng  
 RT: 20.14 min Scan# 2902  
 Delta R.T. -0.01 min  
 Lab File: BG039375.D  
 Acq: 6 Feb 2019 17:56

Instrument :  
 BNA\_G  
 ClientSampleId :  
 PB116873BL

Tot Ion:244 Resp: 1690466  

| Ion | Ratio | Lower | Upper |
|-----|-------|-------|-------|
| 244 | 100   |       |       |
| 212 | 9.4   | 7.3   | 10.9  |
| 122 | 10.1  | 8.4   | 12.6  |

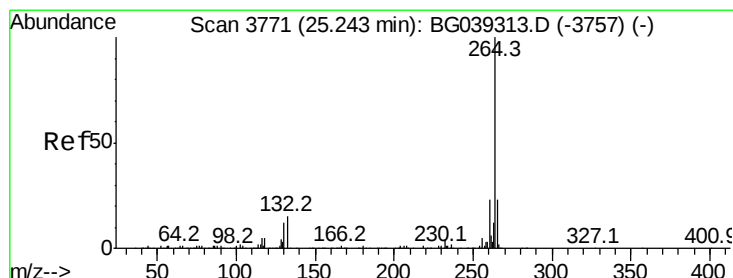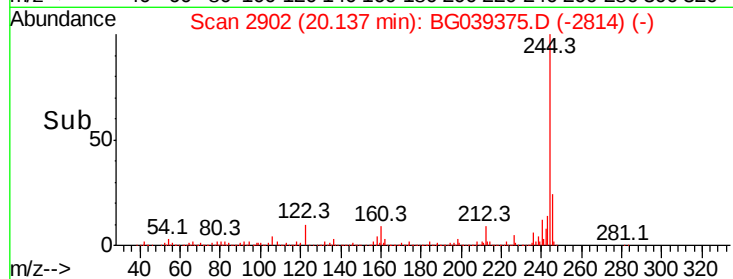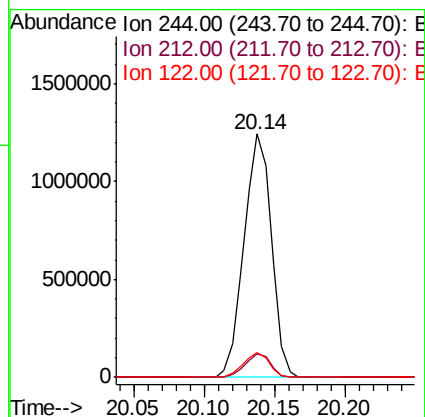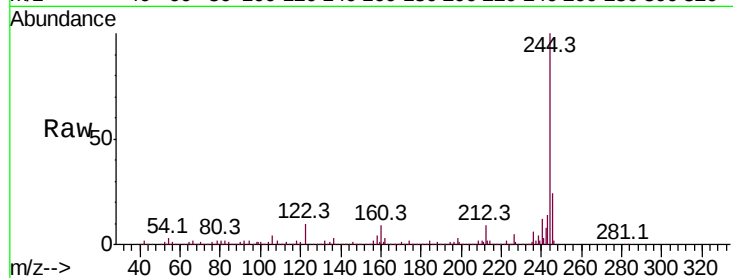

#87  
 Perylene-d12  
 Concen: 20.000 ng  
 RT: 25.22 min Scan# 3767  
 Delta R.T. -0.02 min  
 Lab File: BG039375.D  
 Acq: 6 Feb 2019 17:56

Tgt Ion:264 Resp: 414705  

| Ion | Ratio | Lower | Upper |
|-----|-------|-------|-------|
| 264 | 100   |       |       |
| 260 | 22.8  | 18.2  | 27.4  |
| 265 | 21.3  | 18.5  | 27.7  |

