
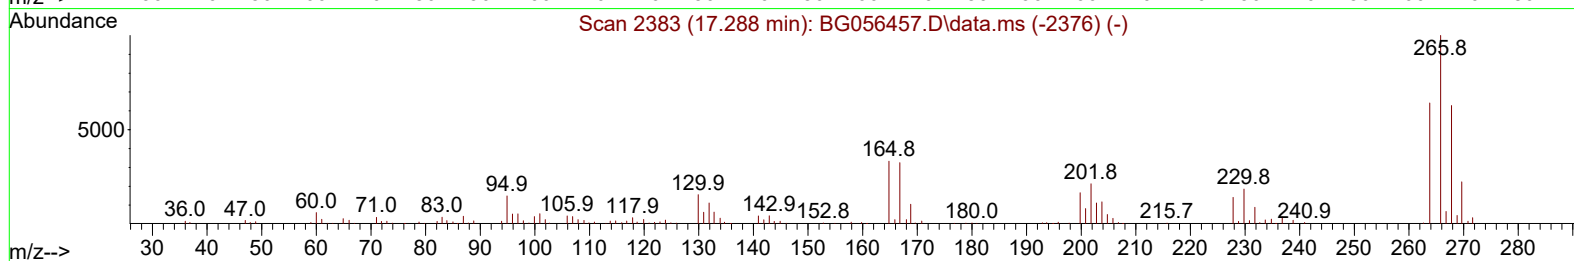
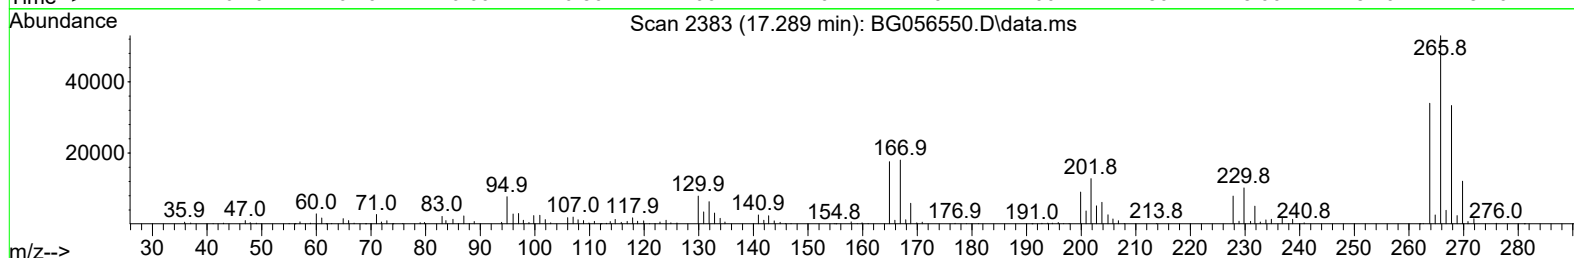


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG020623\
Data File : BG056550.D
Acq On : 6 Feb 2023 10:25
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Feb 07 05:37:53 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG012723.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Feb 07 04:30:04 2023
Response via : Initial Calibration

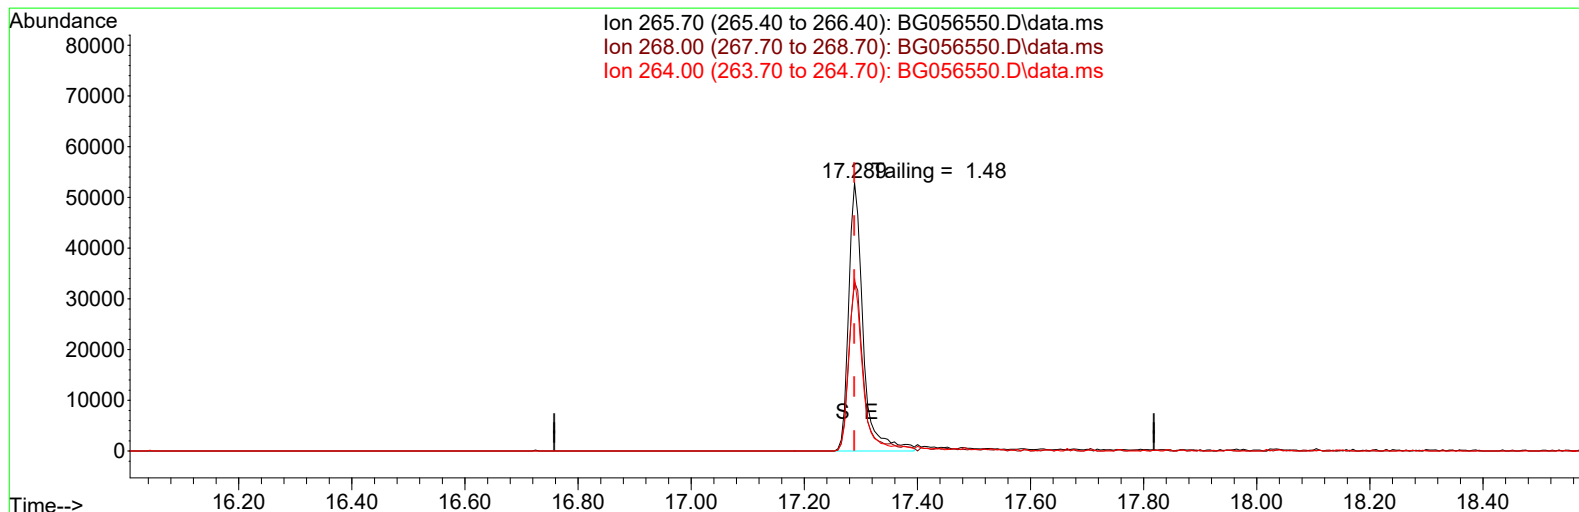

TIC: BG056550.D\data.ms

(70) Pentachlorophenol (C)

17.289min (+ 0.001) 188137.52 ng

response 92778

Ion	Exp%	Act%
-----	------	------

265.70	100.00	100.00
--------	--------	--------




268.00	62.80	63.04
--------	-------	-------

264.00	64.20	64.22
--------	-------	-------

0.00 0.00 0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG020623\
Data File : BG056550.D
Acq On : 6 Feb 2023 10:25
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Feb 07 05:37:53 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG012723.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Feb 07 04:30:04 2023
Response via : Initial Calibration

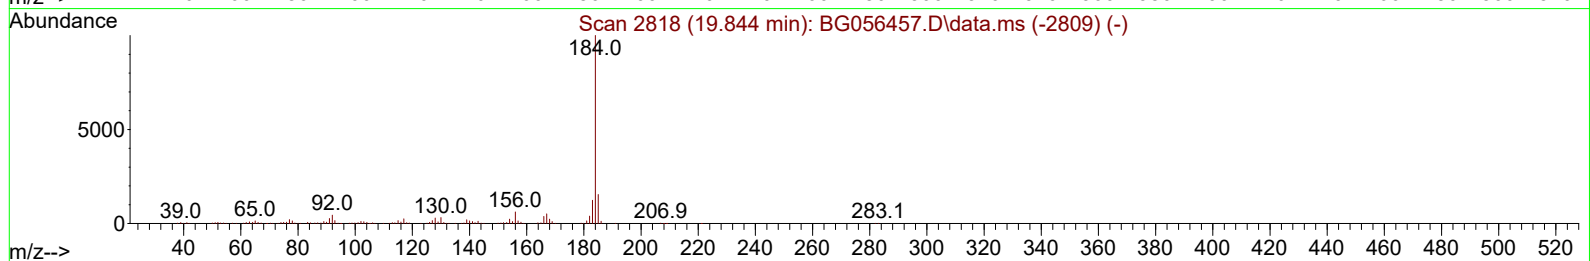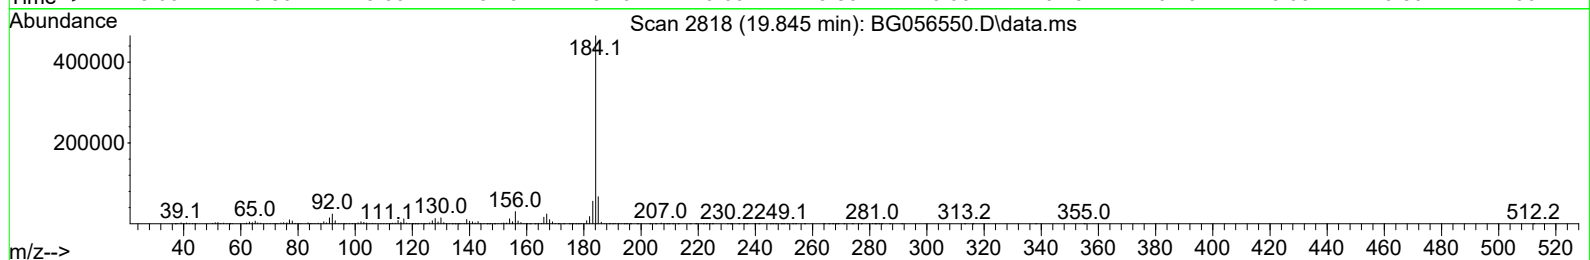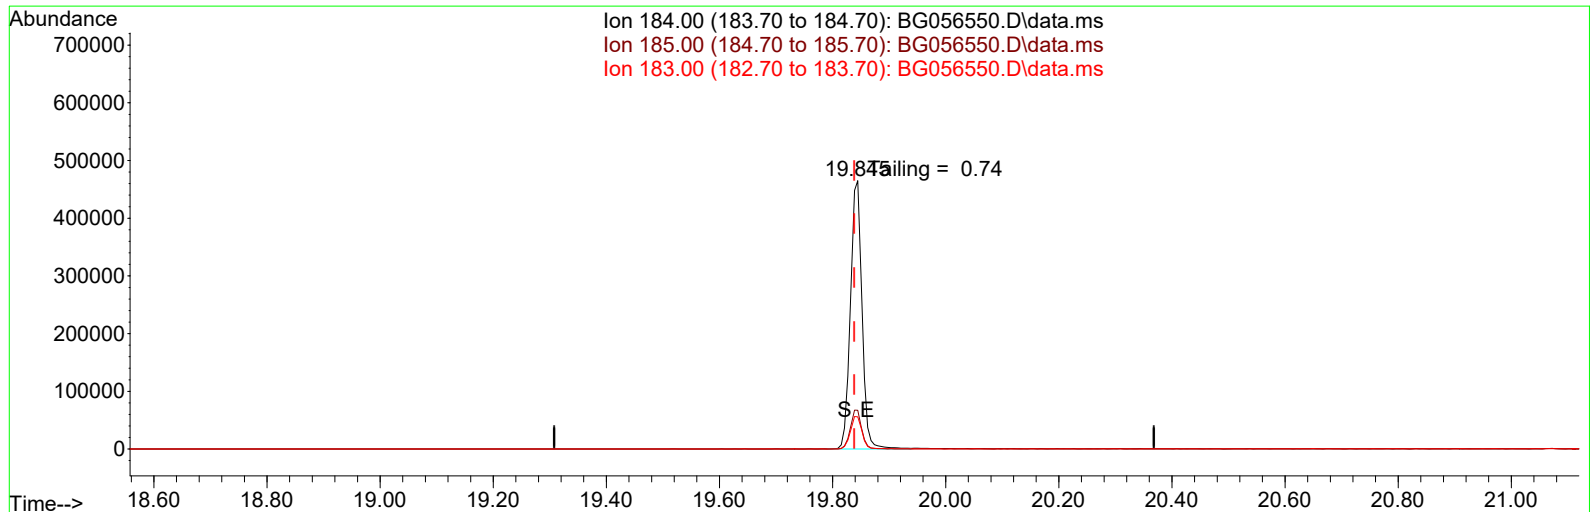

TIC: BG056550.D\data.ms

(77) Benzidine**19.845min (+ 0.007) 33033.89 ng****response 666877**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.40	14.43
183.00	12.30	12.02
0.00	0.00	0.00