

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG020623\
 Data File : BG056552.D
 Acq On : 6 Feb 2023 12:45
 Operator : CG/JU
 Sample : PB150235BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 PB150235BL

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG012723.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BG056552.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.309	337	344	354	rBB	128887	199115	5.28%	1.525%
2	5.796	420	427	440	rBV	564133	880562	23.37%	6.744%
3	7.424	694	704	716	rBV	540986	937795	24.89%	7.182%
4	8.276	842	849	856	rBB	111980	188192	4.99%	1.441%
5	9.451	1041	1049	1059	rBV	313845	555366	14.74%	4.253%
6	11.108	1323	1331	1344	rBB	157145	280315	7.44%	2.147%
7	13.523	1734	1742	1758	rBV	1252985	1945408	51.63%	14.899%
8	14.897	1969	1976	1984	rBV	316242	492343	13.07%	3.771%
9	16.378	2222	2228	2244	rBV	926141	1480023	39.28%	11.335%
10	17.635	2435	2442	2451	rBV	474668	734712	19.50%	5.627%
11	20.215	2874	2881	2888	rBV	2719543	3768313	100.00%	28.860%
12	21.924	3166	3172	3181	rVB2	465389	798805	21.20%	6.118%
13	25.356	3747	3756	3766	rVB2	266588	796487	21.14%	6.100%




Sum of corrected areas: 13057436

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG020623\
Data File : BG056552.D
Acq On : 6 Feb 2023 12:45
Operator : CG/JU
Sample : PB150235BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
PB150235BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG012723.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

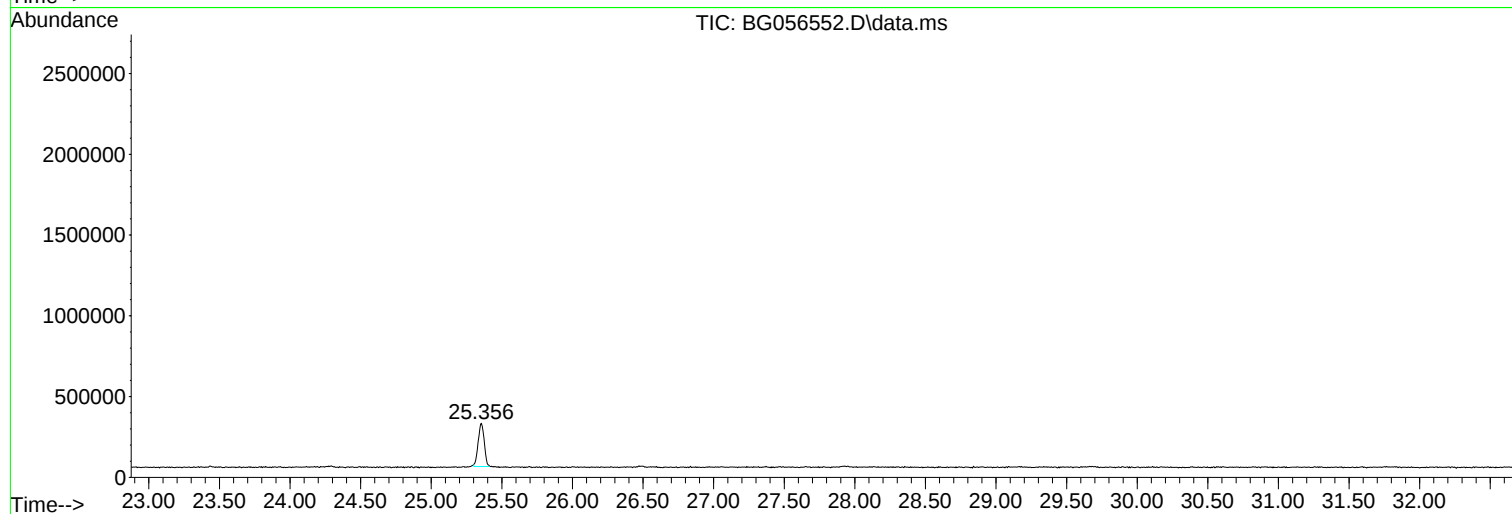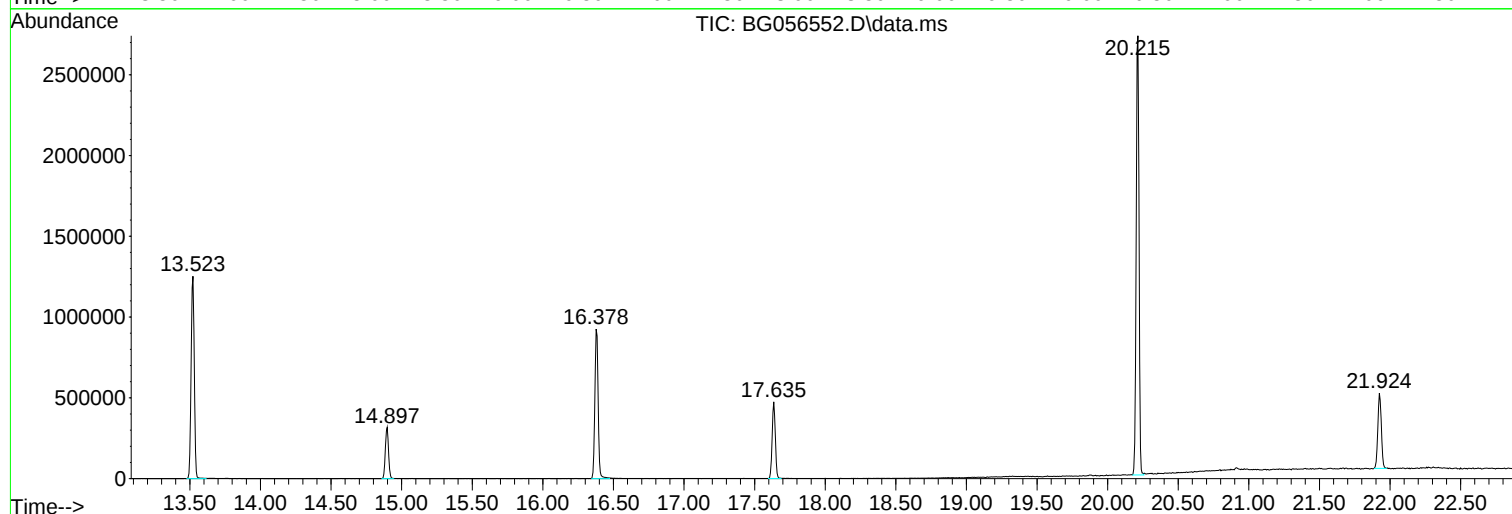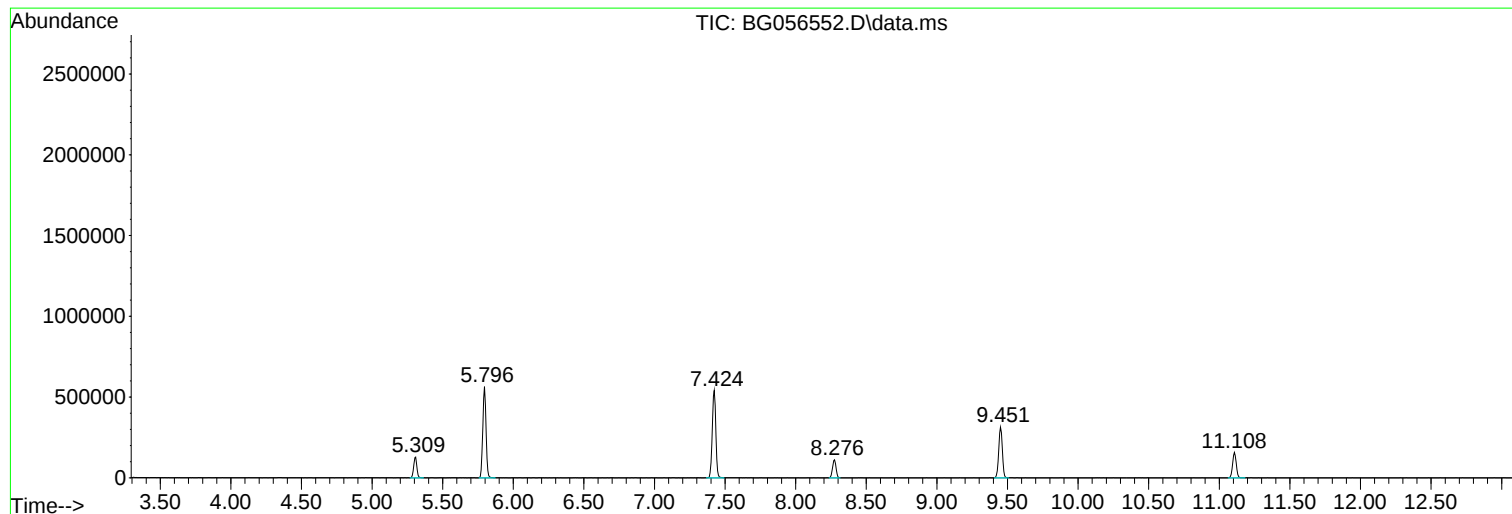

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG020623\
Data File : BG056552.D
Acq On : 6 Feb 2023 12:45
Operator : CG/JU
Sample : PB150235BL
Misc :
ALS Vial : 3 Sample Multiplier: 1










Instrument :
BNA_G
ClientSampleId :
PB150235BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG012723.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 2-Pentanone, 4-hydroxy-4-me... Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.	
5.309	21.16 ng	199115	1,4-Dichlorobenzene-d4	8.276	
Hit# of 5	Tentative ID	MW	MolForm	CAS#	Qual
1	2-Pentanone, 4-hydroxy-4-methyl-	116	C6H12O2	000123-42-2	50
2	Guanidine	59	CH5N3	000113-00-8	37
3	Propane, 1-ethoxy-2-methyl-	102	C6H14O	000627-02-1	32
4	3-Hydroxy-3-methyl-2-butanone	102	C5H10O2	000115-22-0	32
5	Oxirane, tetramethyl-	100	C6H12O	005076-20-0	23

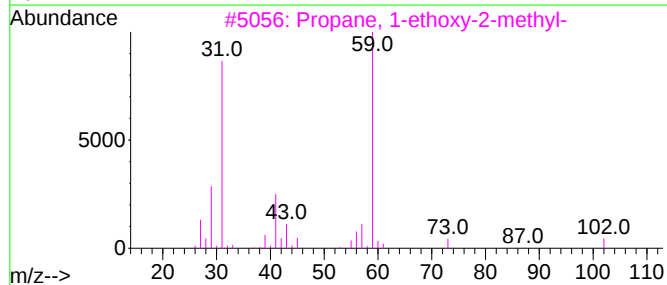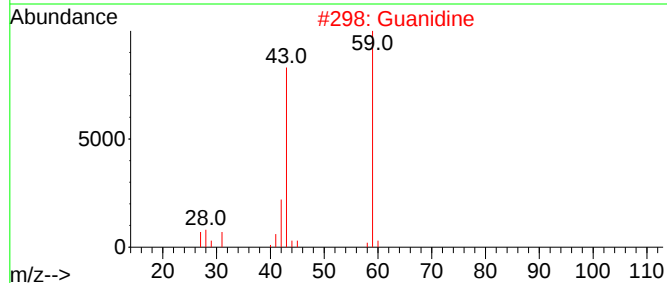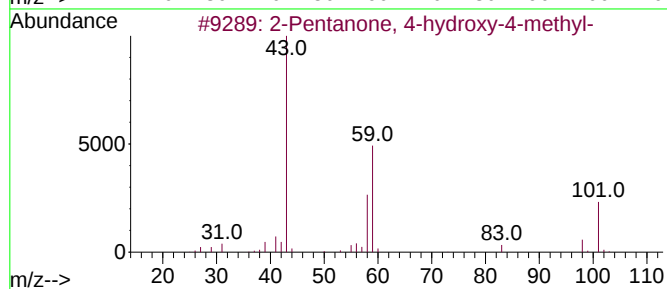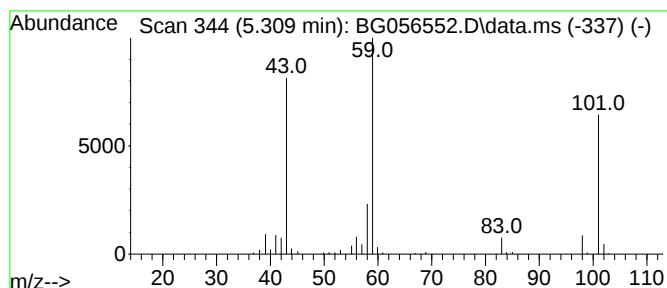

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG020623\
Data File : BG056552.D
Acq On : 6 Feb 2023 12:45
Operator : CG/JU
Sample : PB150235BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
PB150235BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG012723.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
2-Pentanone, 4-...	5.309	21.2	ng	199115	1	8.276	188192	20.0