


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG020623\
Data File : BG056550.D
Acq On : 6 Feb 2023 10:25
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG012723.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Tue Feb 07 04:30:04 2023

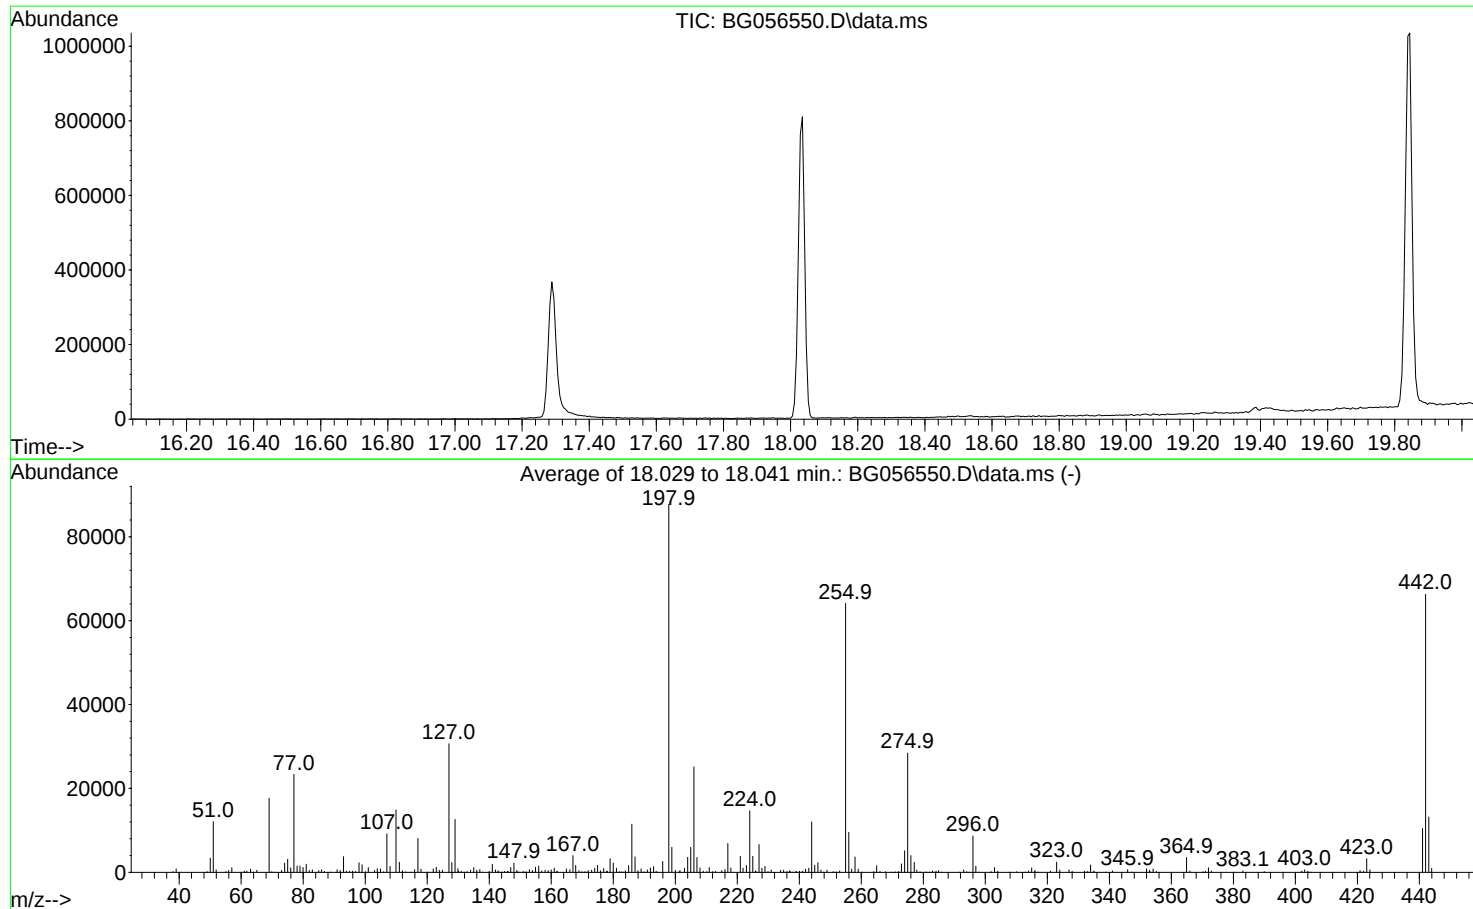




AutoFind: Scans 2509, 2510, 2511; Background Corrected with Scan 2501

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	13.8	12088	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	20.2	17692	PASS
70	69	0.00	2	0.9	158	PASS
127	198	10	80	35.0	30664	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	87717	PASS
199	198	5	9	6.8	5965	PASS
275	198	10	60	32.4	28405	PASS
365	198	1	100	4.0	3543	PASS
441	198	0.01	100	11.9	10437	PASS
442	442	50	100	100.0	66272	PASS
443	442	15	24	19.9	13180	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG020623\
Data File : BG056550.D
Acq On : 6 Feb 2023 10:25
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: Feb 07 05:37:53 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG012723.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Feb 07 04:30:04 2023
Response via : Initial Calibration

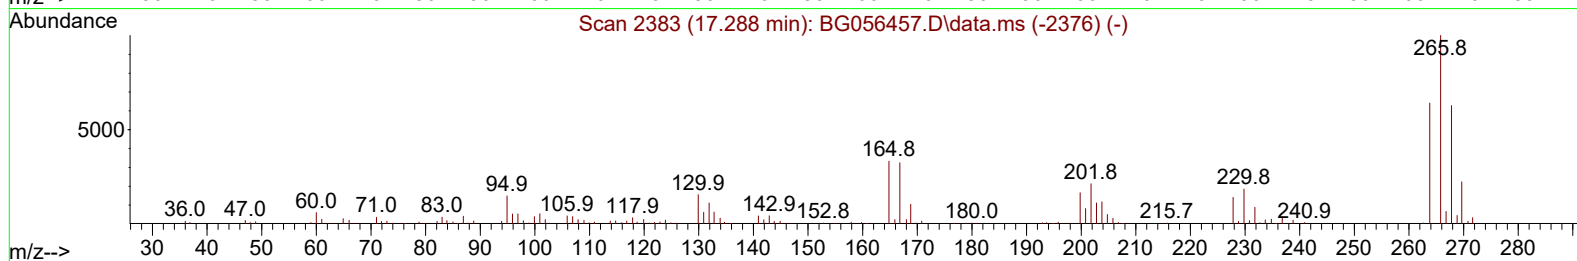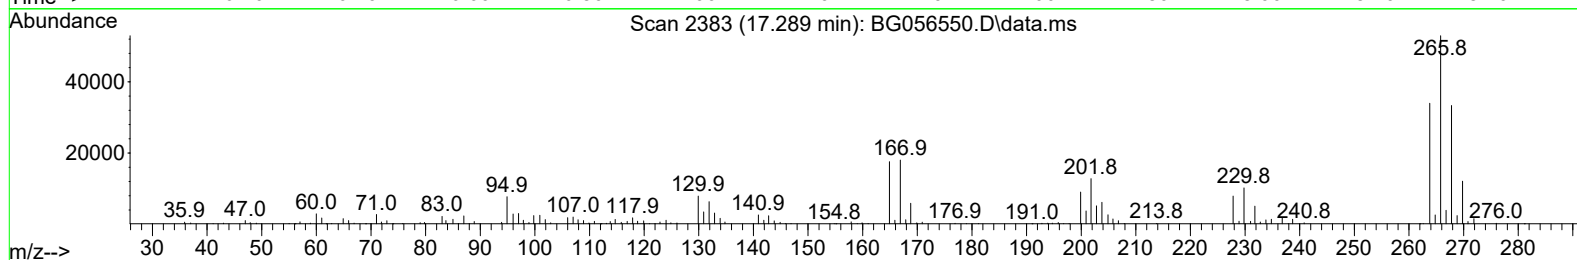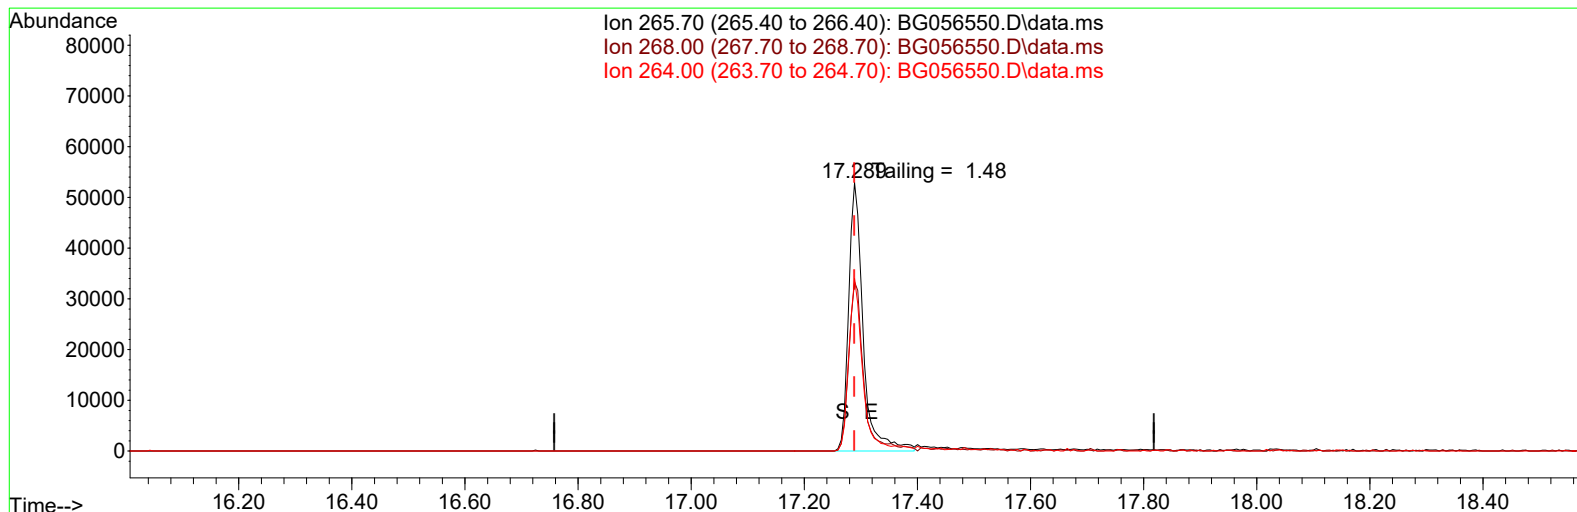

TIC: BG056550.D\data.ms

(70) Pentachlorophenol (C)

17.289min (+ 0.001) 188137.52 ng

response **92778**

Ion	Exp%	Act%
-----	------	------

265.70	100.00	100.00
--------	--------	--------

268.00	62.80	63.04
--------	-------	-------




264.00	64.20	64.22
--------	-------	-------

0.00 0.00 0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG020623\
Data File : BG056550.D
Acq On : 6 Feb 2023 10:25
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: Feb 07 05:37:53 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG012723.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Feb 07 04:30:04 2023
Response via : Initial Calibration

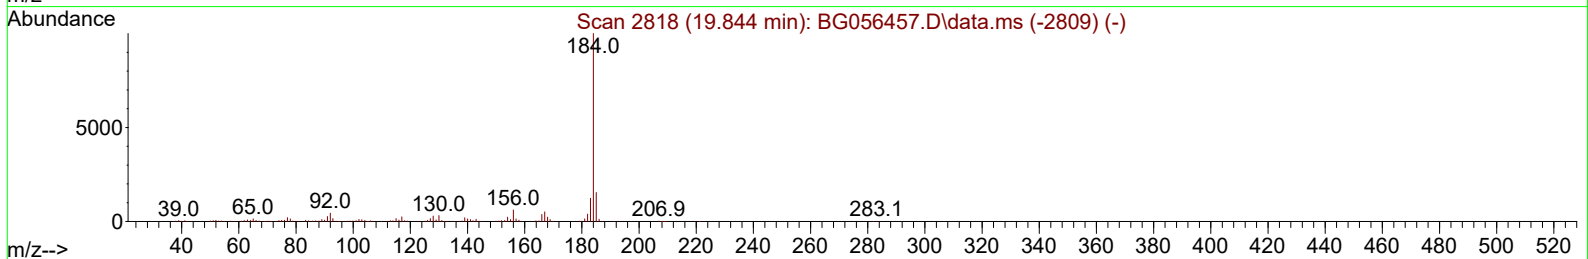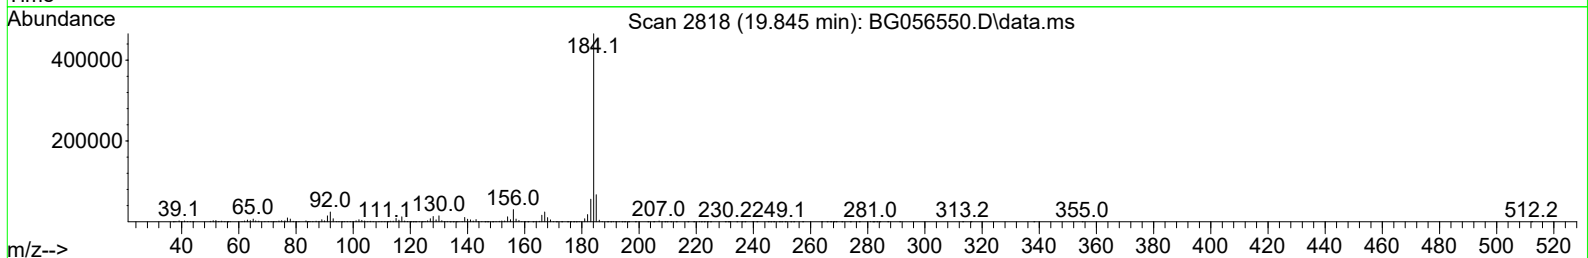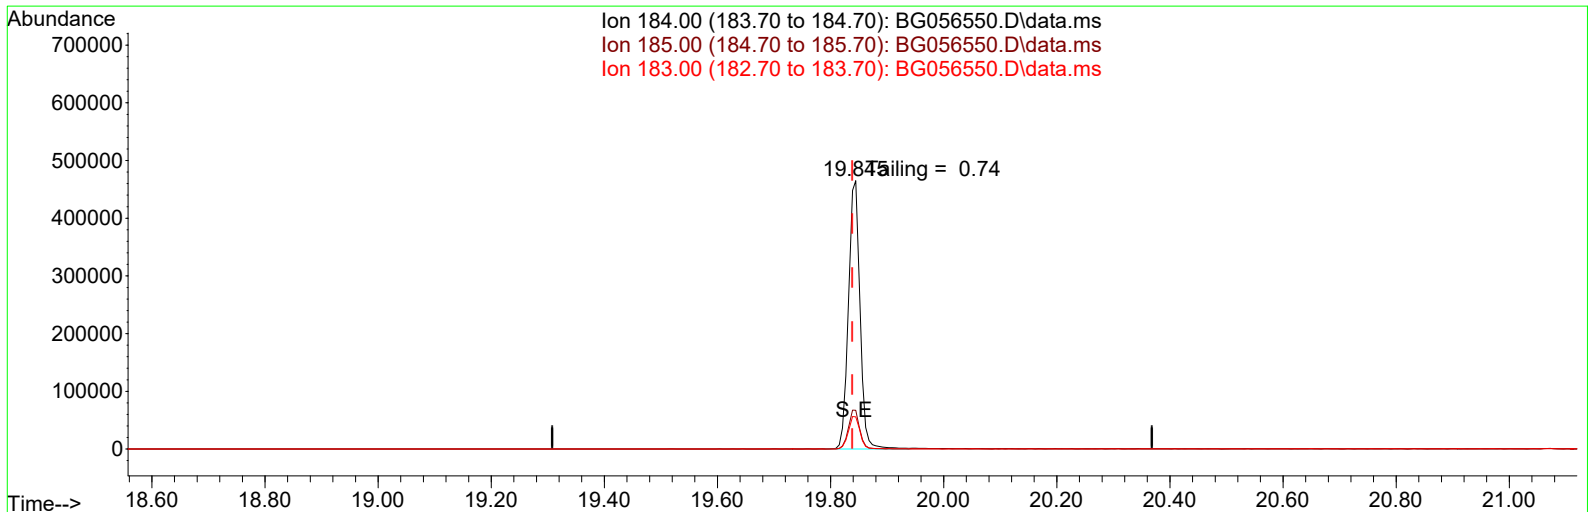

TIC: BG056550.D\data.ms

(77) Benzidine

19.845min (+ 0.007) 33033.89 ng

response 666877

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.40	14.43
183.00	12.30	12.02
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
2/6/2023	BNA_G	<u>BG056550.D</u>
Compound Name	Response	Retention Time
DDT	291372	21.073
DDD	9210	20.62
DDE	986	20.115
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
10196	301568	3.38

Instrument :
BNA_G
ClientSampleId :
DFTPP