

Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG020719\
 Data File : BG039412.D
 Acq On : 8 Feb 2019 11:22
 Operator : JU/SJ
 Sample : K1401-08
 Misc :
 ALS Vial : 30 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 RT-3451

Quant Time: Feb 09 02:05:58 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG012919.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Jan 29 15:41:51 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.18	152	50911	20.00	ng	0.00
21) Naphthalene-d8	11.00	136	214555	20.00	ng	-0.01
39) Acenaphthene-d10	14.80	164	141247	20.00	ng	-0.01
64) Phenanthrene-d10	17.54	188	345404	20.00	ng	-0.01
76) Chrysene-d12	21.83	240	374850	20.00	ng	-0.02
87) Perylene-d12	25.22	264	352912	20.00	ng	-0.02
System Monitoring Compounds						
5) 2-Fluorophenol	5.72	112	425551	143.06	ng	0.00
7) Phenol-d6	7.32	99	553247	126.35	ng	0.00
23) Nitrobenzene-d5	9.35	82	403743	117.56	ng	0.00
42) 2,4,6-Tribromophenol	16.28	330	204358	134.36	ng	-0.01
45) 2-Fluorobiphenyl	13.43	172	980129	99.55	ng	-0.01
79) Terphenyl-d14	20.14	244	1585039	89.50	ng	-0.01


Target Compounds Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG020719\
Data File : BG039412.D
Acq On : 8 Feb 2019 11:22
Operator : JU/SJ
Sample : K1401-08
Misc :
ALS Vial : 30 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
RT-3451

Quant Time: Feb 09 02:05:58 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG012919.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jan 29 15:41:51 2019
Response via : Initial Calibration

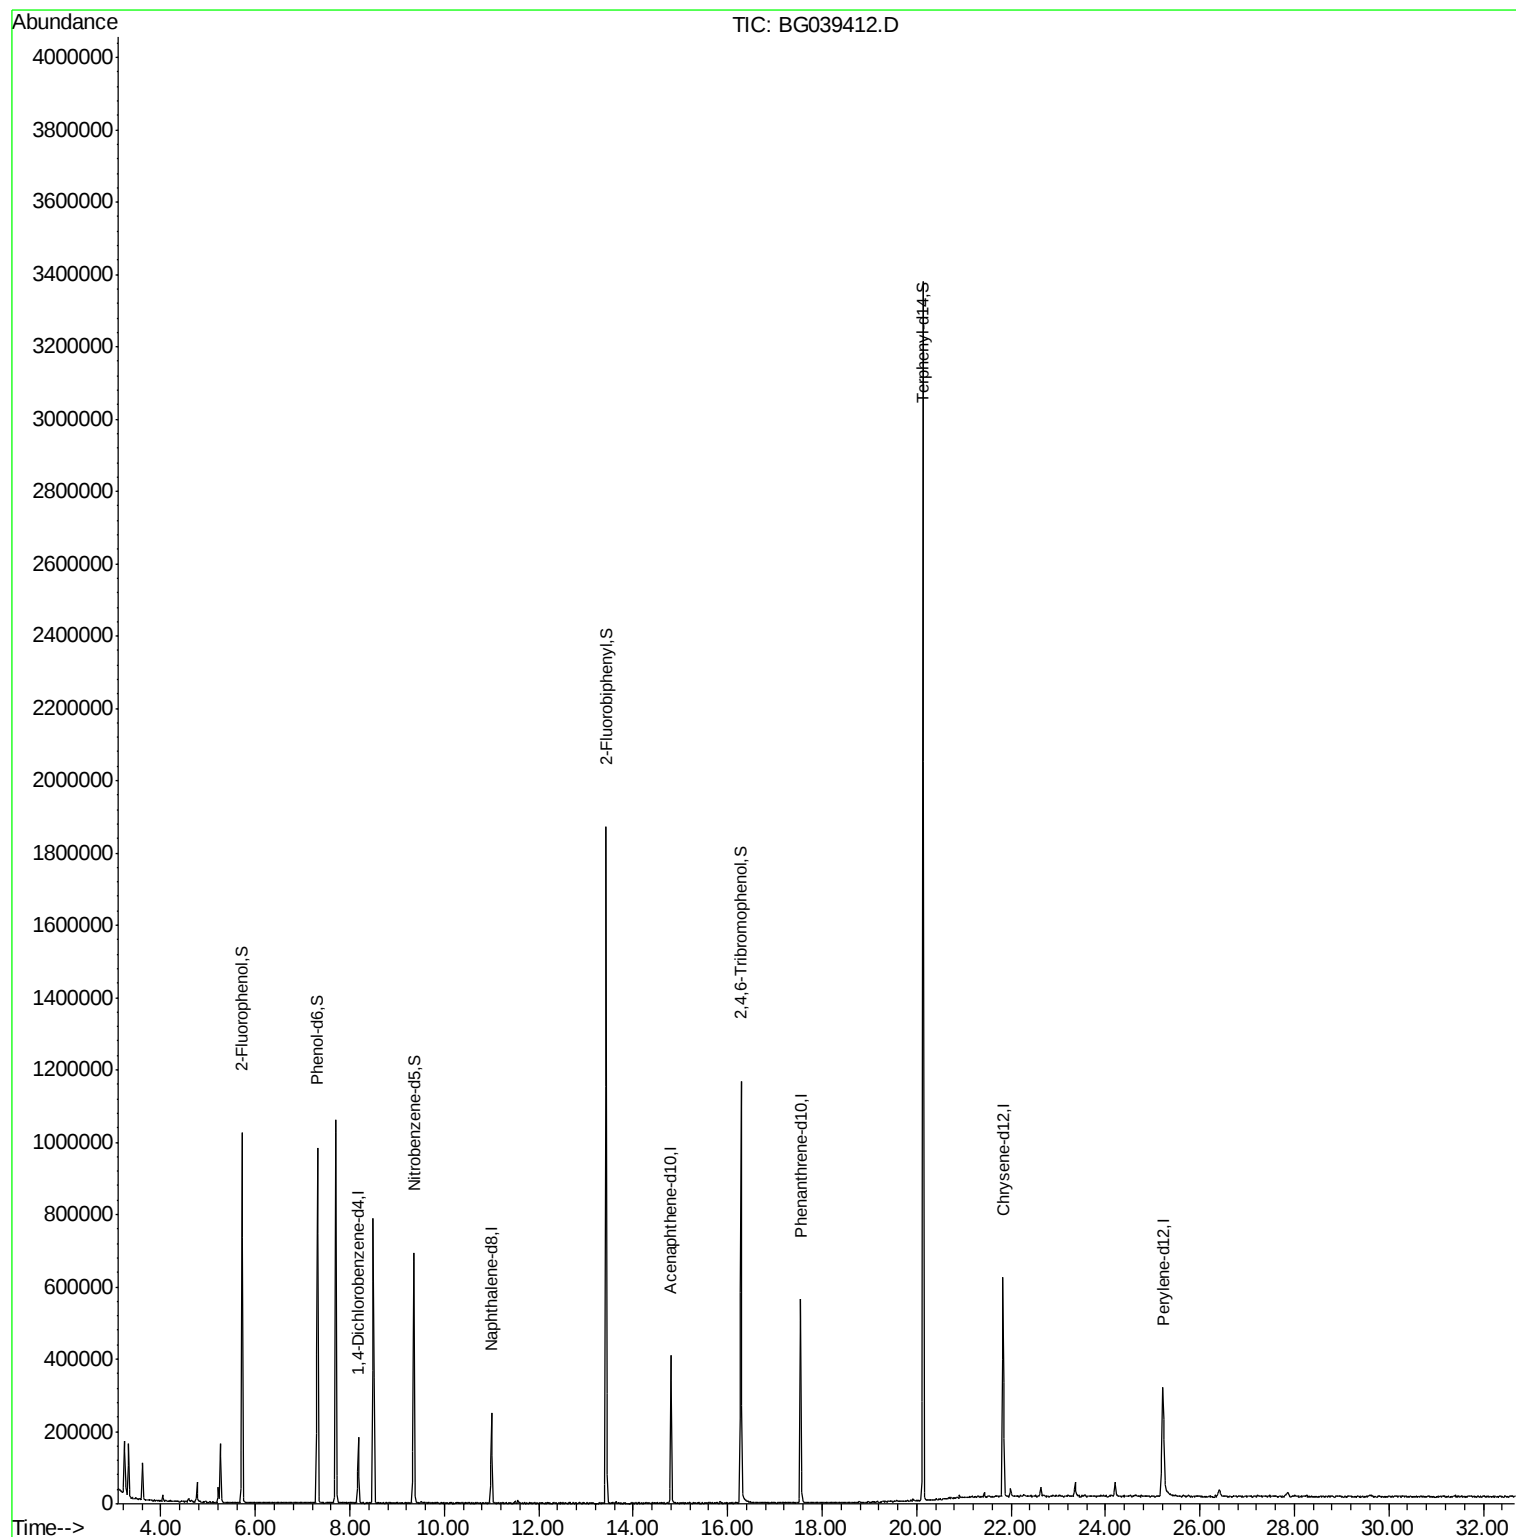

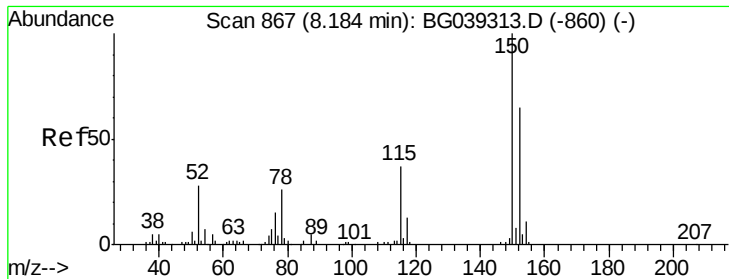


#1

1,4-Dichlorobenzene-d4
Concen: 20.000 ng
RT: 8.18 min Scan# 867
Delta R.T. -0.00 min
Lab File: BG039412.D
Acq: 8 Feb 2019 11:22

Instrument :
BNA_G
ClientSampleId :
RT-3451

Tot Ion	Ratio	Lower	Upper
152	100		
150	153.9	123.7	185.5
115	59.0	45.9	68.9



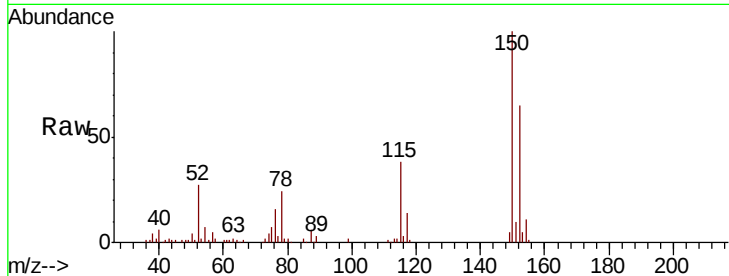


Abundance

Ion 152.00 (151.70 to 152.70): E

Ion 150.00 (149.70 to 150.70): E


Ion 115.00 (114.70 to 115.70): E

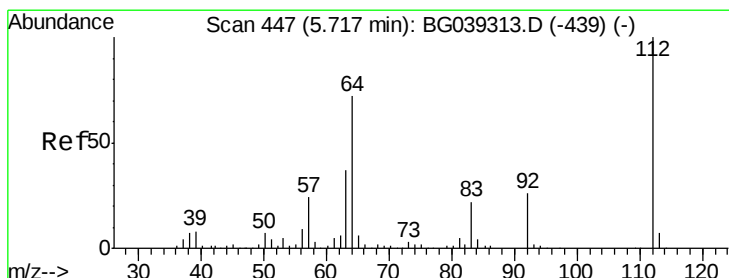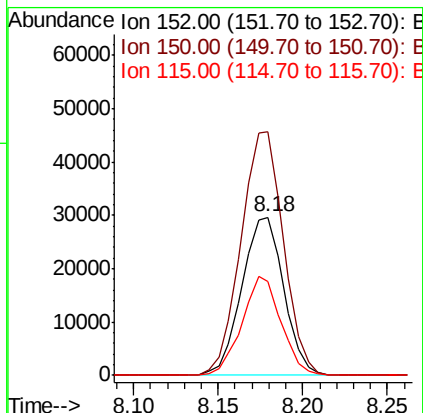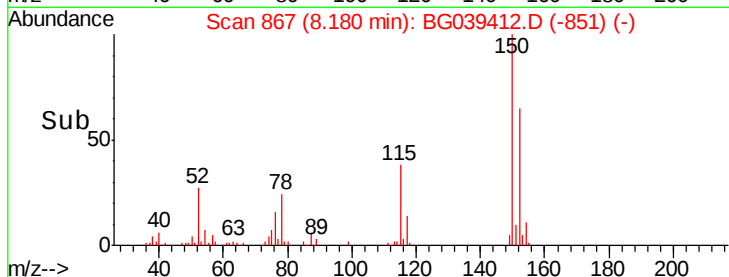

#5

2-Fluorophenol
Concen: 143.060 ng
RT: 5.72 min Scan# 448
Delta R.T. 0.00 min
Lab File: BG039412.D
Acq: 8 Feb 2019 11:22

Tgt Ion	Ratio	Lower	Upper
112	100		
64	68.5	57.8	86.8
63	36.0	29.8	44.6


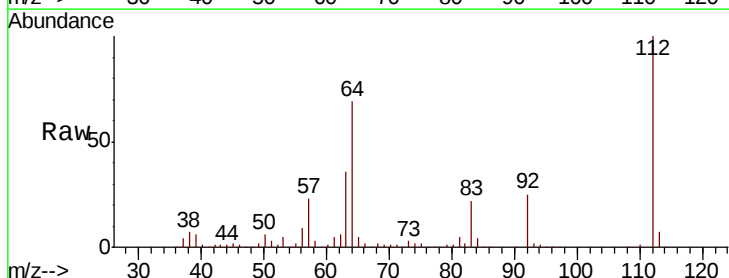


Abundance

Ion 112.00 (111.70 to 112.70): E

Ion 64.00 (63.70 to 64.70): BGC

Ion 63.00 (62.70 to 63.70): BGC

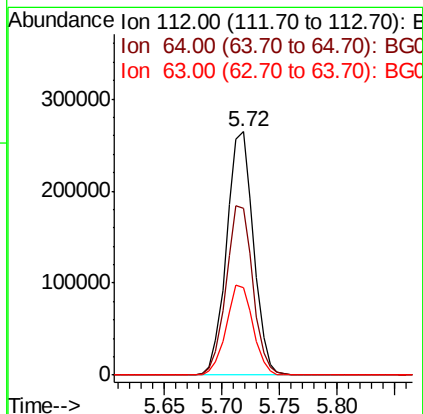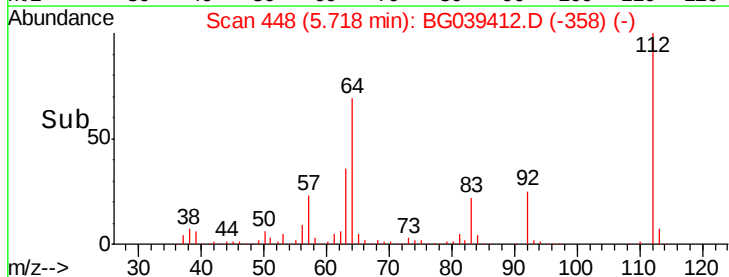



#7

Phenol-d6

Concen: 126.353 ng

RT: 7.32 min Scan# 720

Delta R.T. -0.00 min

Lab File: BG039412.D

Acq: 8 Feb 2019 11:22

Instrument :

BNA_G

ClientSampleId :

RT-3451


Tot Ion: 99 Resp: 553247

Ion Ratio Lower Upper




99 100

42 20.8 18.2 27.2

71 36.3 28.0 42.0

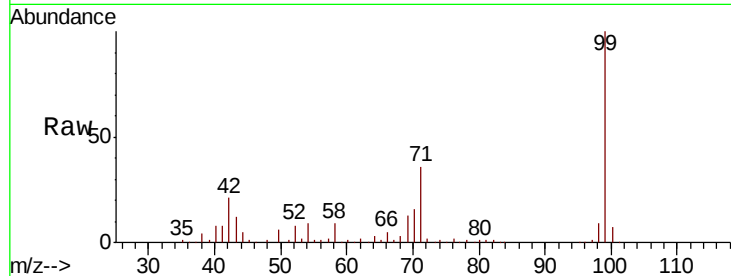

Abundance Ion 99.00 (98.70 to 99.70): BGC
Ion 42.00 (41.70 to 42.70): BGC
Ion 71.00 (70.70 to 71.70): BGC

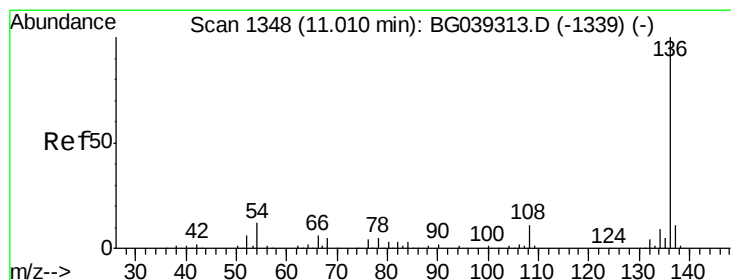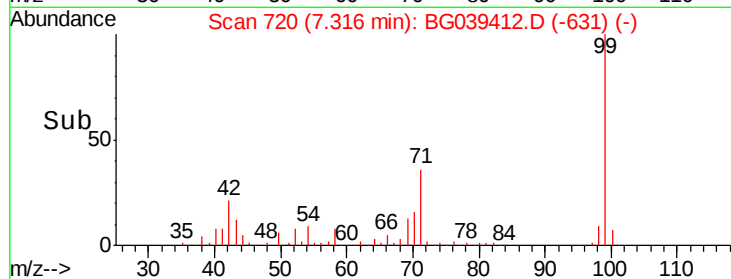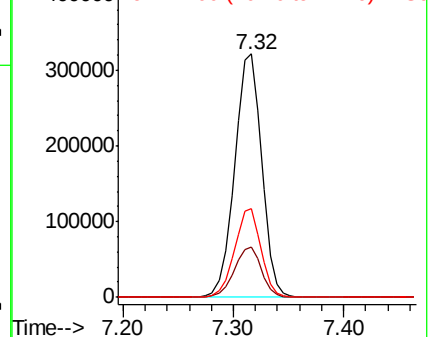

#21

Naphthalene-d8

Concen: 20.000 ng

RT: 11.00 min Scan# 1347

Delta R.T. -0.01 min

Lab File: BG039412.D

Acq: 8 Feb 2019 11:22

Tgt Ion: 136 Resp: 214555


Ion Ratio Lower Upper

136 100



137 12.0 9.1 13.7


54 10.5 9.4 14.2

68 5.4 4.2 6.4

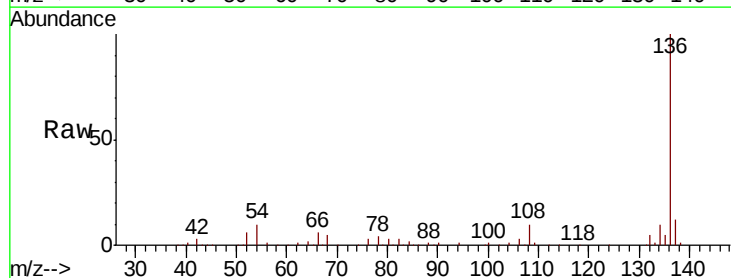

Abundance Ion 136.00 (135.70 to 136.70): BGC
Ion 137.00 (136.70 to 137.70): BGC
Ion 54.00 (53.70 to 54.70): BGC
Ion 68.00 (67.70 to 68.70): BGC



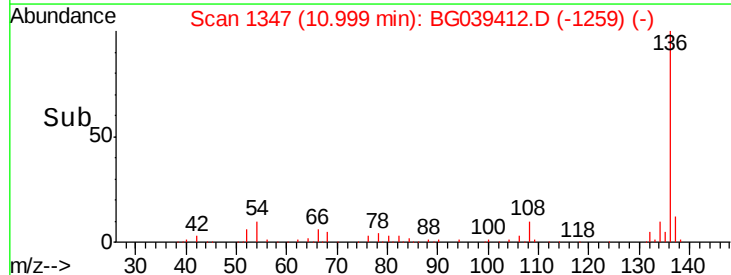
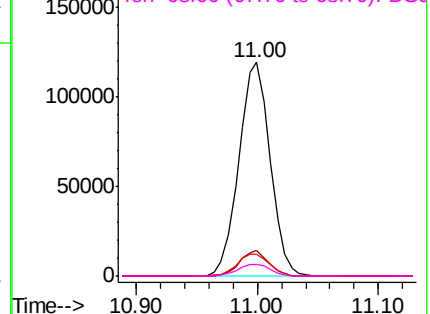


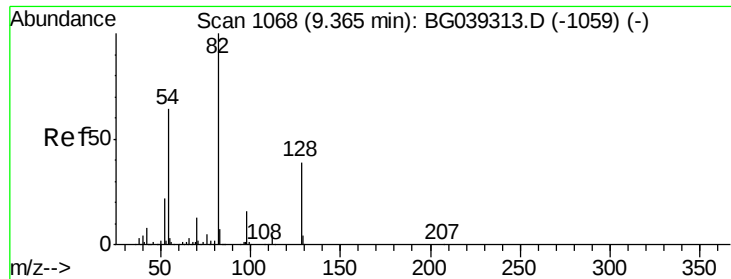

#23
 Nitrobenzene-d5
 Concen: 117.557 ng
 RT: 9.35 min Scan# 1067
 Delta R.T. -0.01 min
 Lab File: BG039412.D
 Acq: 8 Feb 2019 11:22




Instrument :
 BNA_G
 ClientSampleId :
 RT-3451


Tot Ion	82	Resp	403743
Ion Ratio	Lower	Upper	
82	100		
128	41.8	31.3	46.9
54	59.3	50.9	76.3

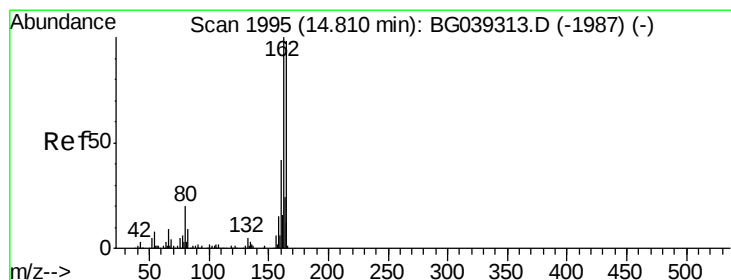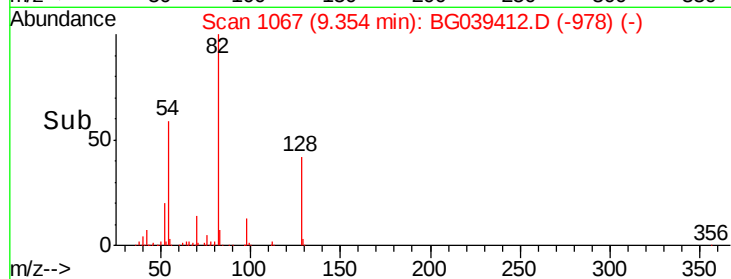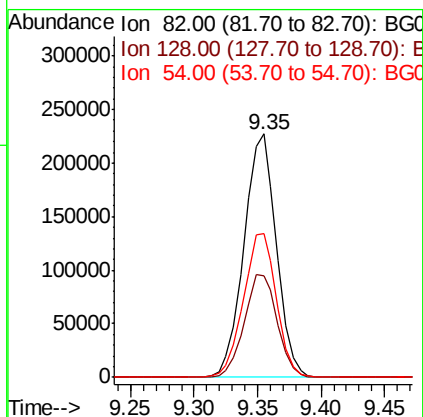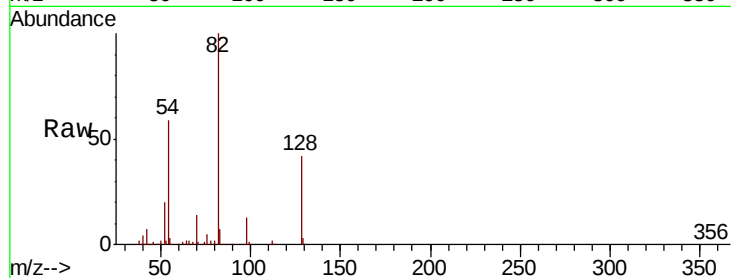

#39
 Acenaphthene-d10
 Concen: 20.000 ng
 RT: 14.80 min Scan# 1994
 Delta R.T. -0.01 min
 Lab File: BG039412.D
 Acq: 8 Feb 2019 11:22

Tgt Ion	164	Resp	141247
Ion Ratio	Lower	Upper	
164	100		
162	104.0	81.6	122.4
160	44.3	34.2	51.2

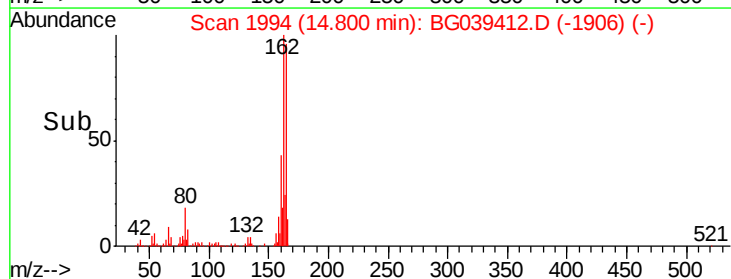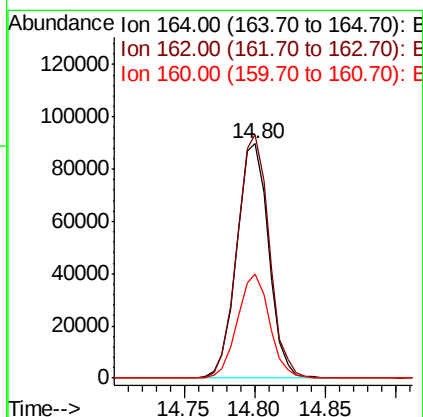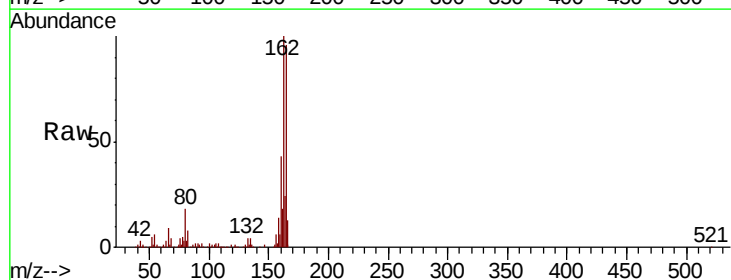


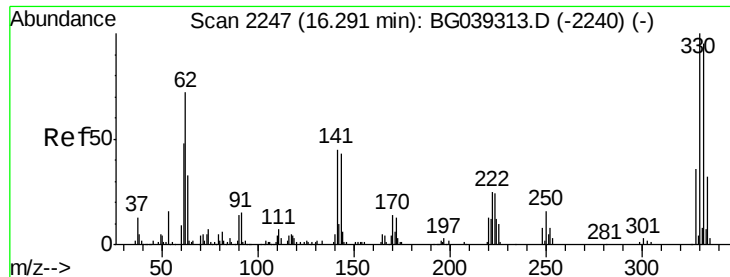



#42
 2,4,6-Tribromophenol
 Concen: 134.359 ng
 RT: 16.28 min Scan# 2246
 Delta R.T. -0.01 min
 Lab File: BG039412.D
 Acq: 8 Feb 2019 11:22

Instrument :
 BNA_G
 ClientSampleId :
 RT-3451

Tot Ion:330 Resp: 204358
 Ion Ratio Lower Upper
 330 100
 332 95.0 75.7 113.5
 141 40.6 35.6 53.4

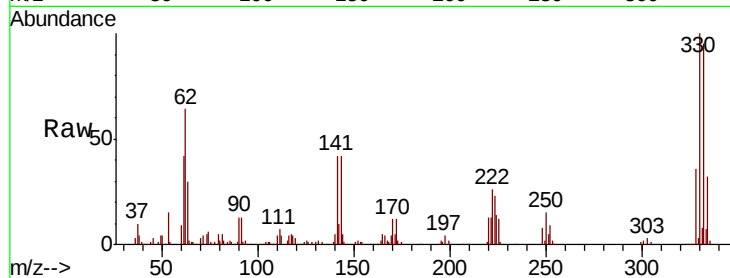


Abundance Ion 329.80 (329.50 to 330.50): E
 Ion 331.80 (331.50 to 332.50): E
 Ion 141.00 (140.70 to 141.70): E

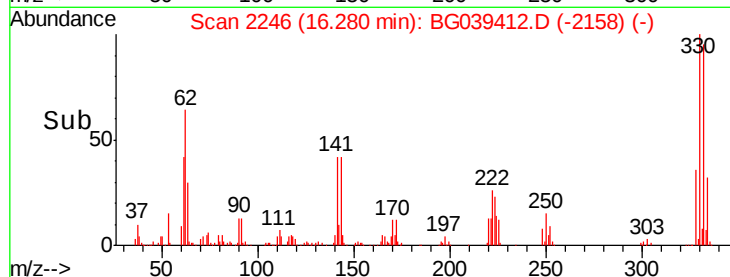
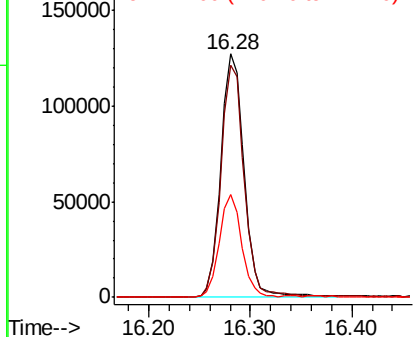



#45
 2-Fluorobiphenyl
 Concen: 99.545 ng
 RT: 13.43 min Scan# 1760
 Delta R.T. -0.01 min
 Lab File: BG039412.D
 Acq: 8 Feb 2019 11:22

Tgt Ion:172 Resp: 980129
 Ion Ratio Lower Upper
 172 100
 171 38.8 30.8 46.2
 170 25.2 20.2 30.4

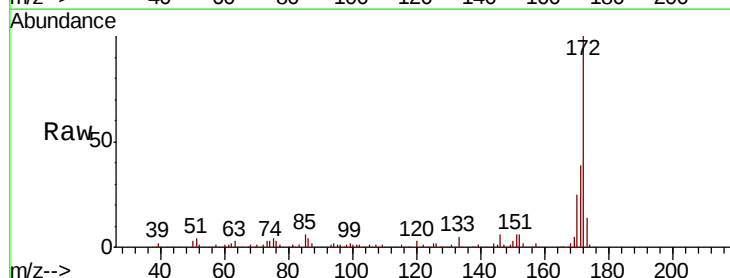

Abundance Ion 172.00 (171.70 to 172.70): E
 Ion 171.00 (170.70 to 171.70): E
 Ion 170.00 (169.70 to 170.70): E

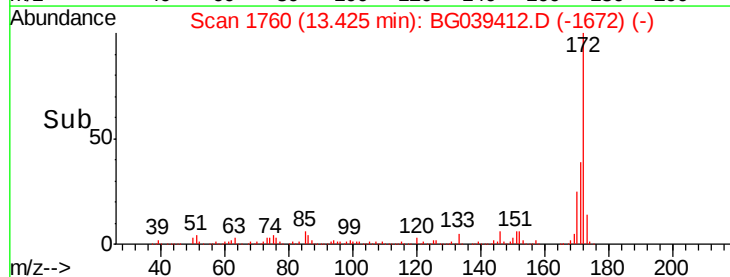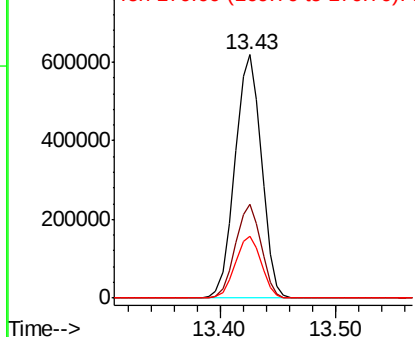

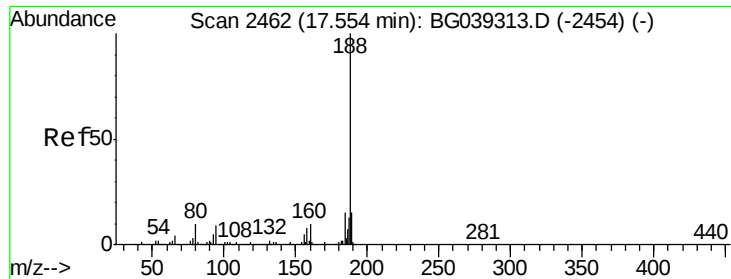

#64

Phenanthrene-d10

Concen: 20.000 ng

RT: 17.54 min Scan# 2461

Delta R.T. -0.01 min

Lab File: BG039412.D

Acq: 8 Feb 2019 11:22

Instrument :

BNA_G

ClientSampleId :

RT-3451


Tot Ion:188 Resp: 345404

Ion Ratio Lower Upper

188 100

94 8.0 6.9 10.3



80 8.8 8.1 12.1

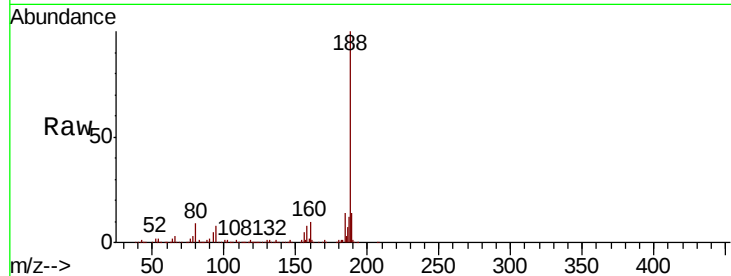

Abundance Ion 188.00 (187.70 to 188.70): E

Ion 94.00 (93.70 to 94.70): BG

Ion 80.00 (79.70 to 80.70): BG

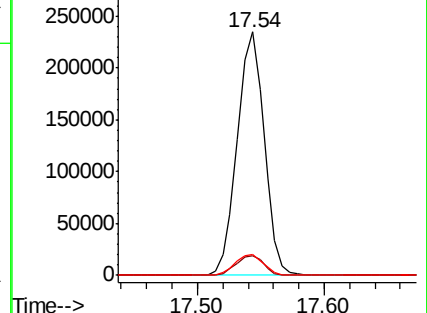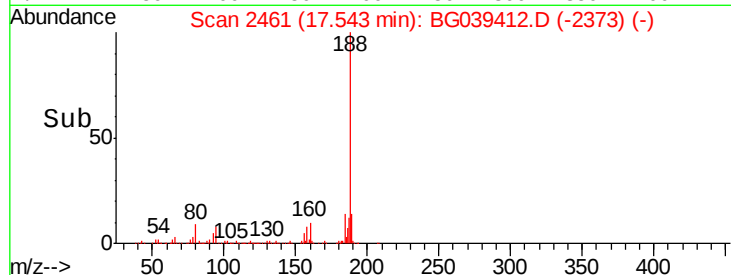

#76

Chrysene-d12

Concen: 20.000 ng

RT: 21.83 min Scan# 3191

Delta R.T. -0.02 min

Lab File: BG039412.D

Acq: 8 Feb 2019 11:22


Tgt Ion:240 Resp: 374850

Ion Ratio Lower Upper

240 100

120 9.4 7.0 10.6



236 25.5 21.0 31.4

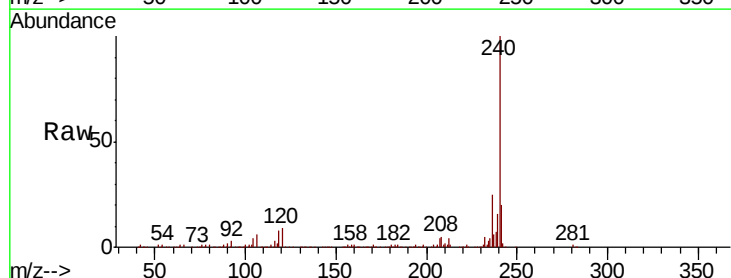

Abundance Ion 240.00 (239.70 to 240.70): E

Ion 120.00 (119.70 to 120.70): E

Ion 236.00 (235.70 to 236.70): E

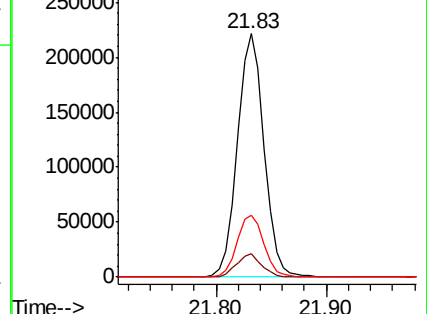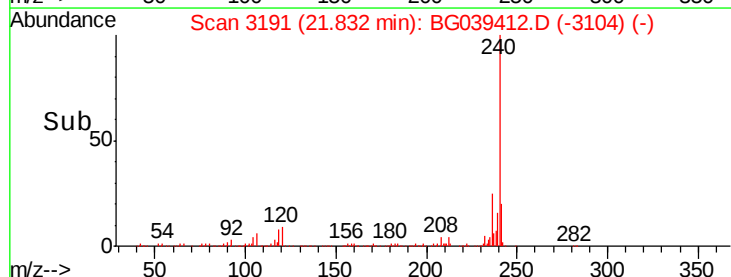



#79

Terphenyl-d14

Concen: 89.503 ng

RT: 20.14 min Scan# 2903

Delta R.T. -0.01 min

Lab File: BG039412.D

Acq: 8 Feb 2019 11:22

Instrument :


BNA_G

ClientSampled :

RT-3451

Tot Ion:244 Resp: 1585039

Ion	Ratio	Lower	Upper
244	100		
212	9.1	7.3	10.9
122	9.6	8.4	12.6



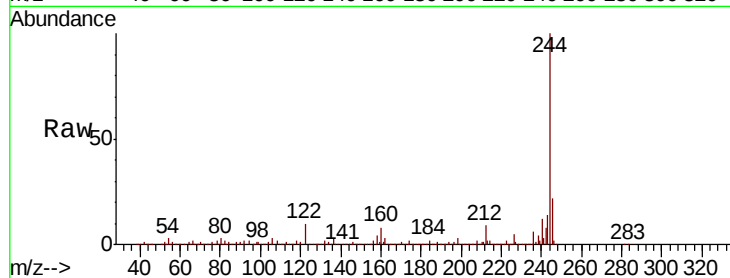


Abundance

Ion 244.00 (243.70 to 244.70): E

Ion 212.00 (211.70 to 212.70): E

Ion 122.00 (121.70 to 122.70): E

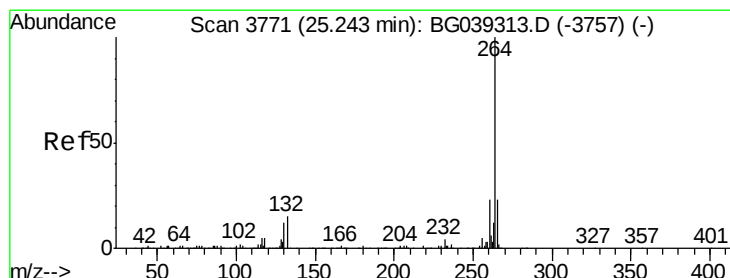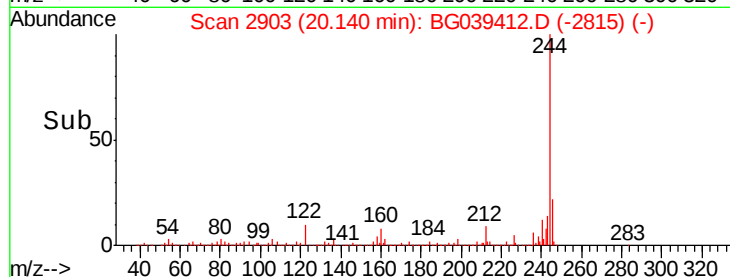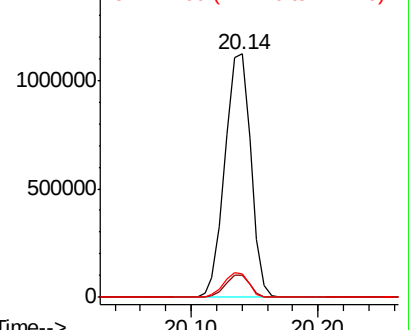

#87

Perylene-d12

Concen: 20.000 ng

RT: 25.22 min Scan# 3768


Delta R.T. -0.02 min

Lab File: BG039412.D

Acq: 8 Feb 2019 11:22

Tgt Ion:264 Resp: 352912

Ion	Ratio	Lower	Upper
264	100		
260	23.2	18.2	27.4
265	21.6	18.5	27.7

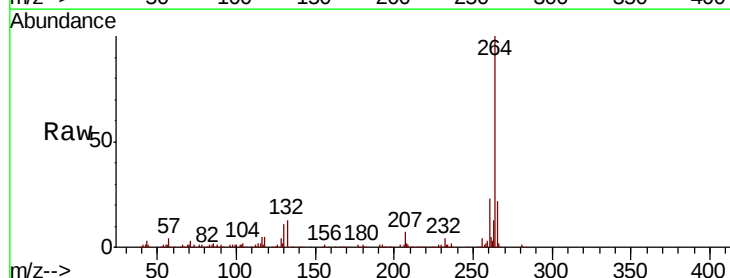

Abundance

Ion 264.00 (263.70 to 264.70): E

Ion 260.00 (259.70 to 260.70): E

Ion 265.00 (264.70 to 265.70): E

