


Data Path : Z:\SVOASRV\HPCHEM1\BNA_G\DATA\BG020719\
 Data File : BG039381.D
 Acq On : 7 Feb 2019 13:58
 Operator : JU/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG012919.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Jan 29 15:41:51 2019

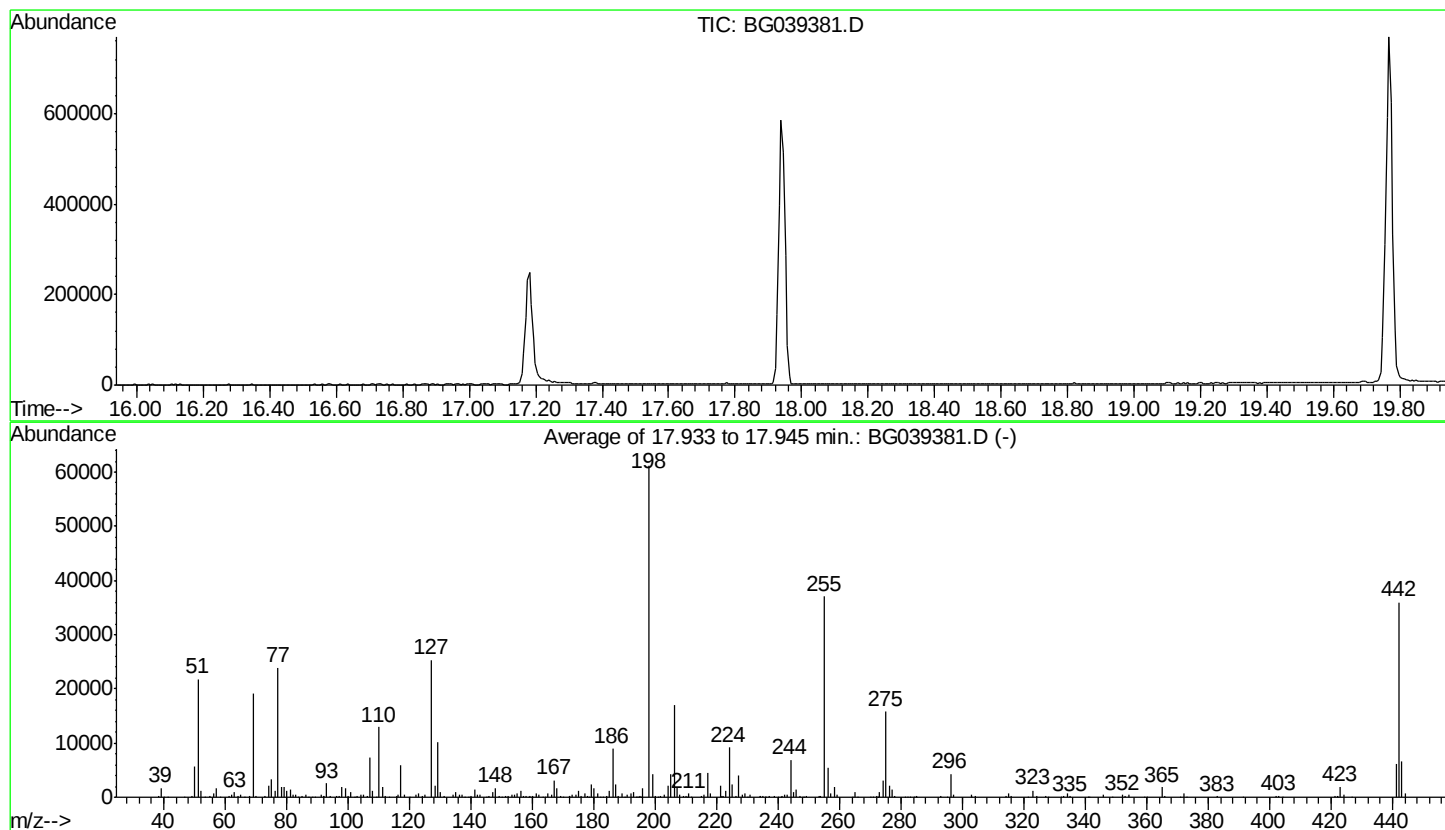

AutoFind: Scans 2527, 2528, 2529; Background Corrected with Scan 2521

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	35.7	21845	PASS
68	69	0.00	2	1.8	350	PASS
69	198	0.00	100	31.5	19250	PASS
70	69	0.00	2	0.9	178	PASS
127	198	10	80	41.5	25389	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	61186	PASS
199	198	5	9	6.9	4218	PASS
275	198	10	60	25.7	15719	PASS
365	198	1	100	3.0	1865	PASS
441	198	0.01	100	10.2	6222	PASS
442	198	50	100	58.8	35981	PASS
443	442	15	24	18.7	6720	PASS