


Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG020720\
 Data File : BG044330.D
 Acq On : 7 Feb 2020 10:14
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG013020.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Thu Jan 30 16:05:09 2020

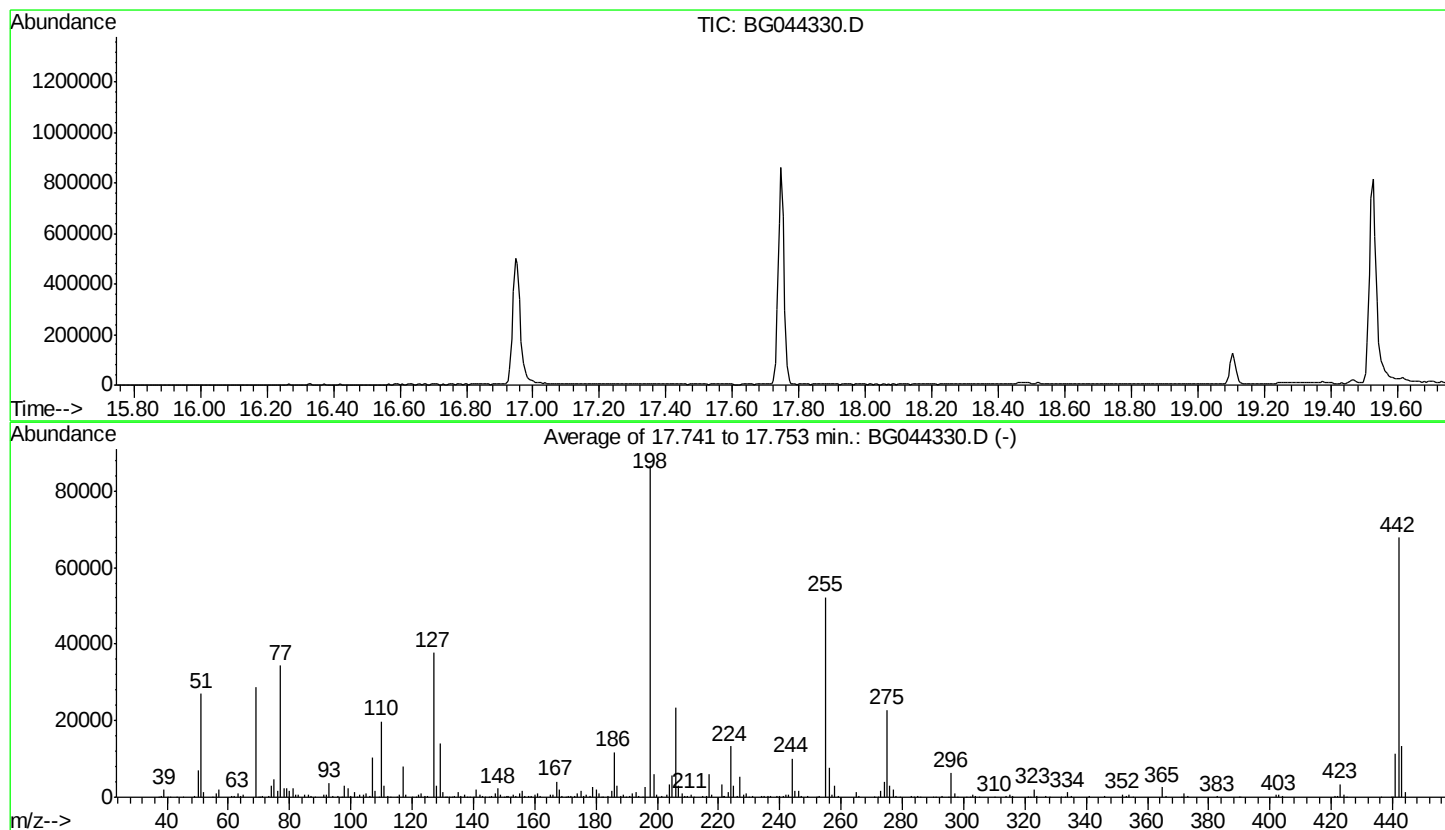

AutoFind: Scans 2494, 2495, 2496; Background Corrected with Scan 2487

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	31.2	27026	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	33.2	28730	PASS
70	69	0.00	2	0.5	147	PASS
127	198	10	80	43.6	37736	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	86605	PASS
199	198	5	9	6.9	5975	PASS
275	198	10	60	26.3	22768	PASS
365	198	1	100	3.0	2566	PASS
441	198	0.01	100	13.0	11285	PASS
442	198	50	100	78.3	67824	PASS
443	442	15	24	19.7	13390	PASS