


Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG020720\
 Data File : BG044348.D
 Acq On : 7 Feb 2020 22:13
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG013020.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Thu Jan 30 16:05:09 2020

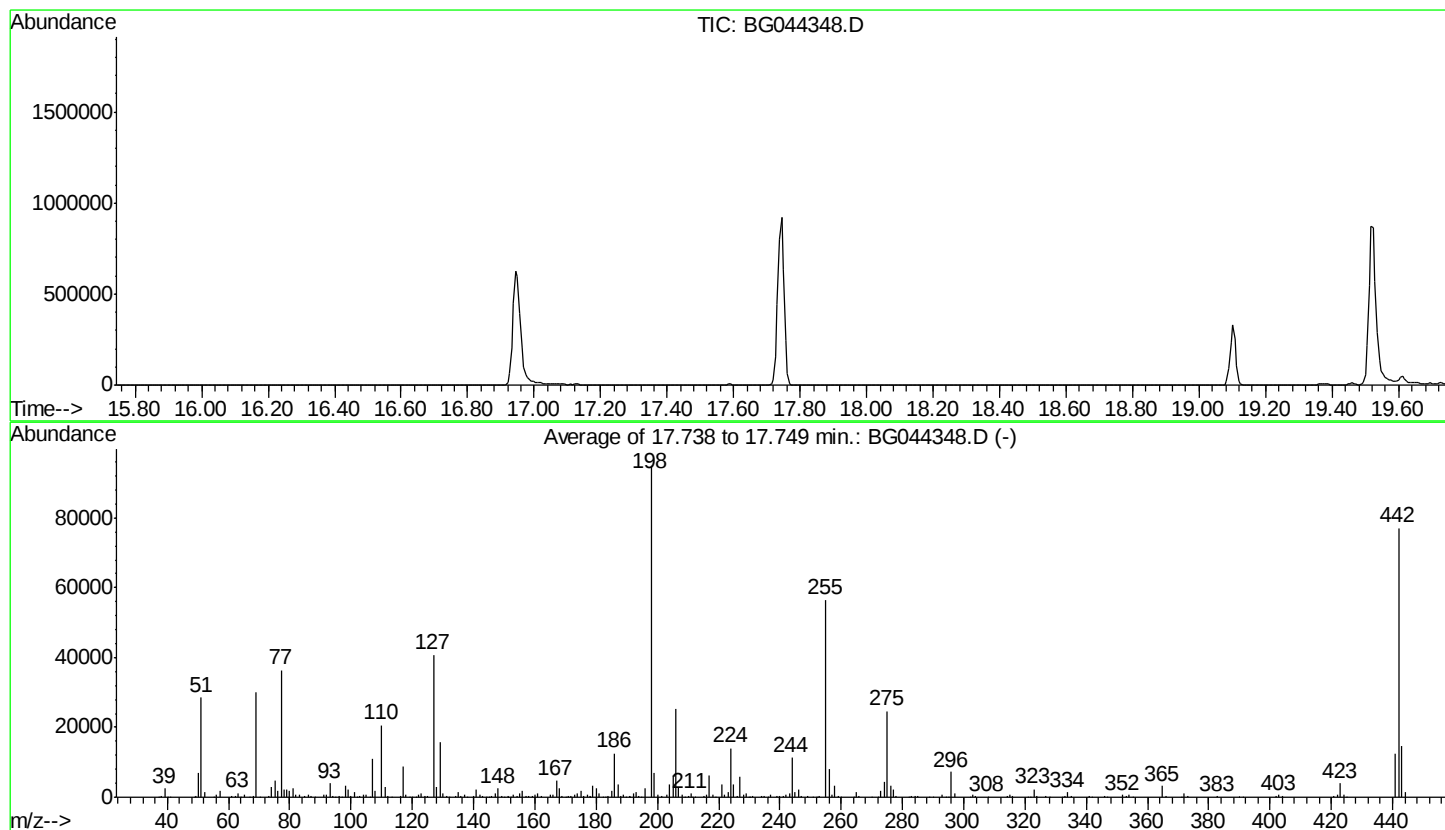

AutoFind: Scans 2493, 2494, 2495; Background Corrected with Scan 2486

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	30.0	28477	PASS
68	69	0.00	2	0.7	200	PASS
69	198	0.00	100	31.6	30050	PASS
70	69	0.00	2	0.5	156	PASS
127	198	10	80	42.9	40757	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	94976	PASS
199	198	5	9	7.4	7058	PASS
275	198	10	60	26.0	24680	PASS
365	198	1	100	3.4	3230	PASS
441	198	0.01	100	13.3	12589	PASS
442	198	50	100	81.2	77154	PASS
443	442	15	24	19.0	14652	PASS