
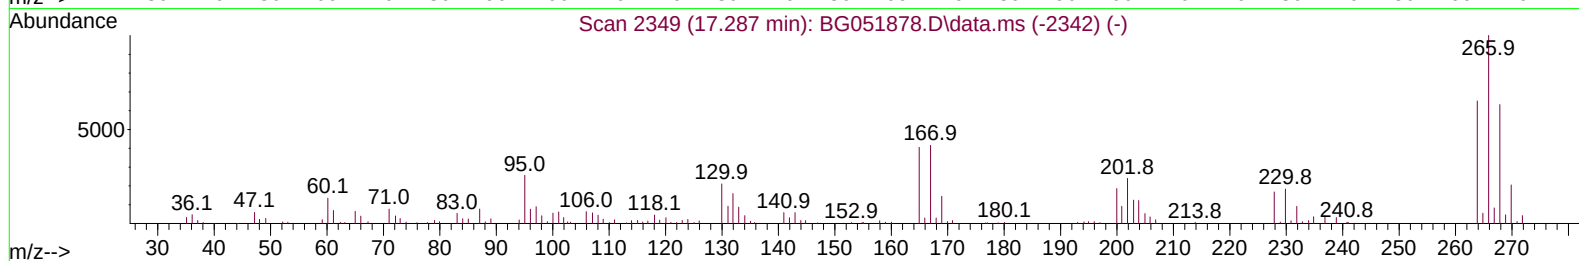
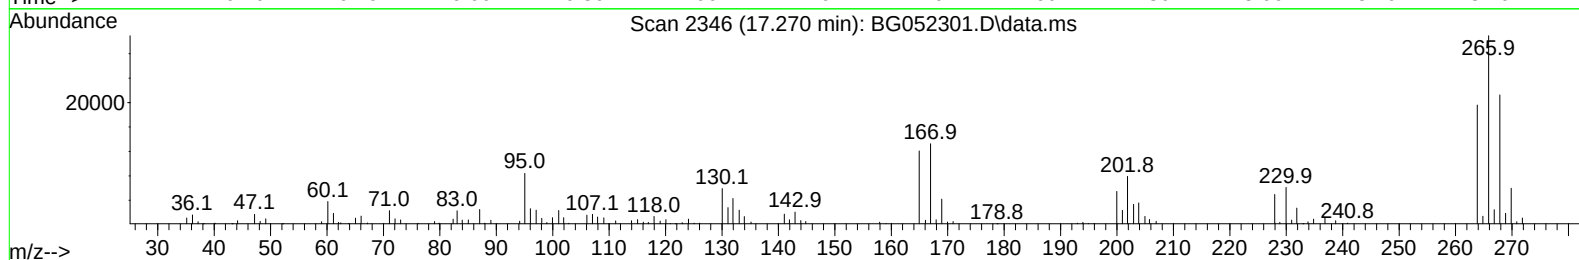


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG020722\
Data File : BG052301.D
Acq On : 7 Feb 2022 12:22
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Feb 07 13:03:38 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG020722.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Feb 07 13:03:27 2022
Response via : Initial Calibration

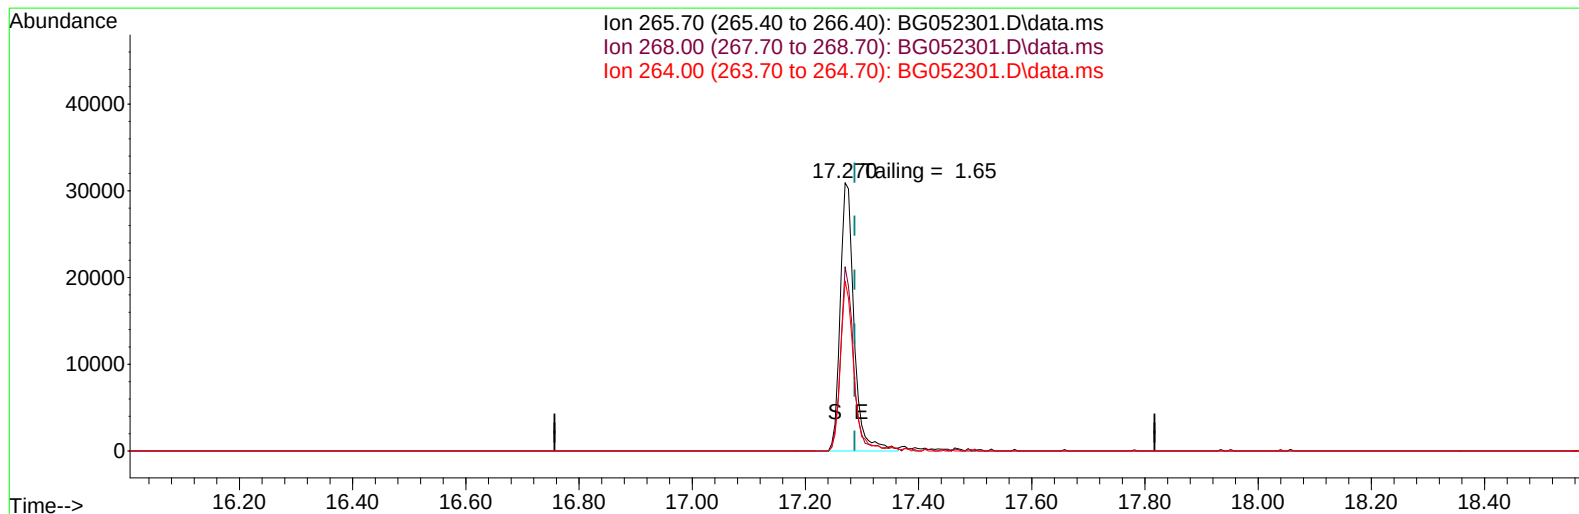

TIC: BG052301.D\data.ms

(70) Pentachlorophenol (C)




17.270min (-0.017) 100261.75 ng

response 52198

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.20	68.64
264.00	65.20	63.37
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG020722\
Data File : BG052301.D
Acq On : 7 Feb 2022 12:22
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Feb 07 13:03:38 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG020722.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Feb 07 13:03:27 2022
Response via : Initial Calibration

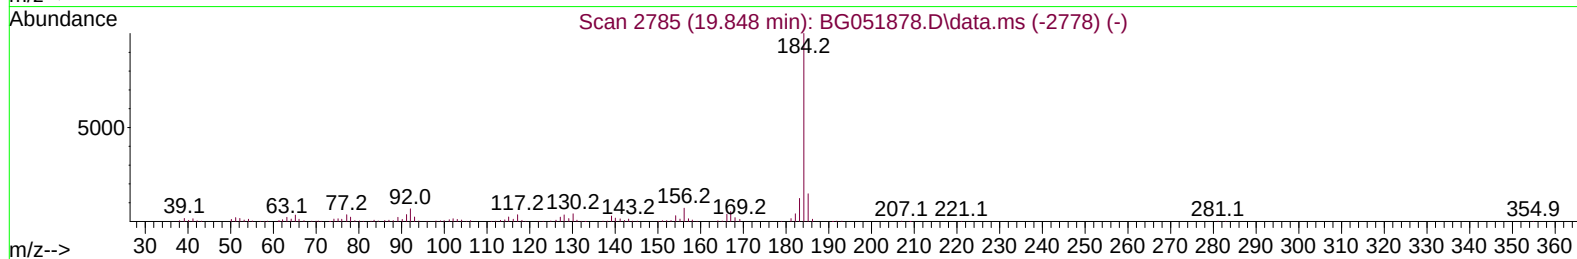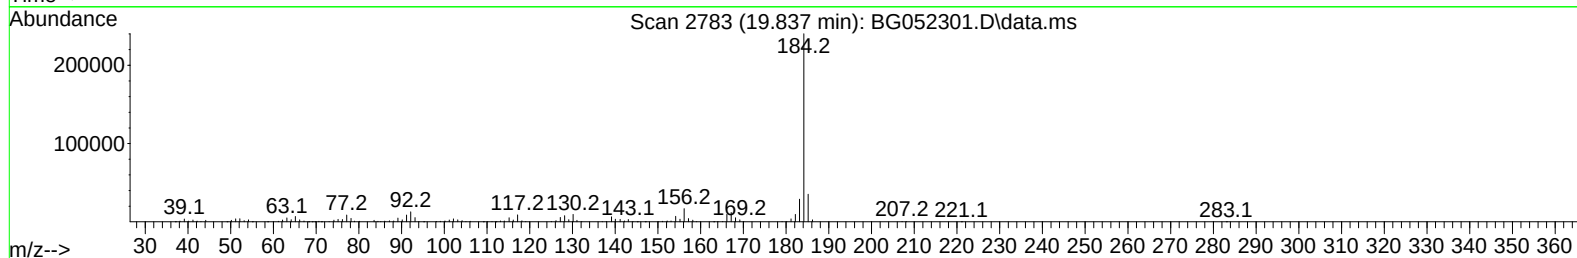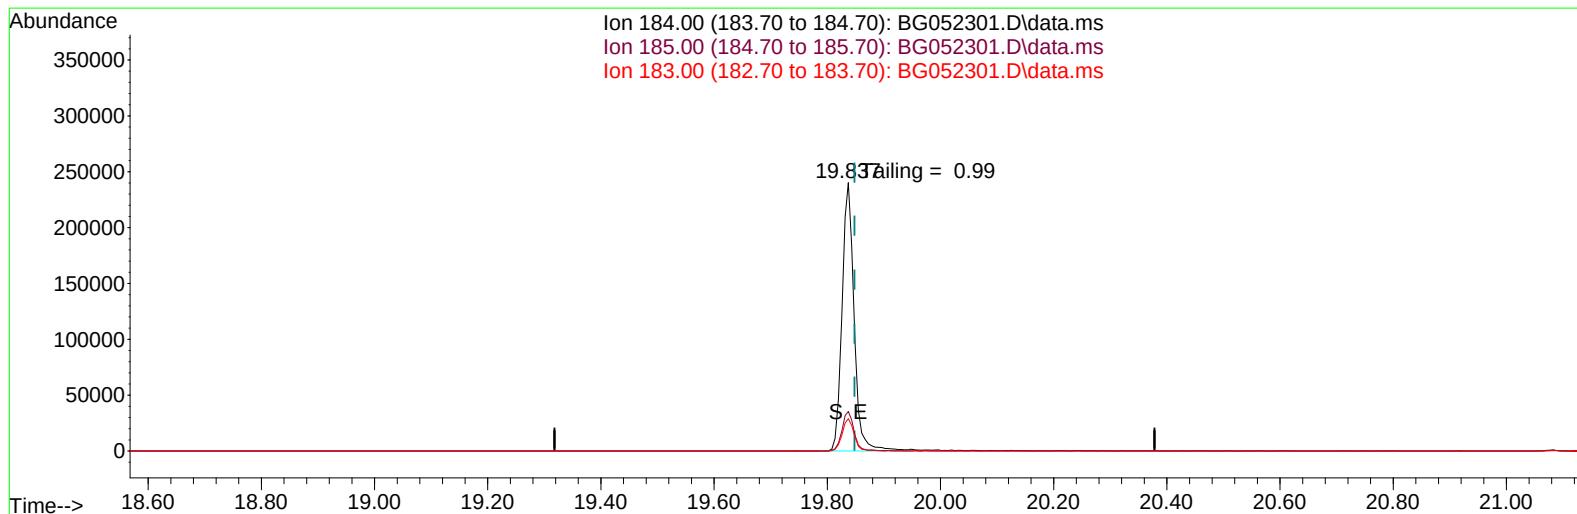

TIC: BG052301.D\data.ms

(77) Benzidine

19.837min (-0.011) 90830.01 ng

response 354337

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.80	14.72
183.00	12.20	12.06
0.00	0.00	0.00