


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG020722\
 Data File : BG052301.D
 Acq On : 7 Feb 2022 12:22
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG020722.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Feb 08 01:21:20 2022

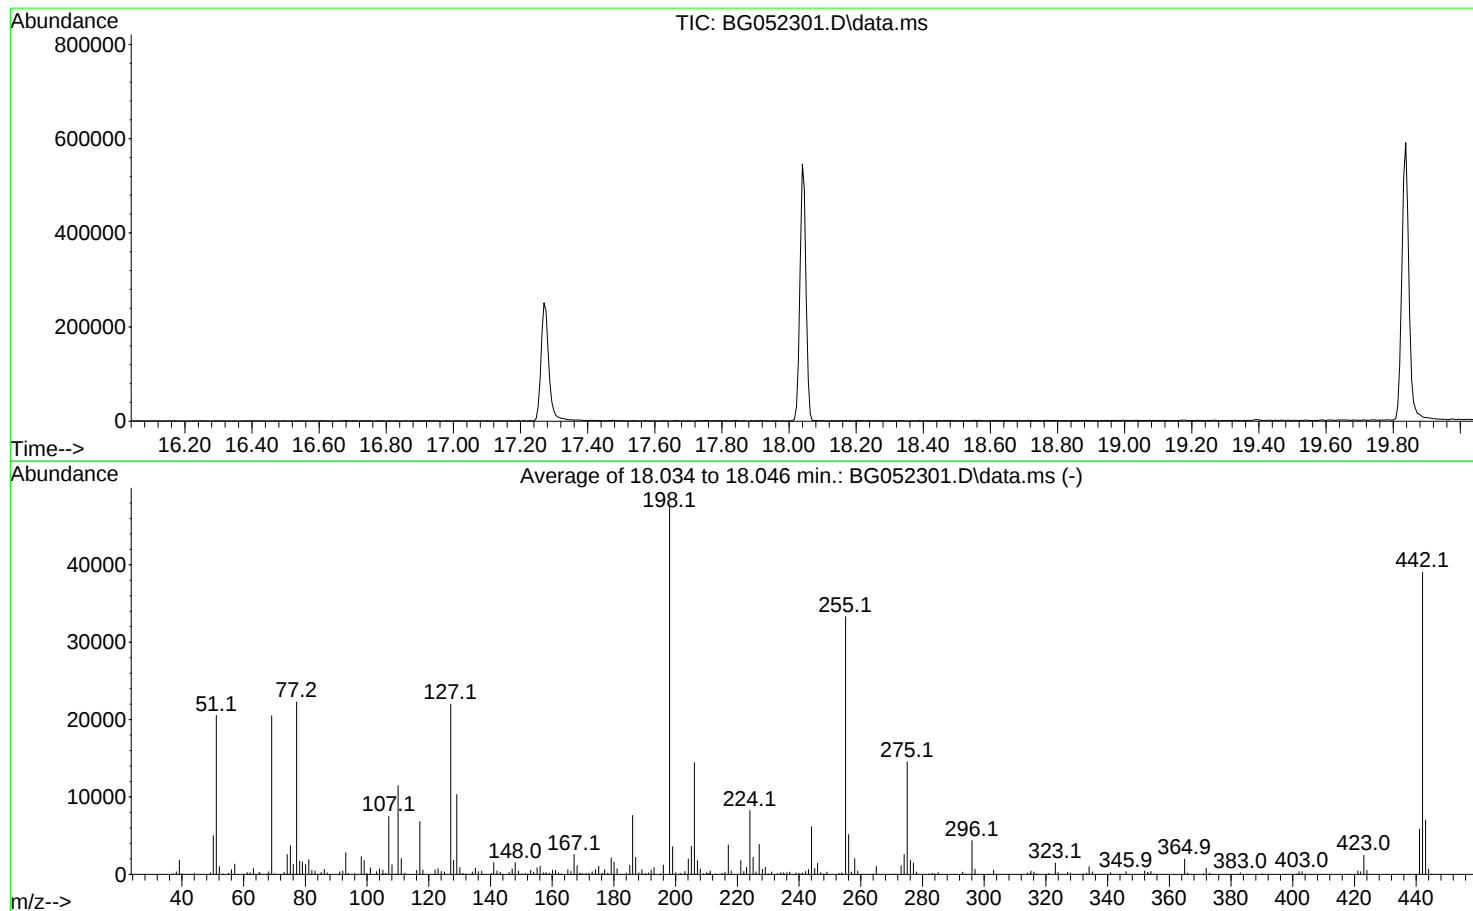

AutoFind: Scans 2476, 2477, 2478; Background Corrected with Scan 2470

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	43.2	20533	PASS
68	69	0.00	2	1.6	337	PASS
69	198	0.00	100	43.1	20501	PASS
70	69	0.00	2	0.3	57	PASS
127	198	10	80	46.3	22011	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	47536	PASS
199	198	5	9	7.5	3581	PASS
275	198	10	60	30.6	14545	PASS
365	198	1	100	4.1	1966	PASS
441	198	0.01	100	12.3	5854	PASS
442	442	50	100	100.0	39021	PASS
443	442	15	24	18.0	7015	PASS




DDT Breakdown

Date	Instrument Name	DFTPP Data File
2/7/2022	BNA_G	<u>BG052301.D</u>
Compound Name	Response	Retention Time
DDT	217963	21.08
DDD	637	20.62
DDE	53	20.44
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
690	218653	0.32

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG020722\
 Data File : BG052301.D
 Acq On : 7 Feb 2022 12:22
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Quant Time: Feb 07 13:03:38 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG020722.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Feb 07 13:03:27 2022
 Response via : Initial Calibration

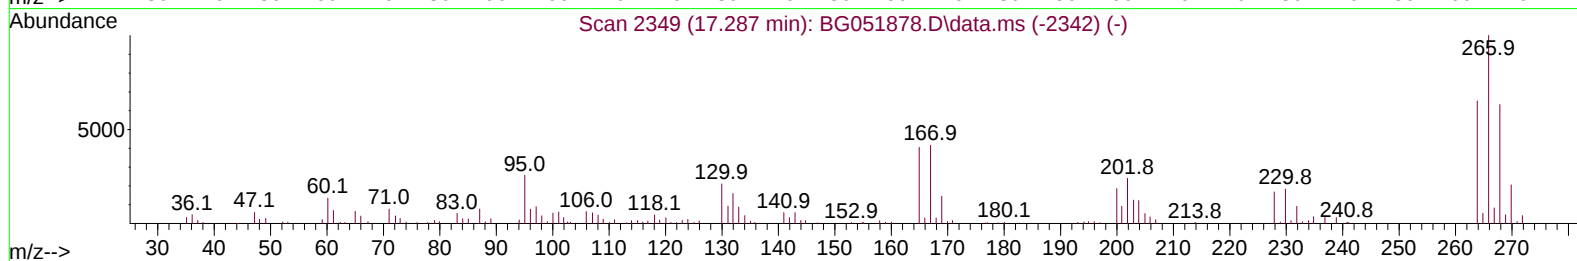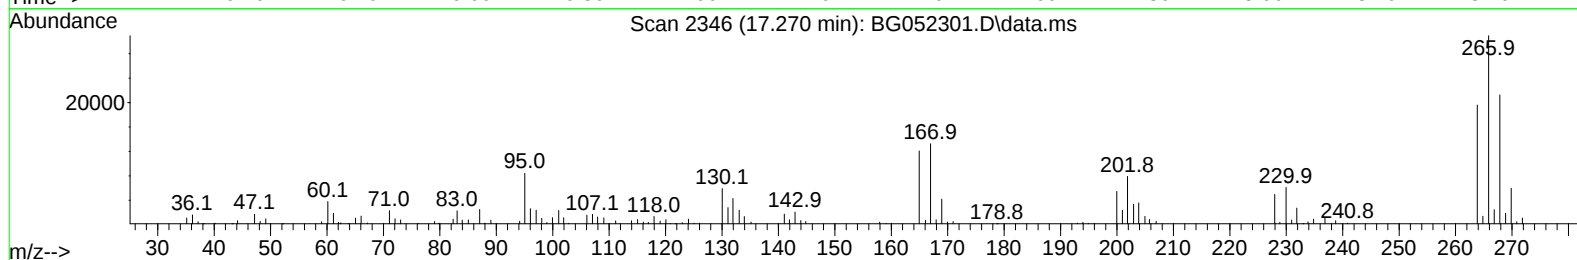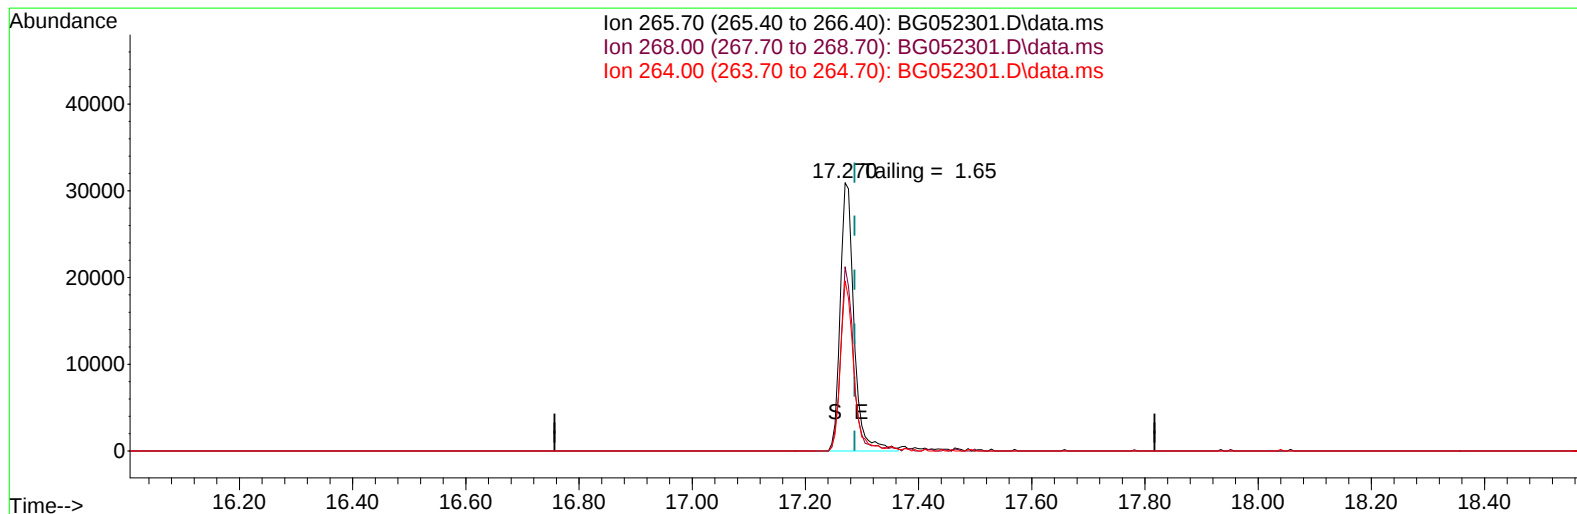

TIC: BG052301.D\data.ms

(70) Pentachlorophenol (C)

17.270min (-0.017) 100261.75 ng




response 52198

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.20	68.64
264.00	65.20	63.37
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG020722\
Data File : BG052301.D
Acq On : 7 Feb 2022 12:22
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: Feb 07 13:03:38 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG020722.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Feb 07 13:03:27 2022
Response via : Initial Calibration

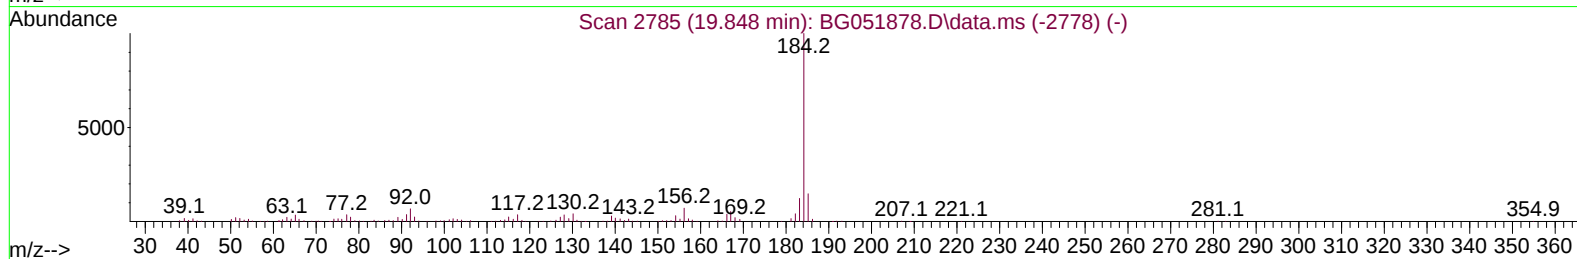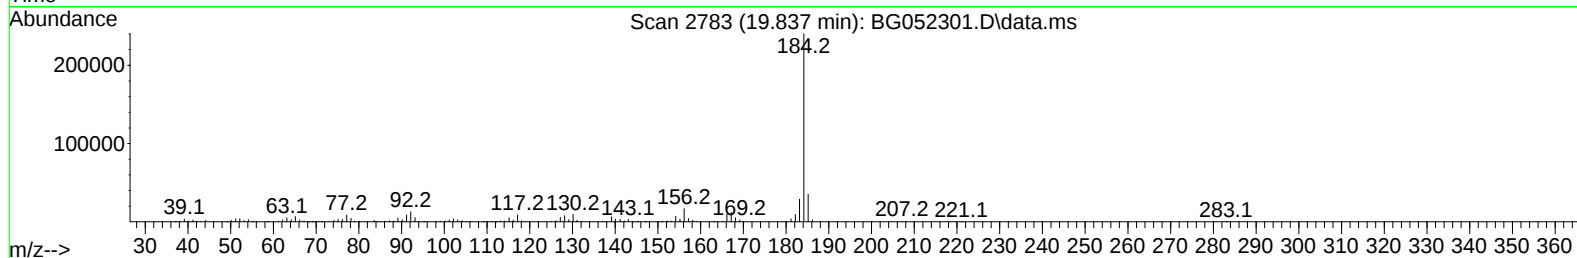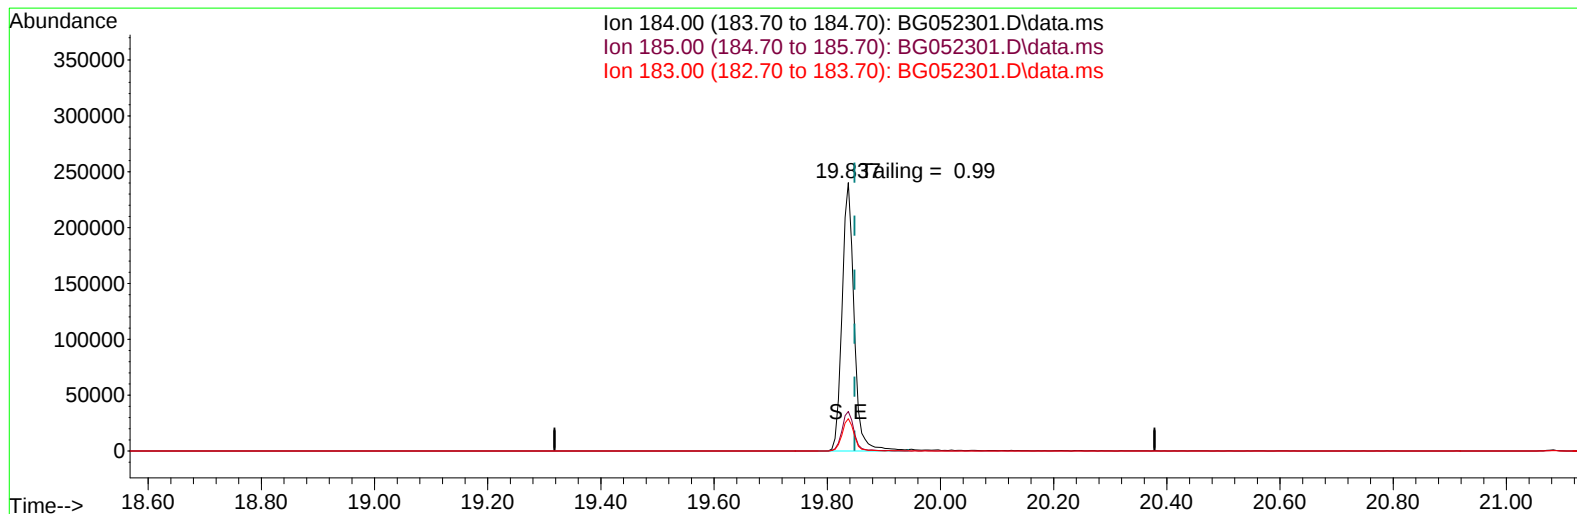

TIC: BG052301.D\data.ms

(77) Benzidine

19.837min (-0.011) 90830.01 ng

response 354337

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.80	14.72
183.00	12.20	12.06
0.00	0.00	0.00