

Data Path : Z:\SVOASRV\HPCHEM1\BNA_G\DATA\BG020819\
 Data File : BG039418.D
 Acq On : 8 Feb 2019 16:39
 Operator : JU/SJ
 Sample : K1404-02
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 A0C12-SS1-7.5-8.0

Quant Time: Feb 08 23:34:24 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG012919.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Jan 29 15:41:51 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.18	152	57222	20.00	ng	0.00
21) Naphthalene-d8	11.00	136	256444	20.00	ng	-0.01
39) Acenaphthene-d10	14.80	164	173437	20.00	ng	-0.01
64) Phenanthrene-d10	17.54	188	420336	20.00	ng	-0.01
76) Chrysene-d12	21.83	240	450302	20.00	ng	-0.02
87) Perylene-d12	25.21	264	458437	20.00	ng	-0.03

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
5) 2-Fluorophenol	5.72	112	529663	158.42	ng	0.00
7) Phenol-d6	7.31	99	765296	155.51	ng	0.00
23) Nitrobenzene-d5	9.35	82	455863	111.05	ng	-0.01
42) 2,4,6-Tribromophenol	16.28	330	292881	156.82	ng	0.00
45) 2-Fluorobiphenyl	13.42	172	974011	80.56	ng	-0.01
79) Terphenyl-d14	20.14	244	1540039	72.39	ng	-0.01


Target Compounds	R.T.	QIon	Response	Conc	Units	Qvalue
9) Benzaldehyde	7.32	77	1814	Below Cal		# 4
10) Phenol	7.34	94	51364	10.012	ng	95
19) n-Nitroso-di-n-propylamine	9.35	70	58018	16.610	ng	# 69
32) Benzoic acid	10.60	122	54	9.039	ng	# 1
48) 2-Nitroaniline	13.89	65	80	8.318	ng	# 10
50) Dimethylphthalate	14.24	163	114476	8.173	ng	99
51) 2,6-Dinitrotoluene	14.23	165	1058	6.908	ng	# 1
53) 3-Nitroaniline	15.00	138	55	5.810	ng	# 1
57) 2,4-Dinitrotoluene	14.80	165	23584	13.712	ng	# 19
65) 4,6-Dinitro-2-methylphenol	16.29	198	1157	5.057	ng	# 38
67) 4-Bromophenyl-phenylether	16.28	248	23057	4.945	ng	# 1

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA_G\DATA\BG020819\
Data File : BG039418.D
Acq On : 8 Feb 2019 16:39
Operator : JU/SJ
Sample : K1404-02
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
A0C12-SS1-7.5-8.0

Quant Time: Feb 08 23:34:24 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG012919.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jan 29 15:41:51 2019
Response via : Initial Calibration

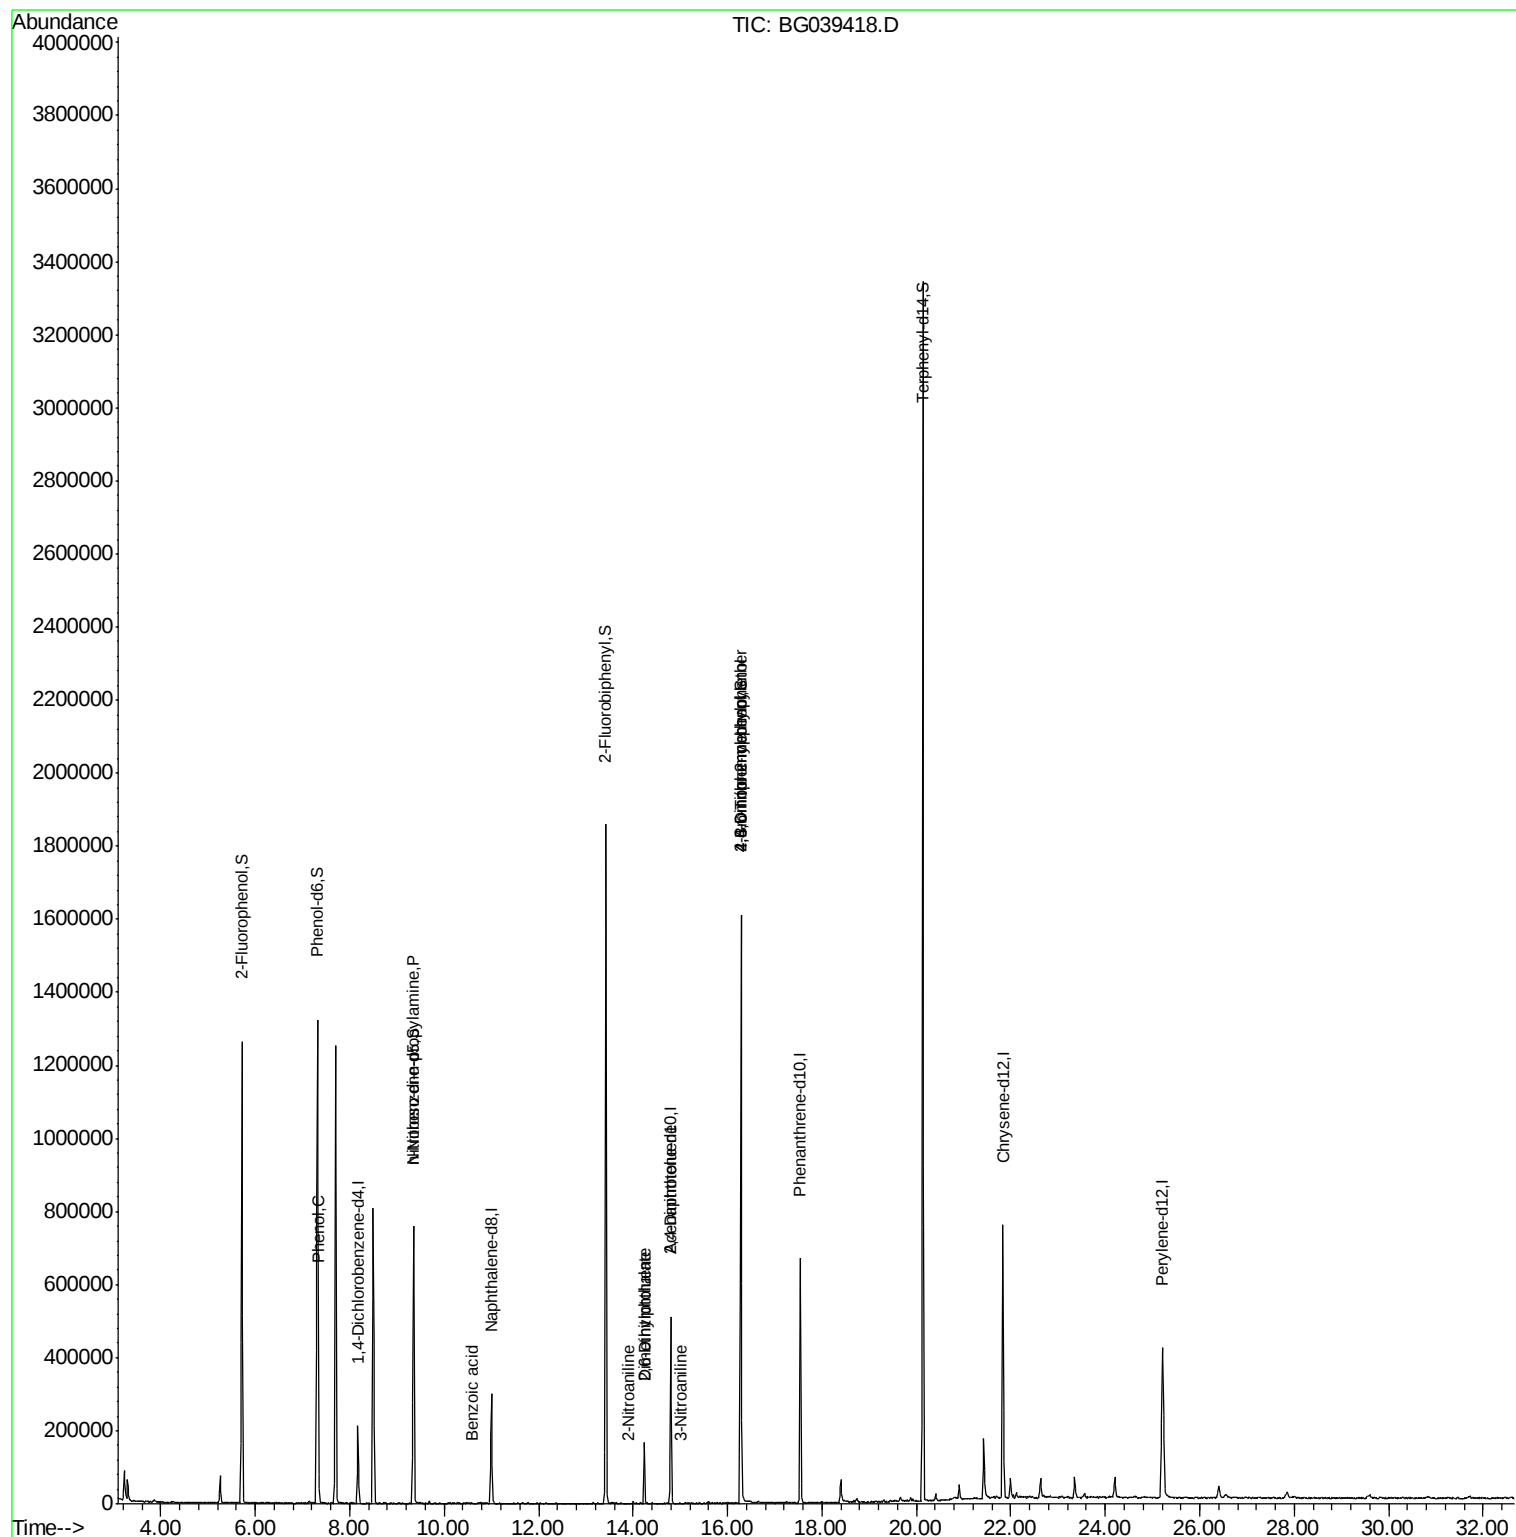




#1



1,4-Dichlorobenzene-d4
 Concen: 20.000 ng
 RT: 8.18 min Scan# 866
 Delta R.T. -0.01 min
 Lab File: BG039418.D
 Acq: 8 Feb 2019 16:39

Instrument :
 BNA_G
 ClientSampleId :
 A0C12-SS1-7.5-8.0

Tgt Ion:152 Resp: 57222
 Ion Ratio Lower Upper
 152 100
 150 158.2 123.7 185.5
 115 64.3 45.9 68.9




Abundance Ion 152.00 (151.70 to 152.70): E
 Ion 150.00 (149.70 to 150.70): E
 Ion 115.00 (114.70 to 115.70): E

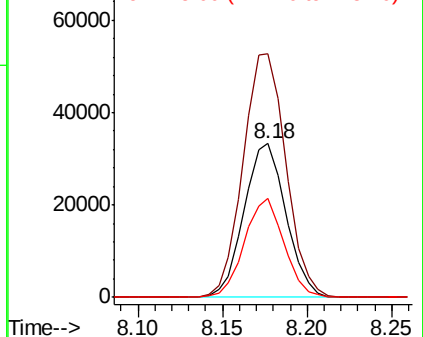



#5

2-Fluorophenol
 Concen: 158.422 ng
 RT: 5.72 min Scan# 447
 Delta R.T. -0.00 min
 Lab File: BG039418.D
 Acq: 8 Feb 2019 16:39

Tgt Ion:112 Resp: 529663
 Ion Ratio Lower Upper
 112 100
 64 68.4 57.8 86.8
 63 36.6 29.8 44.6



Abundance Ion 112.00 (111.70 to 112.70): E
 Ion 64.00 (63.70 to 64.70): BGC
 Ion 63.00 (62.70 to 63.70): BGC

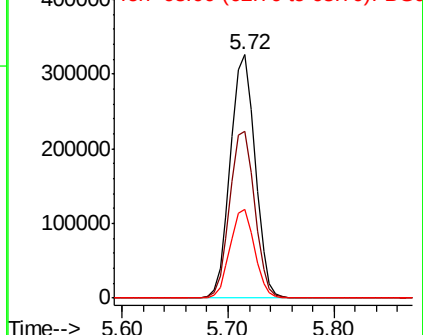



#7

Phenol-d6

Concen: 155.506 ng

RT: 7.31 min Scan# 719

Delta R.T. -0.01 min

Lab File: BG039418.D

Acq: 8 Feb 2019 16:39

Instrument :

BNA_G

ClientSampleId :

A0C12-SS1-7.5-8.0


Tgt Ion: 99 Resp: 765296

Ion Ratio Lower Upper




99 100

42 21.4 18.2 27.2

71 36.6 28.0 42.0

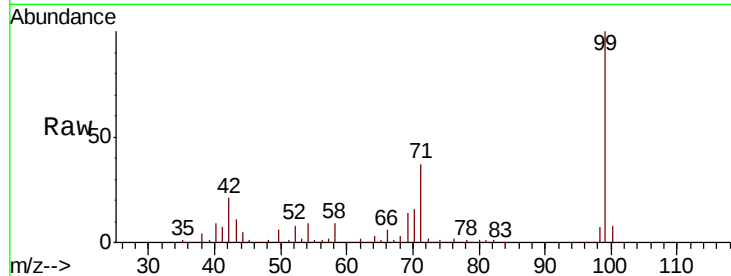

Abundance Ion 99.00 (98.70 to 99.70): BGC
Ion 42.00 (41.70 to 42.70): BGC
Ion 71.00 (70.70 to 71.70): BGC

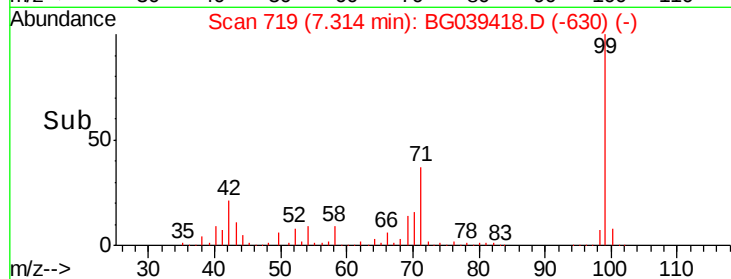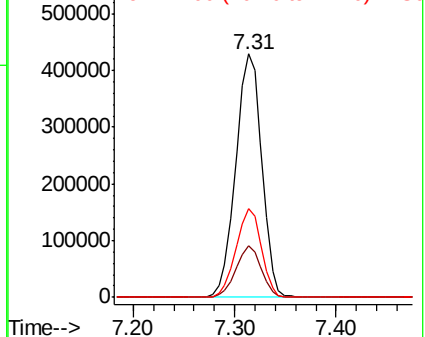

#10

Phenol

Concen: 10.012 ng

RT: 7.34 min Scan# 723

Delta R.T. -0.01 min

Lab File: BG039418.D

Acq: 8 Feb 2019 16:39


Tgt Ion: 94 Resp: 51364

Ion Ratio Lower Upper



94 100


65 31.3 11.7 51.7

66 48.7 23.7 63.7



Abundance Ion 94.00 (93.70 to 94.70): BGC
Ion 65.00 (64.70 to 65.70): BGC
Ion 66.00 (65.70 to 66.70): BGC



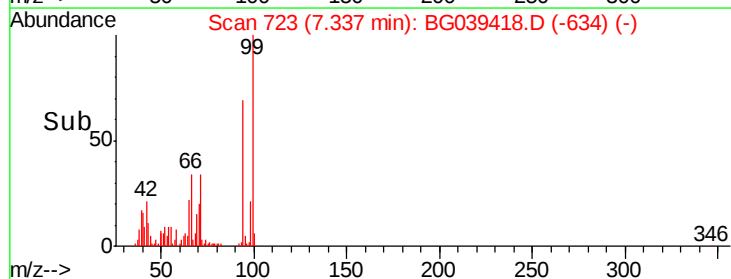
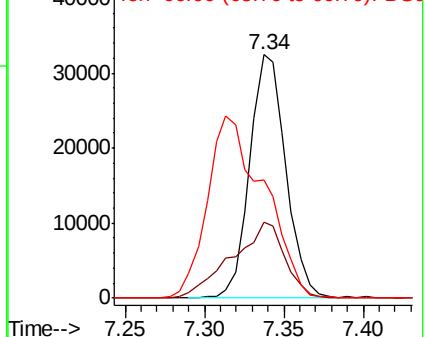




#19
n-Nitroso-di-n-propylamine
Concen: 16.610 ng
RT: 9.35 min Scan# 1066
Delta R.T. 0.36 min
Lab File: BG039418.D
Acq: 8 Feb 2019 16:39




Instrument :
BNA_G
ClientSampleId :
A0C12-SS1-7.5-8.0

Tgt Ion: 70 Resp: 58018
Ion Ratio Lower Upper
70 100
42 50.2 60.4 90.6#
101 0.0 7.5 11.3#
130 2.1 16.9 25.3#

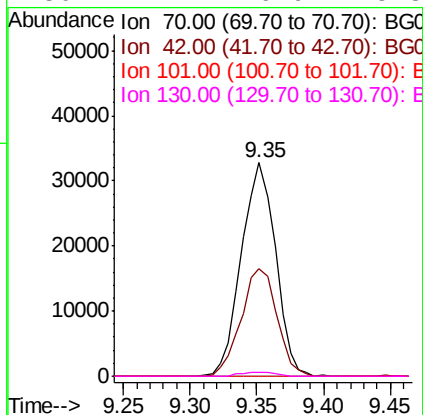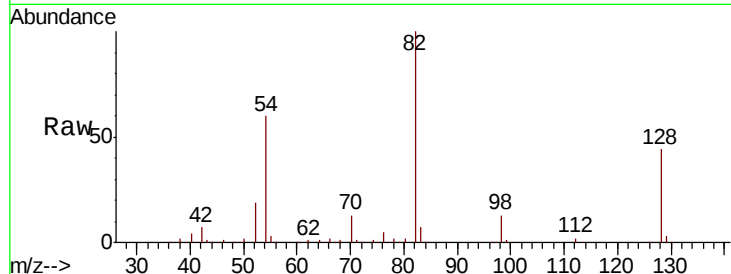

#21
Naphthalene-d8
Concen: 20.000 ng
RT: 11.00 min Scan# 1346
Delta R.T. -0.01 min
Lab File: BG039418.D
Acq: 8 Feb 2019 16:39

Tgt Ion: 136 Resp: 256444
Ion Ratio Lower Upper
136 100
137 11.8 9.1 13.7
54 10.7 9.4 14.2
68 6.2 4.2 6.4


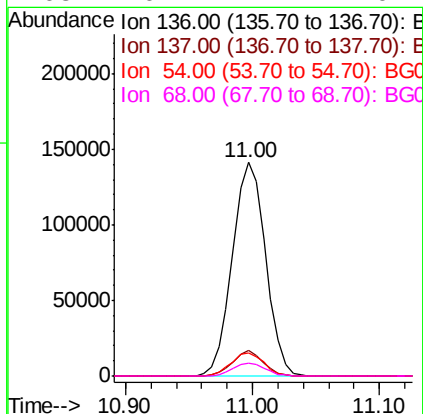

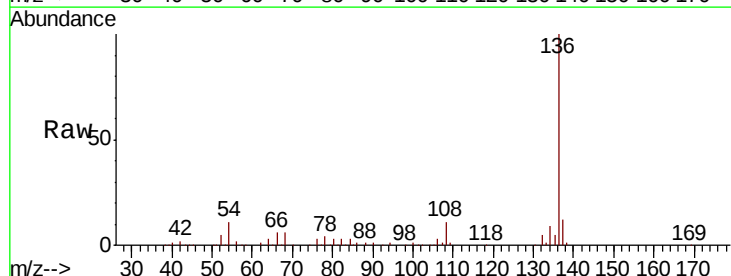




#23
 Nitrobenzene-d5
 Concen: 111.051 ng
 RT: 9.35 min Scan# 1066
 Delta R.T. -0.01 min
 Lab File: BG039418.D
 Acq: 8 Feb 2019 16:39




Instrument :
 BNA_G
 ClientSampleId :
 A0C12-SS1-7.5-8.0


Tgt Ion	Ratio	Lower	Upper
82	100		
128	44.0	31.3	46.9
54	60.4	50.9	76.3

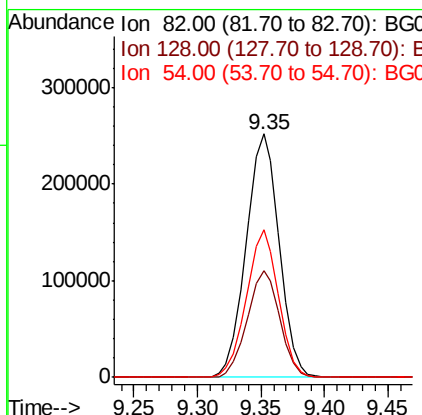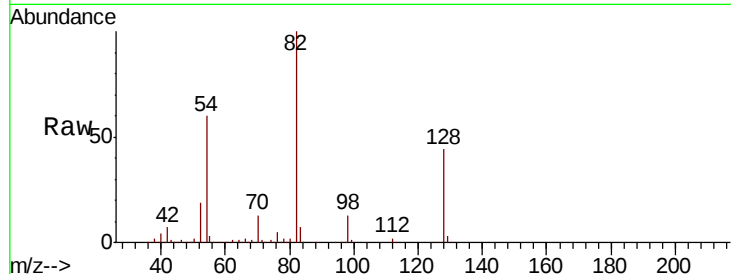

#32
 Benzoic acid
 Concen: 9.039 ng
 RT: 10.60 min Scan# 1279
 Delta R.T. 0.34 min
 Lab File: BG039418.D
 Acq: 8 Feb 2019 16:39

Tgt Ion	Ratio	Lower	Upper
122	100		
105	0.0	101.8	141.8#
77	0.0	76.3	116.3#

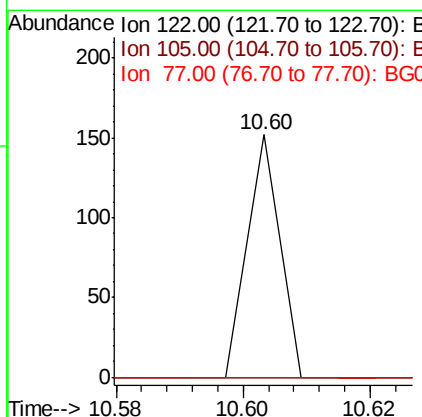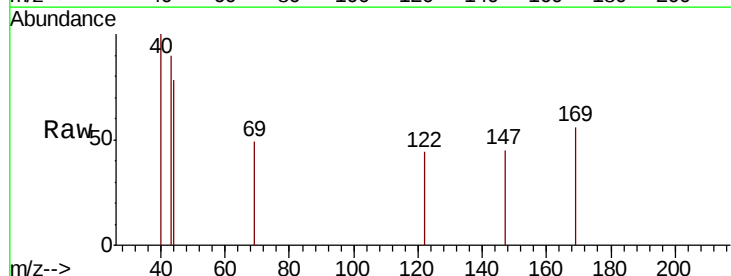

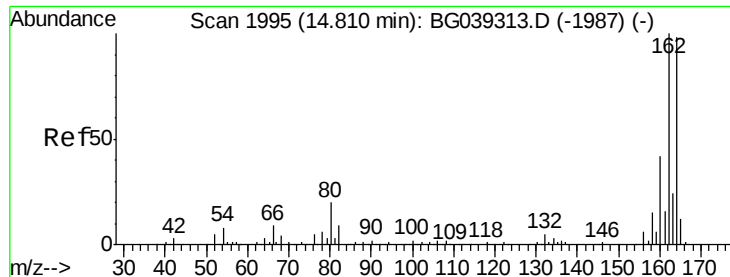

#39

Acenaphthene-d10

Concen: 20.000 ng

RT: 14.80 min Scan# 1993

Delta R.T. -0.01 min

Lab File: BG039418.D

Acq: 8 Feb 2019 16:39

Instrument :

BNA_G

ClientSampleId :

A0C12-SS1-7.5-8.0


Tgt Ion:164 Resp: 173437

Ion Ratio Lower Upper

164 100

162 101.3 81.6 122.4




160 43.5 34.2 51.2

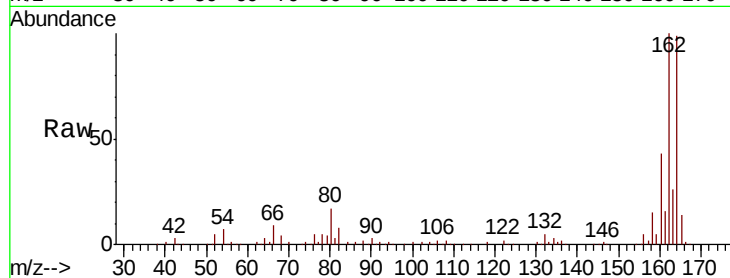

Abundance Ion 164.00 (163.70 to 164.70): E

Ion 162.00 (161.70 to 162.70): E

Ion 160.00 (159.70 to 160.70): E

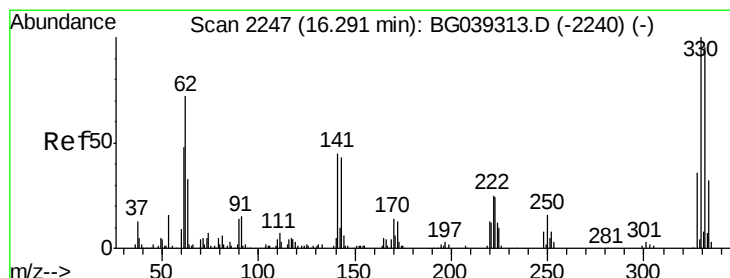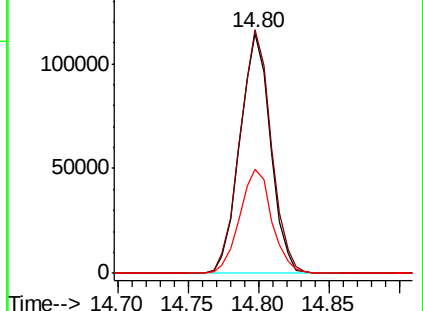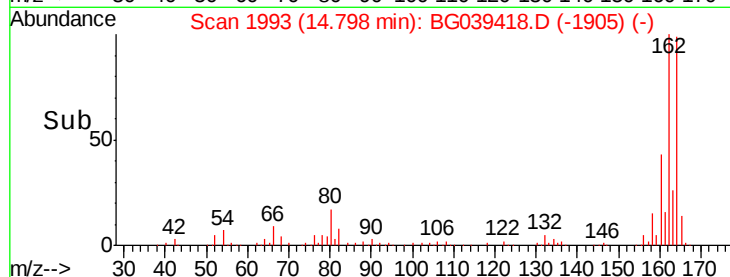

#42

2,4,6-Tribromophenol

Concen: 156.820 ng

RT: 16.28 min Scan# 2246

Delta R.T. -0.01 min

Lab File: BG039418.D

Acq: 8 Feb 2019 16:39


Tgt Ion:330 Resp: 292881

Ion Ratio Lower Upper

330 100

332 96.2 75.7 113.5



141 40.0 35.6 53.4

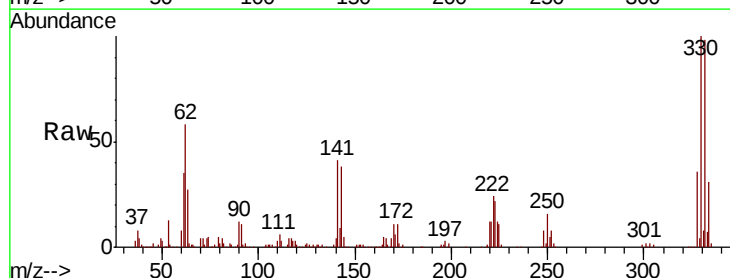


Abundance Ion 329.80 (329.50 to 330.50): E

Ion 331.80 (331.50 to 332.50): E

Ion 141.00 (140.70 to 141.70): E



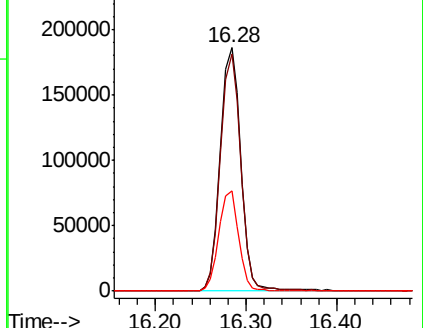
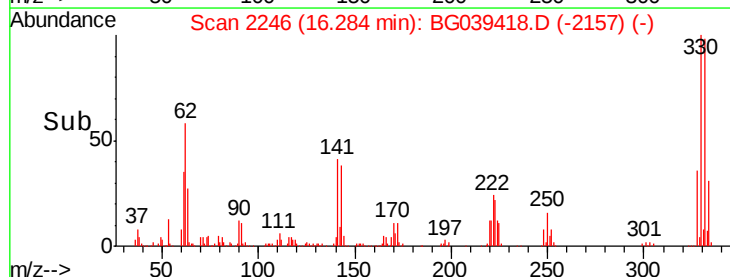


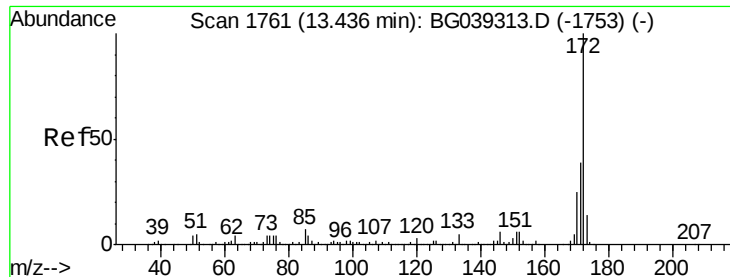

#45
 2-Fluorobiphenyl
 Concen: 80.563 ng
 RT: 13.42 min Scan# 1759
 Delta R.T. -0.01 min
 Lab File: BG039418.D
 Acq: 8 Feb 2019 16:39




Instrument :
 BNA_G
 ClientSampleId :
 A0C12-SS1-7.5-8.0


Tgt Ion: 172 Resp: 974011
 Ion Ratio Lower Upper
 172 100
 171 37.6 30.8 46.2
 170 24.7 20.2 30.4

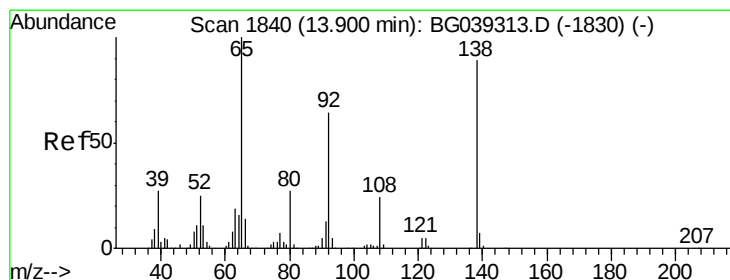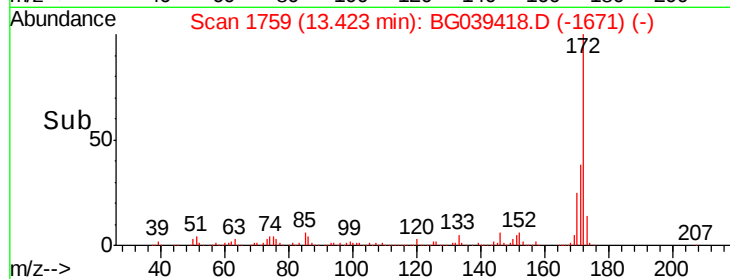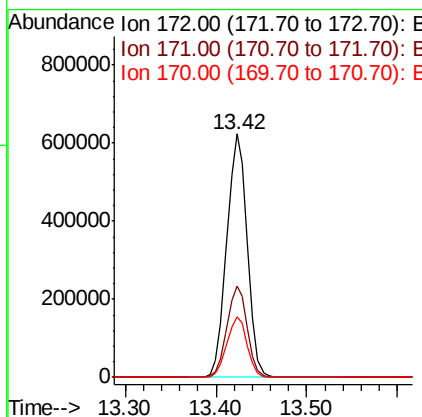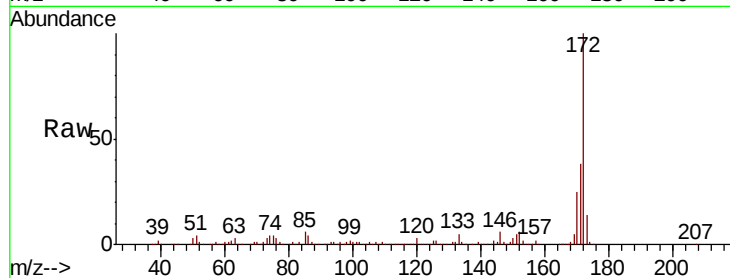

#48
 2-Nitroaniline
 Concen: 8.318 ng
 RT: 13.89 min Scan# 1838
 Delta R.T. -0.01 min
 Lab File: BG039418.D
 Acq: 8 Feb 2019 16:39

Tgt Ion: 65 Resp: 80
 Ion Ratio Lower Upper
 65 100
 92 0.0 51.4 77.2#
 138 0.0 71.4 107.2#

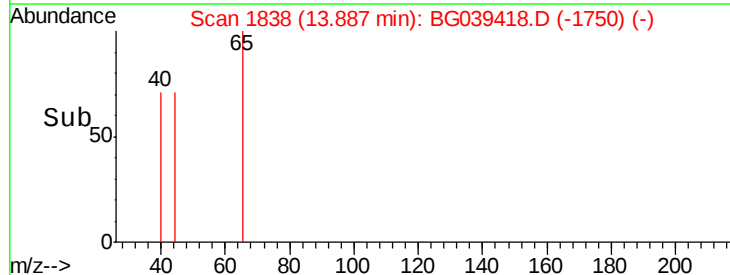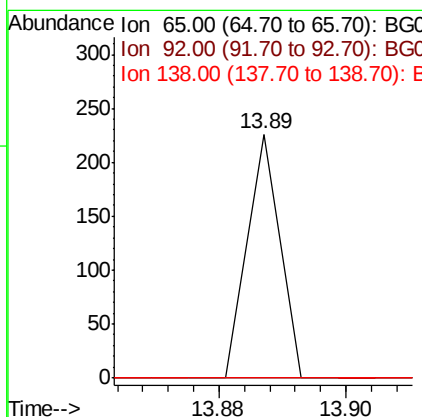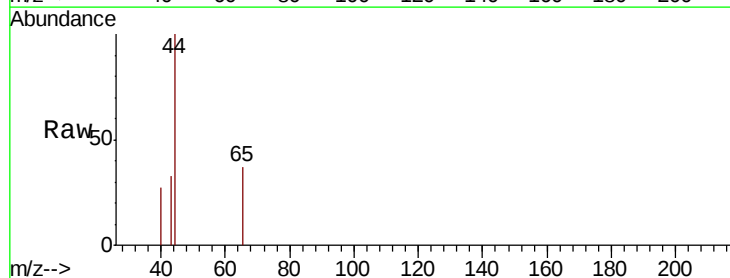

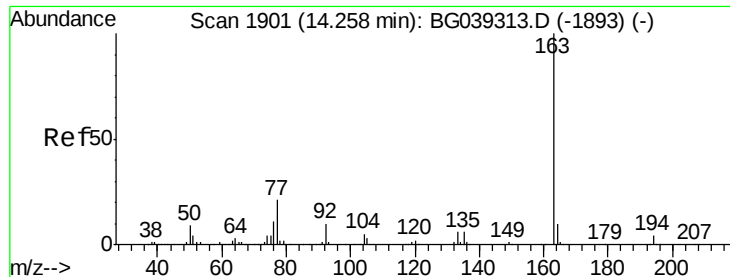

#50

Dimethylphthalate

Concen: 8.173 ng

RT: 14.24 min Scan# 1898

Delta R.T. -0.02 min

Lab File: BG039418.D

Acq: 8 Feb 2019 16:39

Instrument :

BNA_G

ClientSampleId :

A0C12-SS1-7.5-8.0


Tgt Ion:163 Resp: 114476

Ion Ratio Lower Upper

163 100

194 4.0 3.6 5.4




164 10.4 8.4 12.6

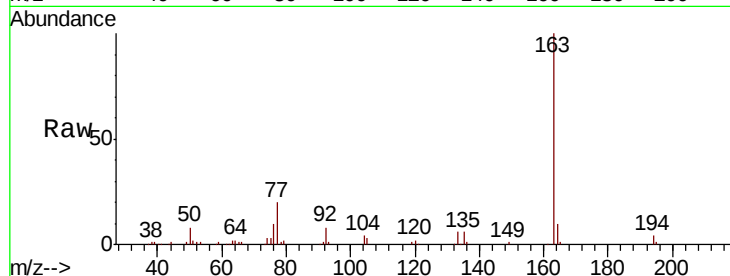

Abundance Ion 163.00 (162.70 to 163.70): E

Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

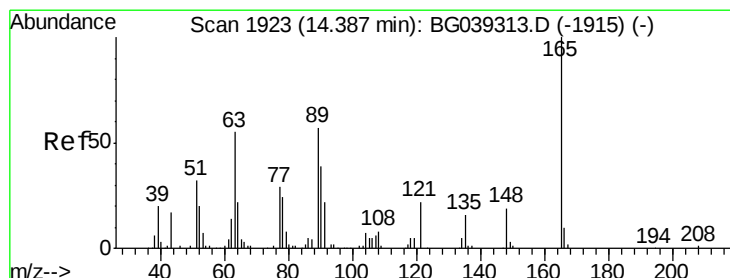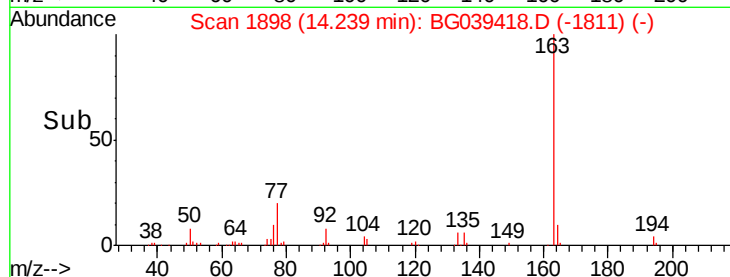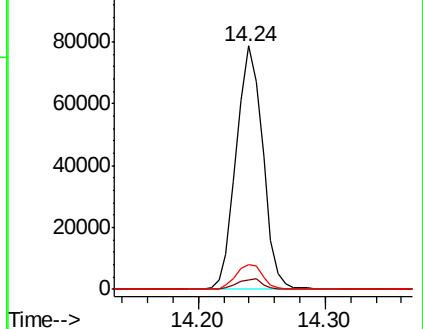

#51

2,6-Dinitrotoluene

Concen: 6.908 ng

RT: 14.23 min Scan# 1897

Delta R.T. -0.15 min

Lab File: BG039418.D

Acq: 8 Feb 2019 16:39


Tgt Ion:165 Resp: 1058

Ion Ratio Lower Upper

165 100

63 155.2 47.0 70.6#



89 0.0 45.8 68.8#

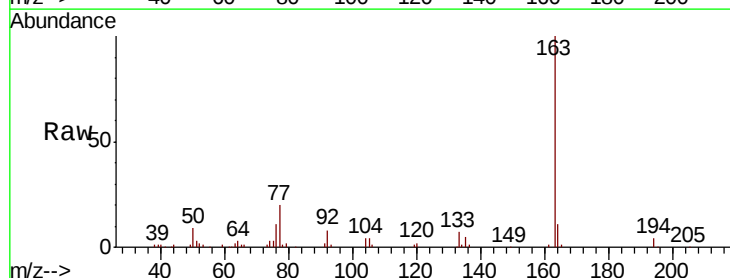


Abundance Ion 165.00 (164.70 to 165.70): E

Ion 63.00 (62.70 to 63.70): BGC

Ion 89.00 (88.70 to 89.70): BGC

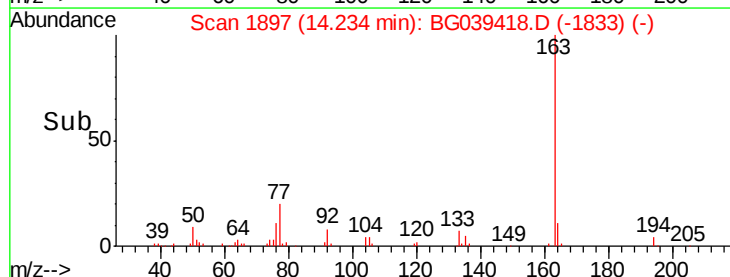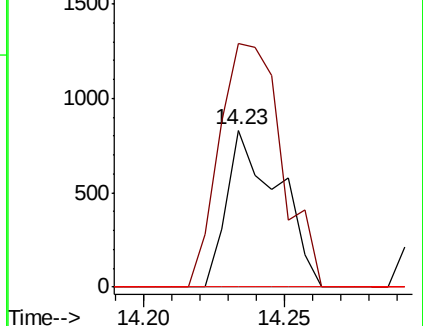

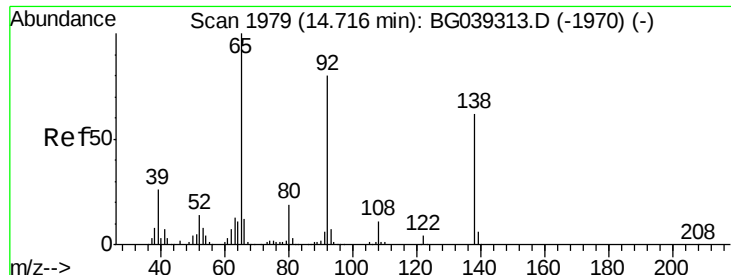

#53

3-Nitroaniline

Concen: 5.810 ng

RT: 15.00 min Scan# 2027

Delta R.T. 0.28 min

Lab File: BG039418.D

Acq: 8 Feb 2019 16:39

Instrument :

BNA_G

ClientSampleId :

A0C12-SS1-7.5-8.0





Tgt Ion:138 Resp: 55

Ion Ratio Lower Upper

138 100

108 0.0 13.8 20.8#

92 0.0 103.7 155.5#

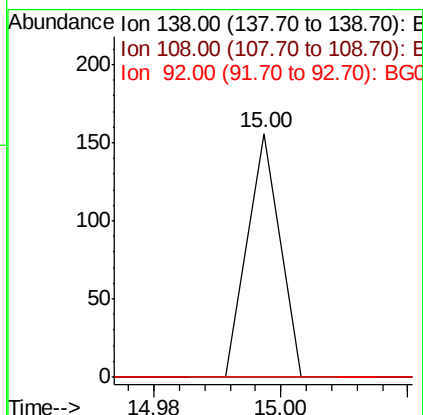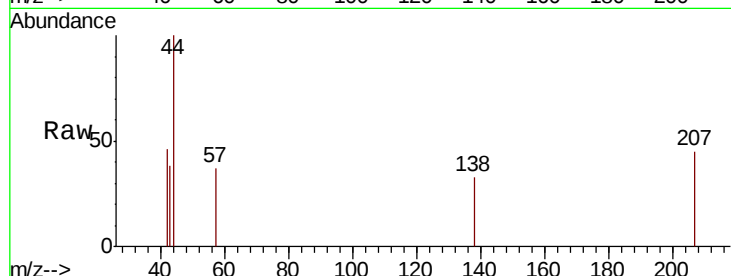

#57

2,4-Dinitrotoluene

Concen: 13.712 ng

RT: 14.80 min Scan# 1993

Delta R.T. -0.36 min

Lab File: BG039418.D

Acq: 8 Feb 2019 16:39

Tgt Ion:165 Resp: 23584




Ion Ratio Lower Upper


165 100

63 1.5 41.0 61.6#

89 1.9 64.6 96.8#

182 0.0 2.0 3.0#

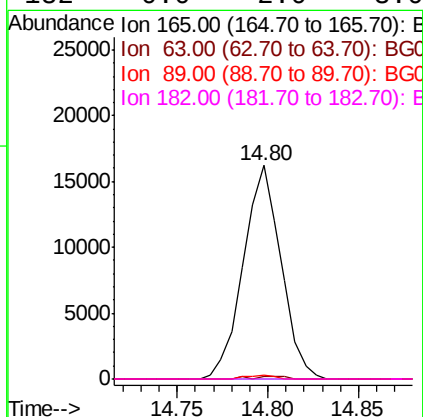



#64

Phenanthrene-d10

Concen: 20.000 ng

RT: 17.54 min Scan# 2460

Delta R.T. -0.01 min

Lab File: BG039418.D

Acq: 8 Feb 2019 16:39

Instrument :

BNA_G

ClientSampleId :

A0C12-SS1-7.5-8.0


Tgt Ion:188 Resp: 420336

Ion Ratio Lower Upper

188 100

94 8.2 6.9 10.3




80 8.8 8.1 12.1

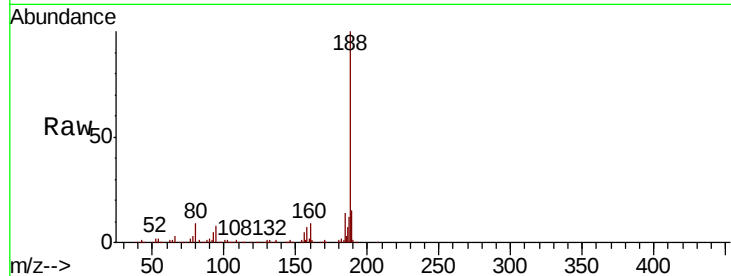

Abundance Ion 188.00 (187.70 to 188.70): E

Ion 94.00 (93.70 to 94.70): BG

Ion 80.00 (79.70 to 80.70): BG

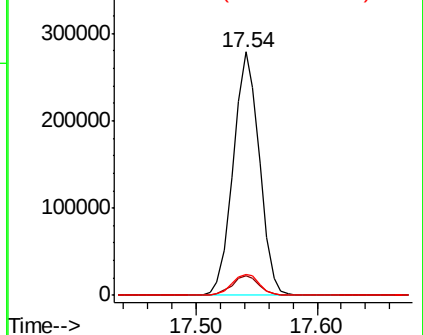

#65

4,6-Dinitro-2-methylphenol

Concen: 5.057 ng

RT: 16.29 min Scan# 2247

Delta R.T. 0.37 min

Lab File: BG039418.D

Acq: 8 Feb 2019 16:39


Tgt Ion:198 Resp: 1157

Ion Ratio Lower Upper

198 100

51 95.5 27.4 67.4#



105 70.7 19.7 59.7#

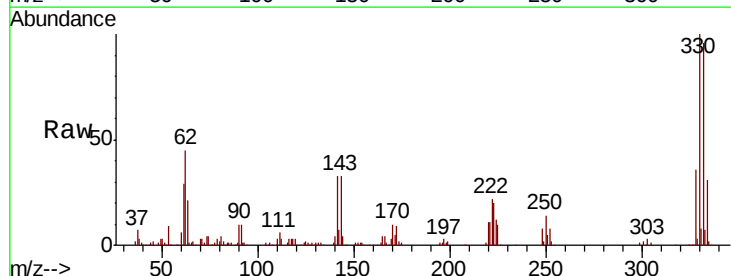


Abundance Ion 198.00 (197.70 to 198.70): E

Ion 51.00 (50.70 to 51.70): BG

Ion 105.00 (104.70 to 105.70): E

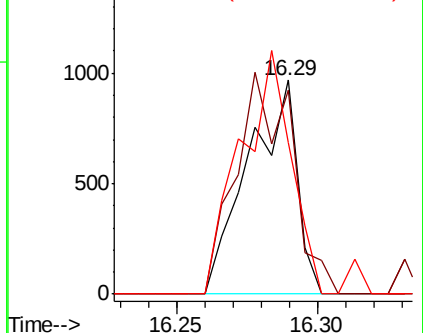


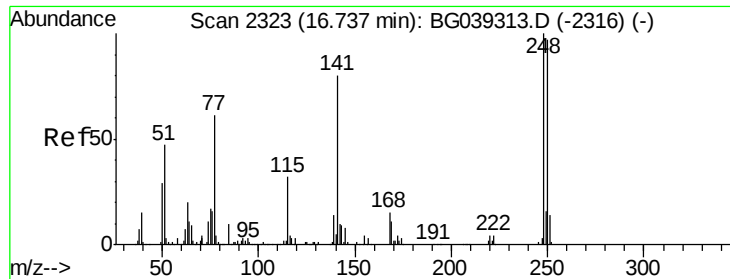




#67
4-Bromophenyl-phenylether
Concen: 4.945 ng
RT: 16.28 min Scan# 2246
Delta R.T. -0.45 min
Lab File: BG039418.D
Acq: 8 Feb 2019 16:39

Instrument :
BNA_G
ClientSampleId :
A0C12-SS1-7.5-8.0

Tgt Ion:248 Resp: 23057
Ion Ratio Lower Upper
248 100
250 198.6 77.6 116.4#
141 513.4 63.9 95.9#

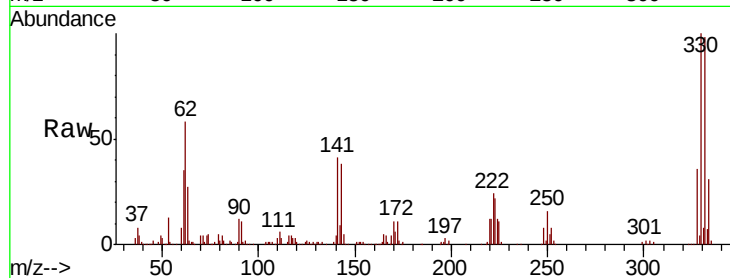


Abundance Ion 248.00 (247.70 to 248.70): E
Ion 250.00 (249.70 to 250.70): E
Ion 141.00 (140.70 to 141.70): E

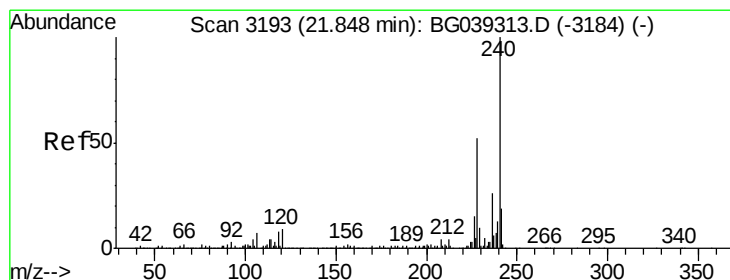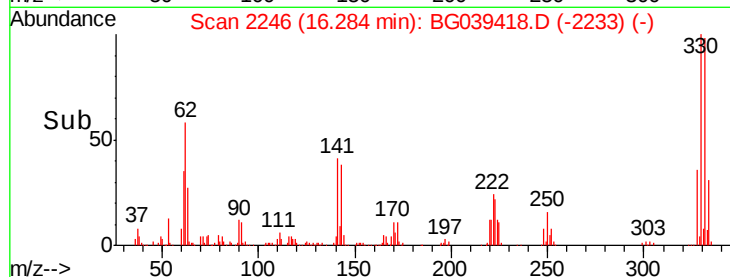
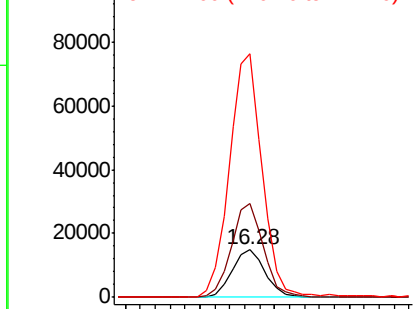



#76
Chrysene-d12
Concen: 20.000 ng
RT: 21.83 min Scan# 3190
Delta R.T. -0.02 min
Lab File: BG039418.D
Acq: 8 Feb 2019 16:39

Tgt Ion:240 Resp: 450302
Ion Ratio Lower Upper
240 100
120 9.0 7.0 10.6
236 25.2 21.0 31.4

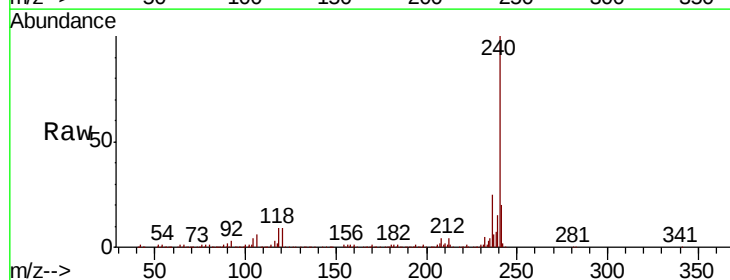

Abundance Ion 240.00 (239.70 to 240.70): E
Ion 120.00 (119.70 to 120.70): E
Ion 236.00 (235.70 to 236.70): E

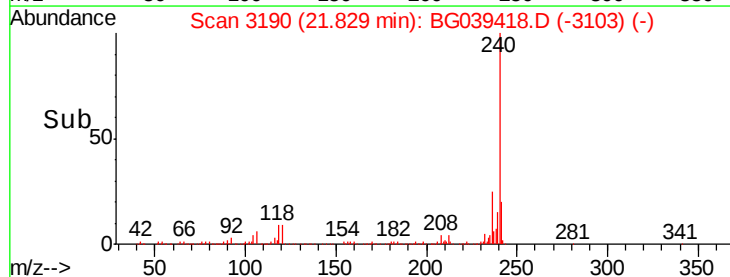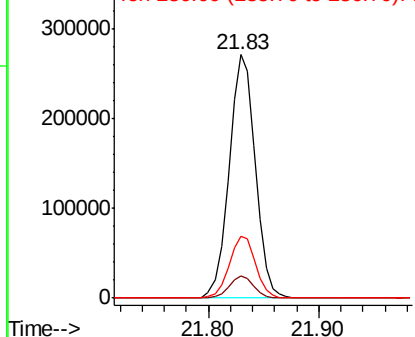

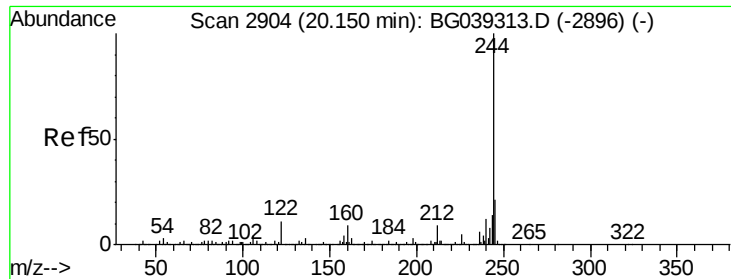

#79

Terphenyl-d14

Concen: 72.391 ng

RT: 20.14 min Scan# 2902

Delta R.T. -0.01 min

Lab File: BG039418.D

Acq: 8 Feb 2019 16:39

Instrument :

BNA_G

ClientSampleId :

A0C12-SS1-7.5-8.0


Tgt Ion:244 Resp: 1540039

Ion Ratio Lower Upper




244 100

212 9.5 7.3 10.9

122 9.6 8.4 12.6

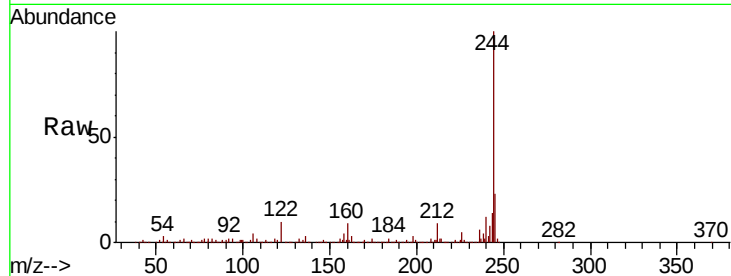

Abundance Ion 244.00 (243.70 to 244.70): E
1500000 Ion 212.00 (211.70 to 212.70): E
Ion 122.00 (121.70 to 122.70): E

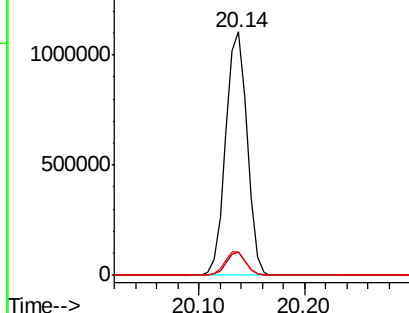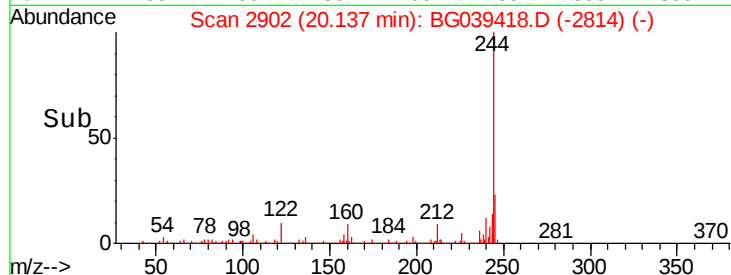

#87

Perylene-d12

Concen: 20.000 ng

RT: 25.21 min Scan# 3766

Delta R.T. -0.03 min

Lab File: BG039418.D

Acq: 8 Feb 2019 16:39


Tgt Ion:264 Resp: 458437

Ion Ratio Lower Upper

264 100

260 23.1 18.2 27.4

265 21.5 18.5 27.7



Abundance Ion 264.00 (263.70 to 264.70): E
200000 Ion 260.00 (259.70 to 260.70): E
Ion 265.00 (264.70 to 265.70): E

