


Data Path : Z:\SVOASRV\HPCHEM1\BNA_G\DATA\BG020819\
 Data File : BG039414.D
 Acq On : 8 Feb 2019 13:21
 Operator : JU/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG012919.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Jan 29 15:41:51 2019

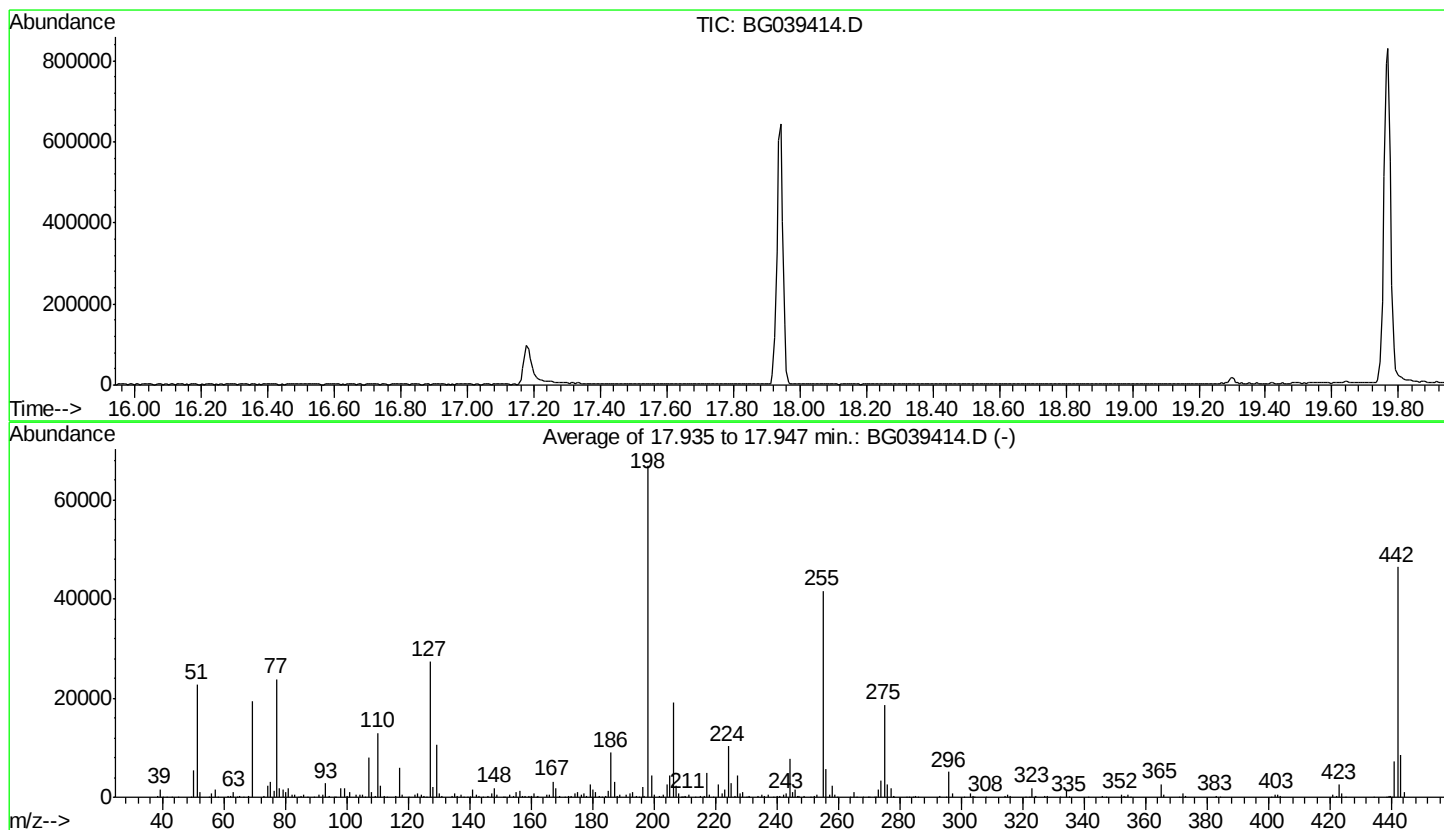

AutoFind: Scans 2527, 2528, 2529; Background Corrected with Scan 2520

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	33.8	22621	PASS
68	69	0.00	2	1.3	250	PASS
69	198	0.00	100	29.0	19418	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	40.8	27266	PASS
197	198	0.00	2	0.5	356	PASS
198	198	100	100	100.0	66882	PASS
199	198	5	9	6.6	4427	PASS
275	198	10	60	27.8	18605	PASS
365	198	1	100	4.0	2671	PASS
441	198	0.01	100	11.0	7331	PASS
442	198	50	100	69.4	46410	PASS
443	442	15	24	18.3	8499	PASS