
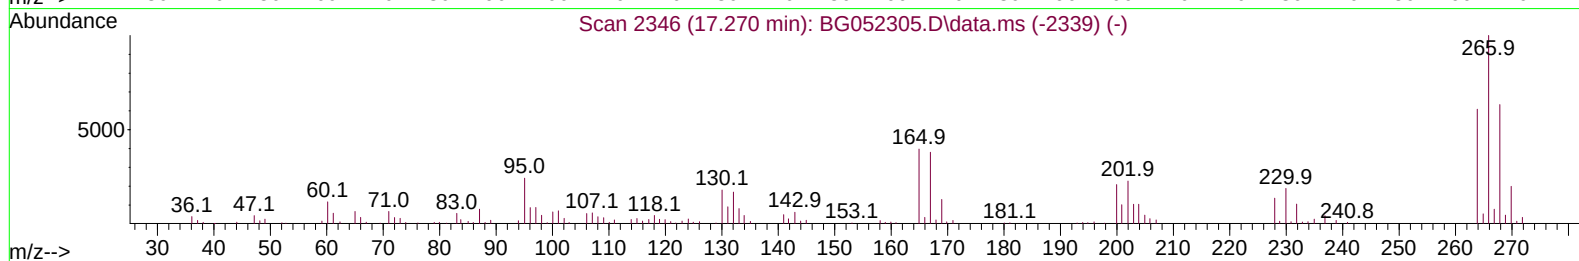
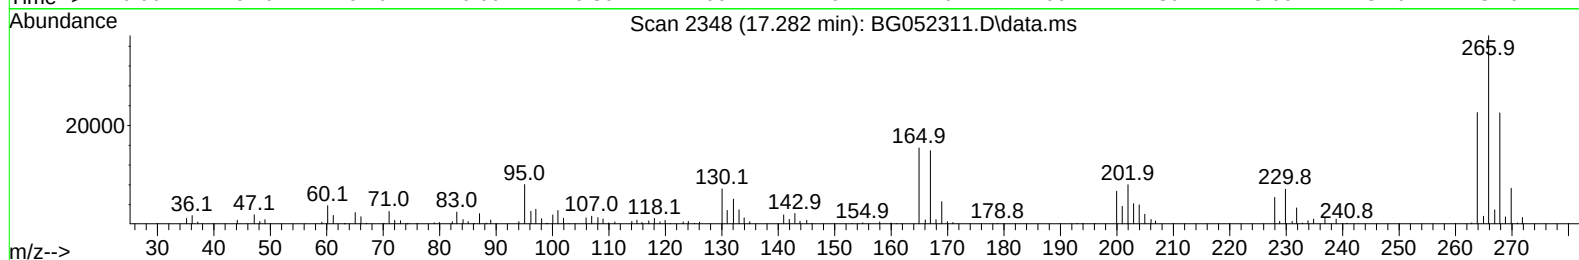


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG020822\
Data File : BG052311.D
Acq On : 8 Feb 2022 9:10
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Feb 08 10:00:37 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG020722.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Feb 08 01:21:20 2022
Response via : Initial Calibration

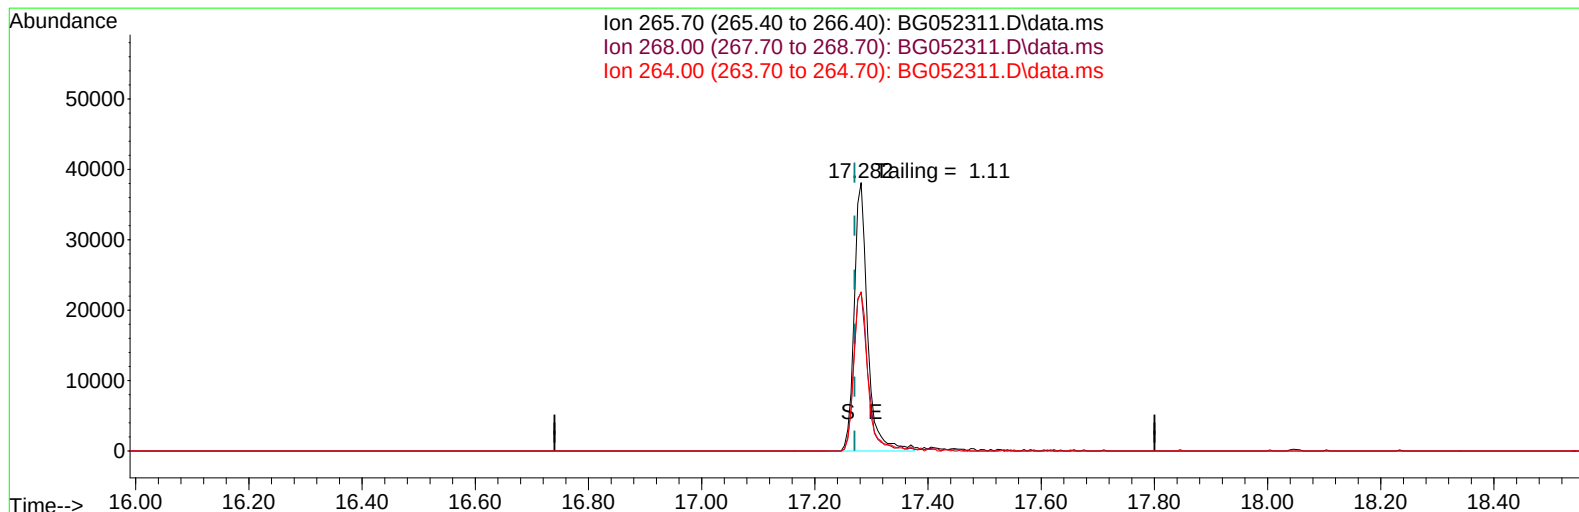

TIC: BG052311.D\data.ms

(70) Pentachlorophenol (C)




17.282min (+ 0.012) 175874.93 ng

response 62419

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.20	59.12
264.00	65.20	59.31
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG020822\
Data File : BG052311.D
Acq On : 8 Feb 2022 9:10
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Feb 08 10:00:37 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG020722.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Feb 08 01:21:20 2022
Response via : Initial Calibration

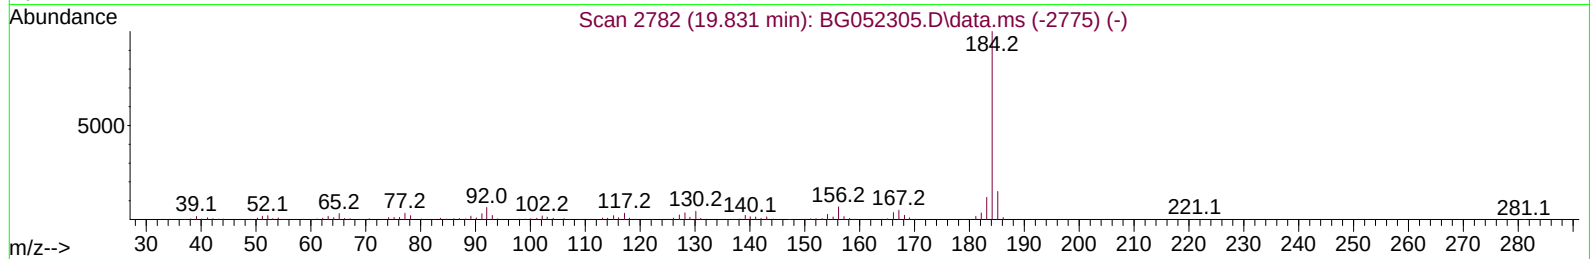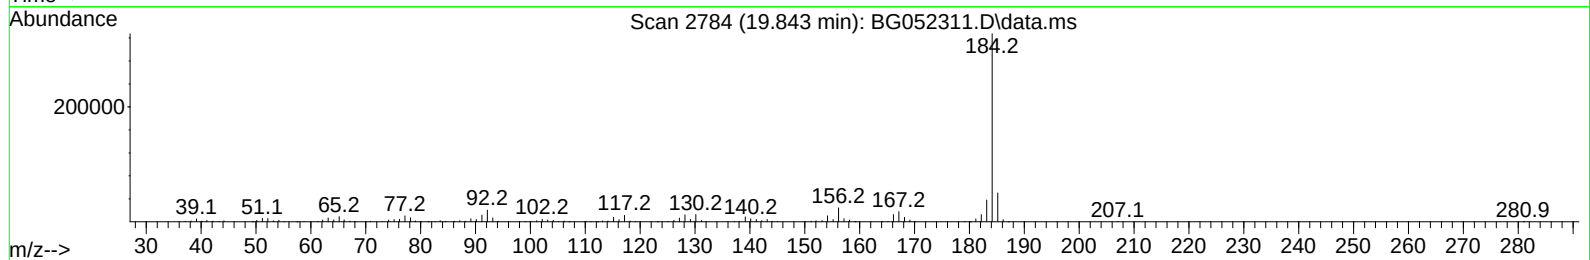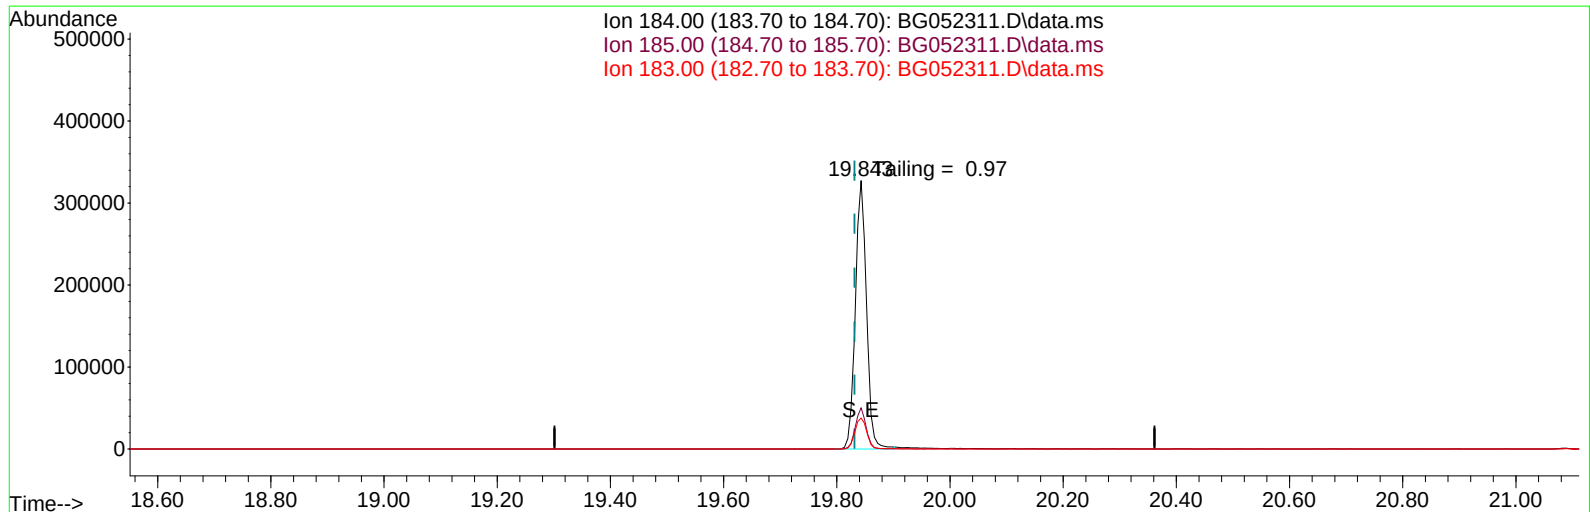

TIC: BG052311.D\data.ms

(77) Benzidine**19.843min (+ 0.012) 85821.36 ng****response 452951**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.80	15.38
183.00	12.20	11.60
0.00	0.00	0.00