


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG020822\
 Data File : BG052311.D
 Acq On : 8 Feb 2022 9:10
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG020722.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Feb 08 01:21:20 2022

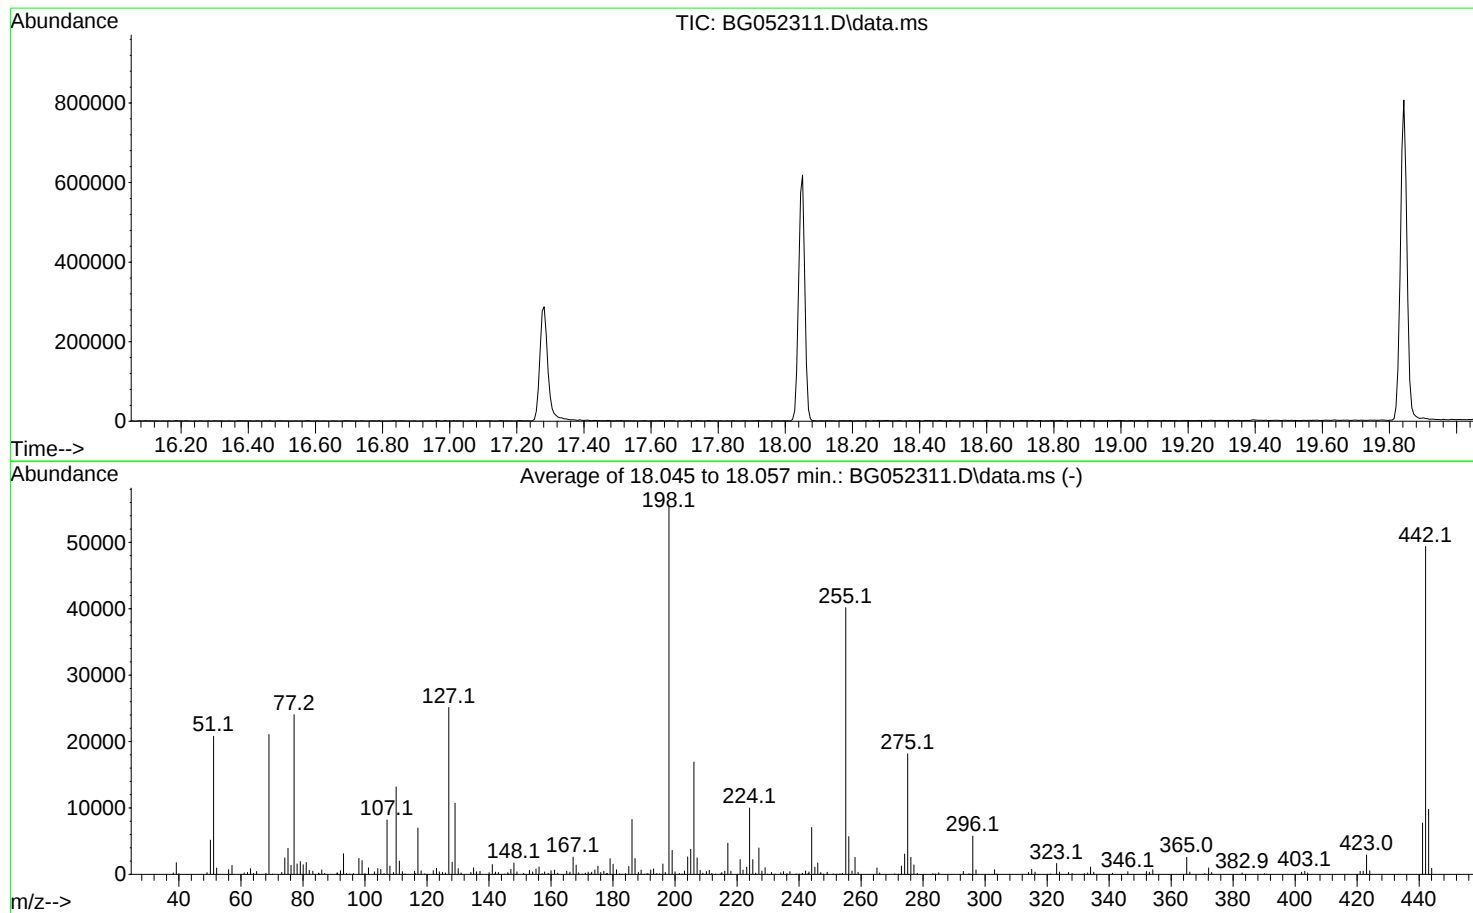




AutoFind: Scans 2478, 2479, 2480; Background Corrected with Scan 2471

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	37.5	20799	PASS
68	69	0.00	2	0.7	151	PASS
69	198	0.00	100	38.0	21065	PASS
70	69	0.00	2	0.3	53	PASS
127	198	10	80	45.4	25133	PASS
197	198	0.00	2	0.5	296	PASS
198	198	100	100	100.0	55403	PASS
199	198	5	9	6.5	3610	PASS
275	198	10	60	32.8	18157	PASS
365	198	1	100	4.7	2580	PASS
441	198	0.01	100	14.0	7749	PASS
442	442	50	100	100.0	49381	PASS
443	442	15	24	19.9	9803	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG020822\
Data File : BG052311.D
Acq On : 8 Feb 2022 9:10
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: Feb 08 10:00:37 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG020722.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Feb 08 01:21:20 2022
Response via : Initial Calibration

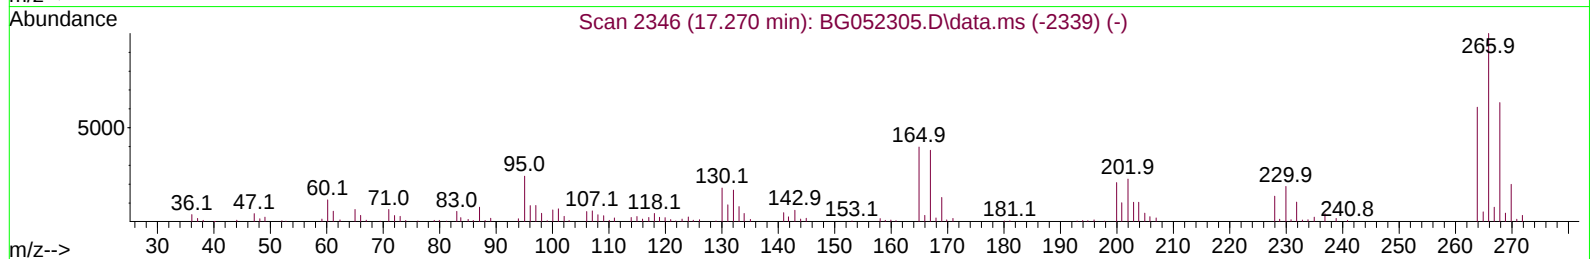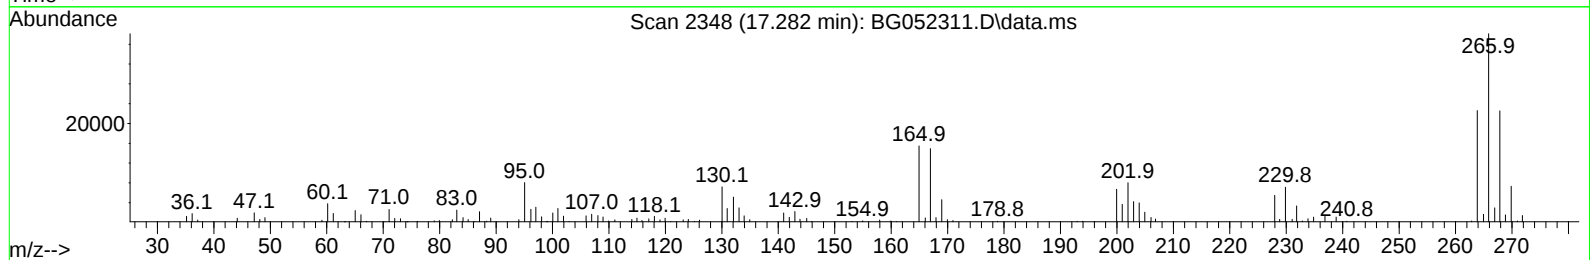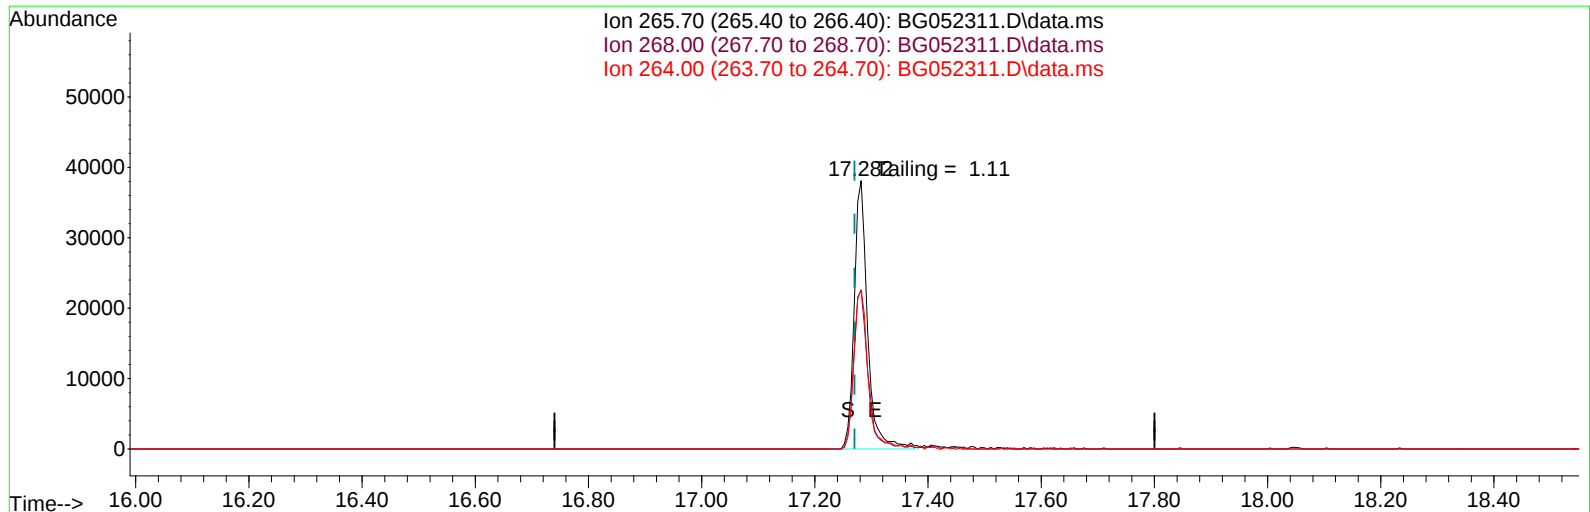

TIC: BG052311.D\data.ms

(70) Pentachlorophenol (C)

17.282min (+ 0.012) 175874.93 ng




response 62419

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.20	59.12
264.00	65.20	59.31
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG020822\
Data File : BG052311.D
Acq On : 8 Feb 2022 9:10
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: Feb 08 10:00:37 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG020722.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Feb 08 01:21:20 2022
Response via : Initial Calibration

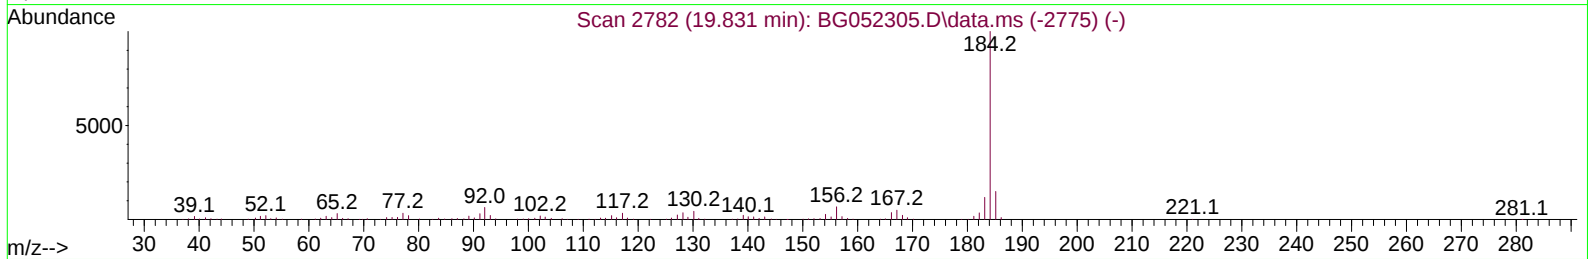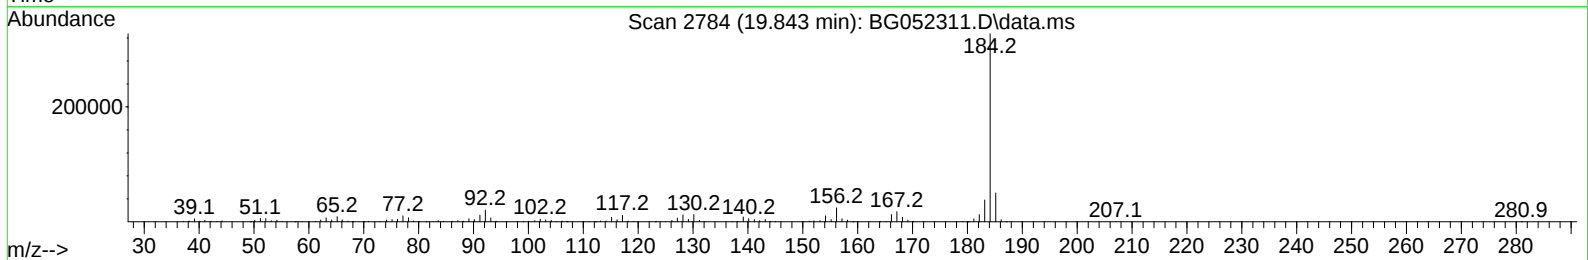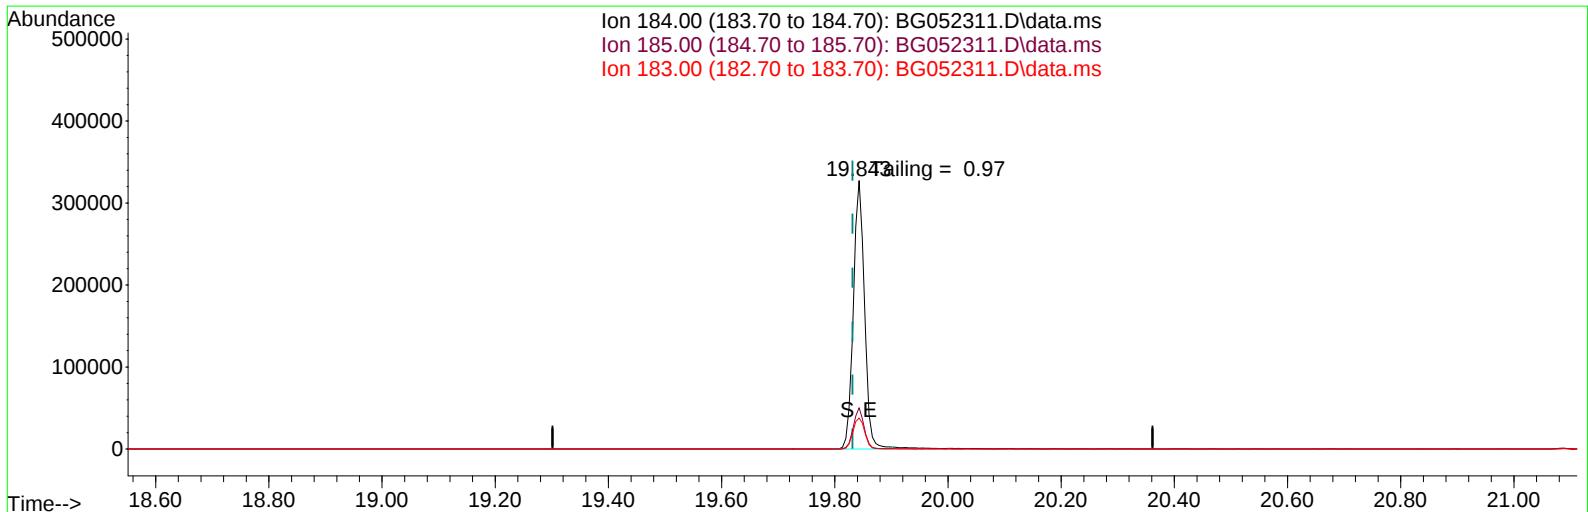

TIC: BG052311.D\data.ms

(77) Benzidine

19.843min (+ 0.012) 85821.36 ng

response 452951

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.80	15.38
183.00	12.20	11.60
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
2/8/2022	BNA_G	<u>BG052311.D</u>
Compound Name	Response	Retention Time
DDT	251798	21.08
DDD	2592	20.63
DDE	0	19.9
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
2592	254390	1.02