
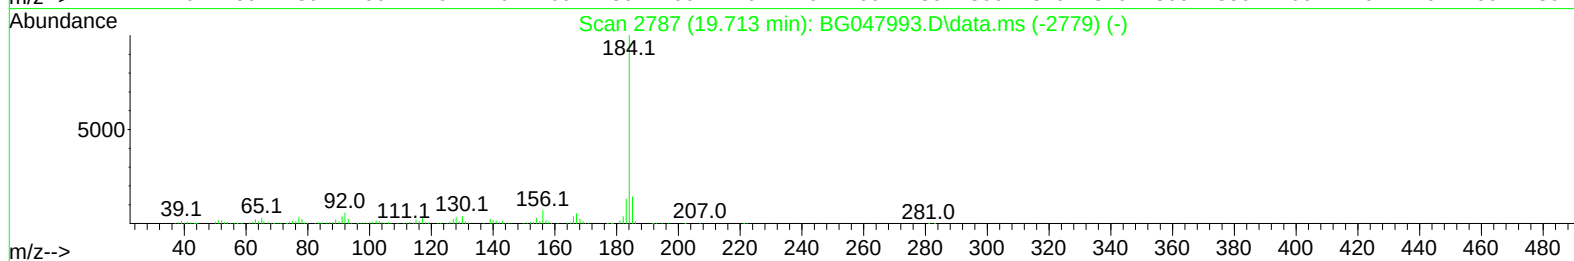
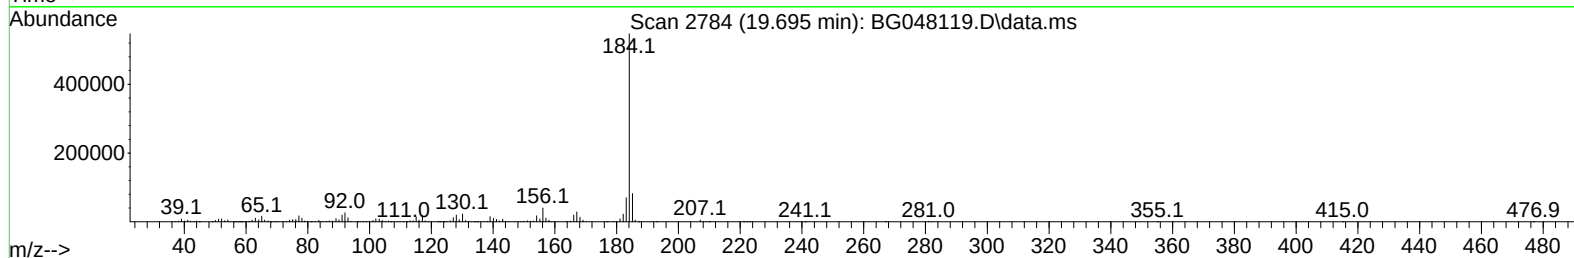


Data Path : Z:\svoasrv\HPCHEM1\BNA\_G\Data\BG020921\  
Data File : BG048119.D  
Acq On : 9 Feb 2021 12:24  
Operator : CG/JU  
Sample : DFTPP  
Misc :  
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Feb 09 15:57:33 2021  
Quant Method : Z:\SVOASRV\HPCHEM1\BNA\_G\METHODS\8270-BG012521.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Tue Feb 09 14:29:17 2021  
Response via : Initial Calibration

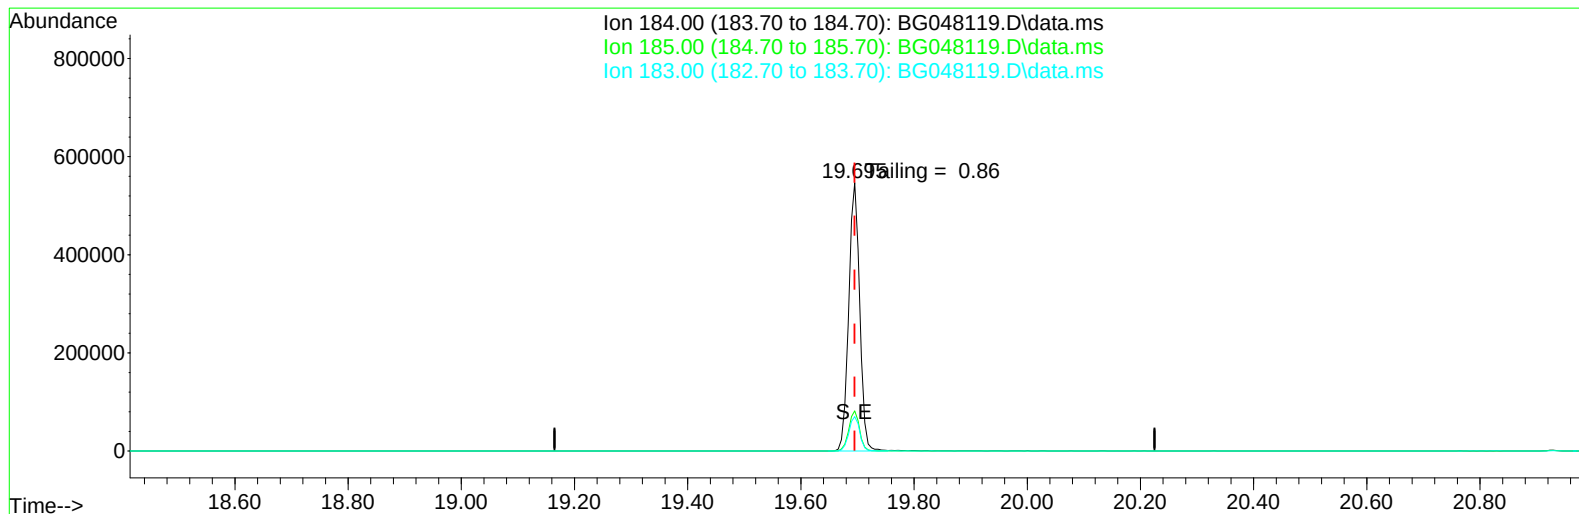

TIC: BG048119.D\data.ms

**(77) Benzidine**




**19.695min (+ 0.001) 433581.39 ng**

**response 737969**

| Ion    | Exp%   | Act%   |
|--------|--------|--------|
| 184.00 | 100.00 | 100.00 |
| 185.00 | 15.50  | 14.98  |
| 183.00 | 13.20  | 12.81  |
| 0.00   | 0.00   | 0.00   |

Data Path : Z:\svoasrv\HPCHEM1\BNA\_G\Data\BG020921\  
Data File : BG048119.D  
Acq On : 9 Feb 2021 12:24  
Operator : CG/JU  
Sample : DFTPP  
Misc :  
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Feb 09 15:57:33 2021  
Quant Method : Z:\SVOASRV\HPCHEM1\BNA\_G\METHODS\8270-BG012521.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Tue Feb 09 14:29:17 2021  
Response via : Initial Calibration

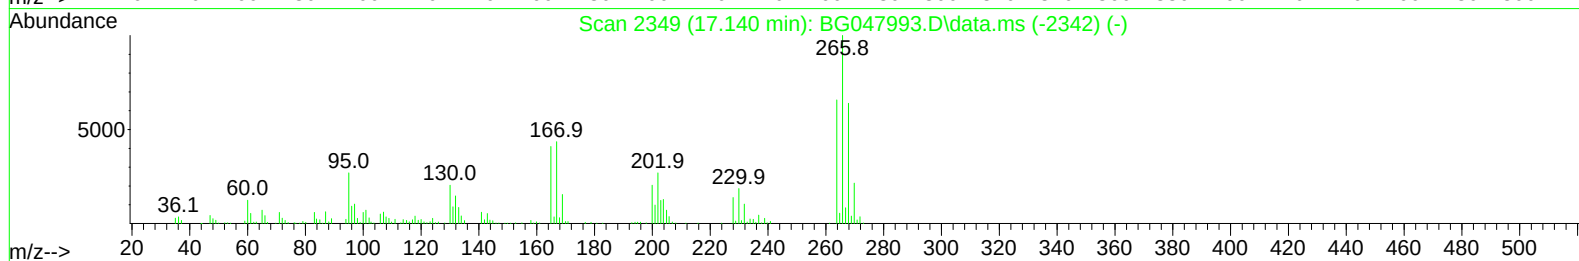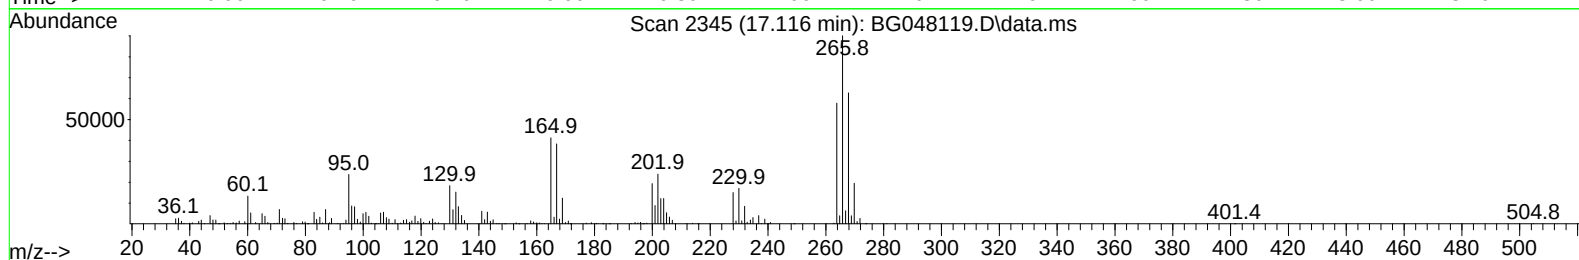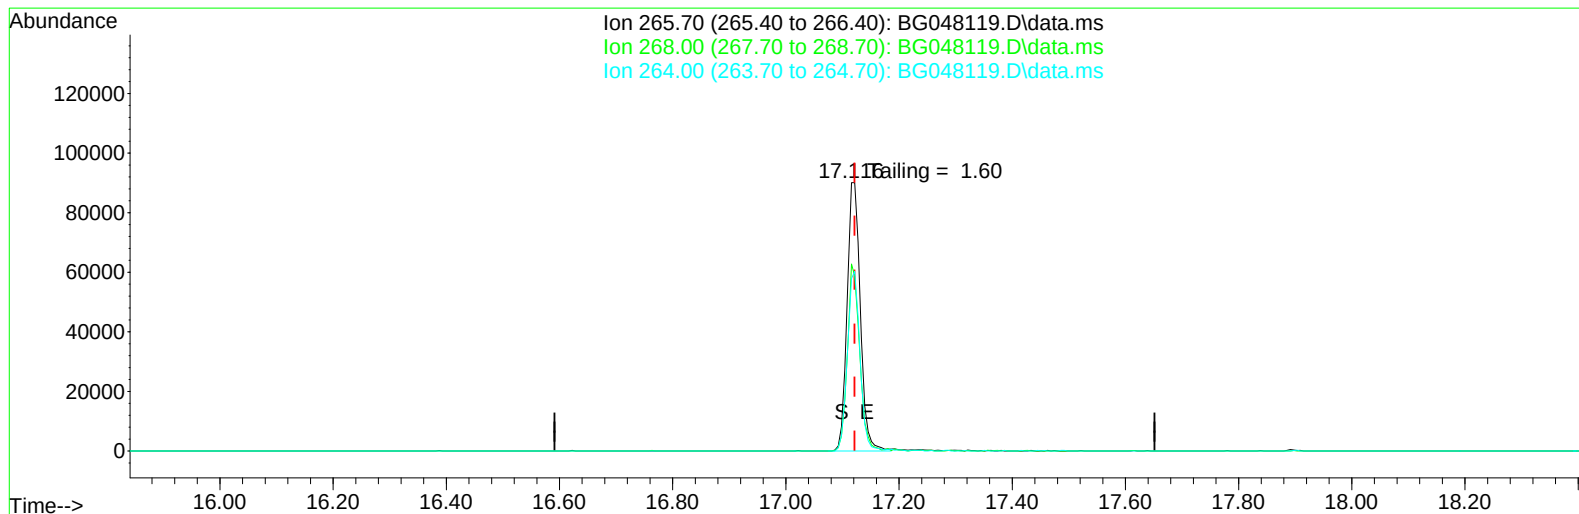

TIC: BG048119.D\data.ms

**(70) Pentachlorophenol (C)**

17.116min (-0.005) 278493.93 ng

response 147442

| Ion    | Exp%   | Act%   |
|--------|--------|--------|
| 265.70 | 100.00 | 100.00 |
| 268.00 | 62.20  | 69.67  |
| 264.00 | 61.60  | 64.27  |
| 0.00   | 0.00   | 0.00   |