
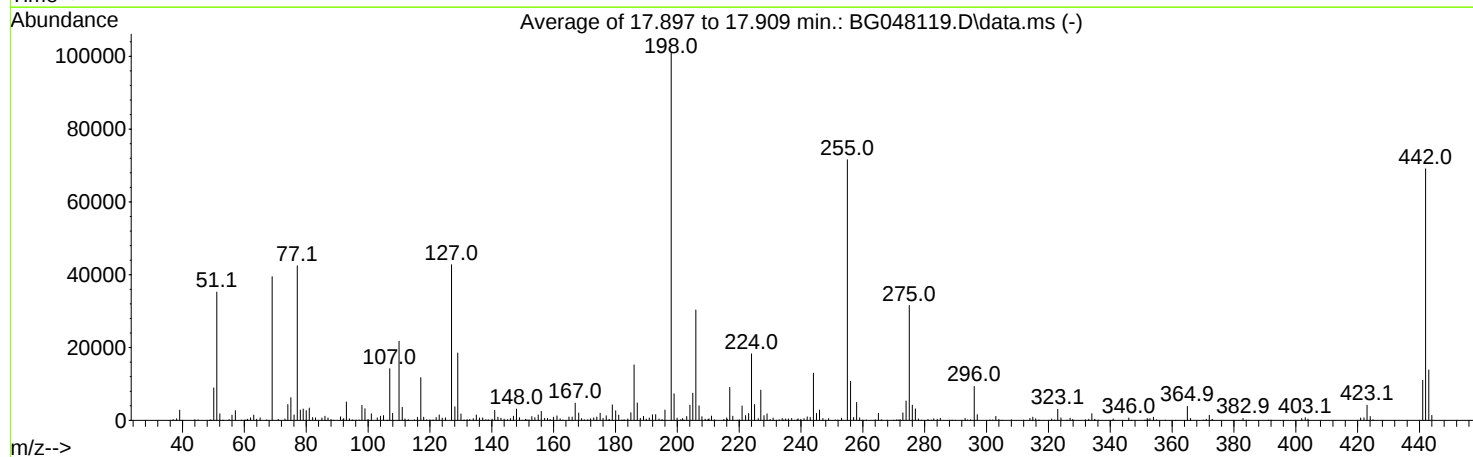


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG020921\
 Data File : BG048119.D
 Acq On : 9 Feb 2021 12:24
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG012521.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Feb 09 14:29:17 2021

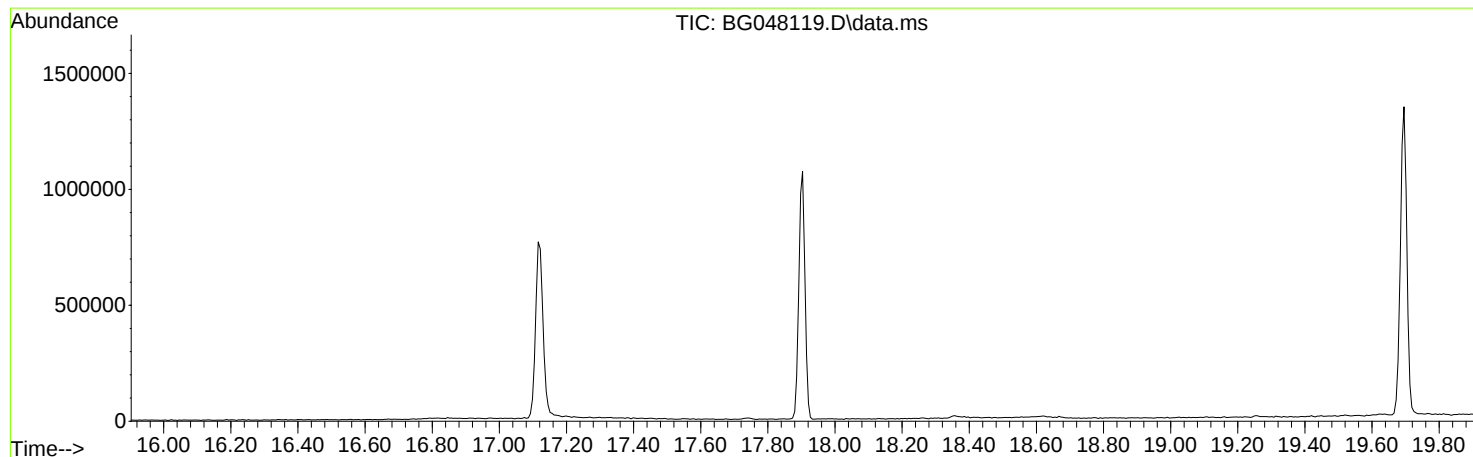

AutoFind: Scans 2478, 2479, 2480; Background Corrected with Scan 2471

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	34.9	35240	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	39.1	39470	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	42.3	42773	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	101045	PASS
199	198	5	9	7.2	7284	PASS
275	198	10	60	31.2	31571	PASS
365	198	1	100	3.8	3824	PASS
441	198	0.01	100	10.9	11028	PASS
442	198	50	100	68.4	69083	PASS
443	442	15	24	20.1	13857	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
2/9/2021	BNA_G	<u>BG048119.D</u>
Compound Name	Response	Retention Time
DDT	391297	20.92
DDD	1569	20.48
DDE	544	19.98
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
2113	393410	0.54

Instrument :
BNA_G
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG020921\
Data File : BG048119.D
Acq On : 9 Feb 2021 12:24
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: Feb 09 15:57:33 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG012521.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Feb 09 14:29:17 2021
Response via : Initial Calibration

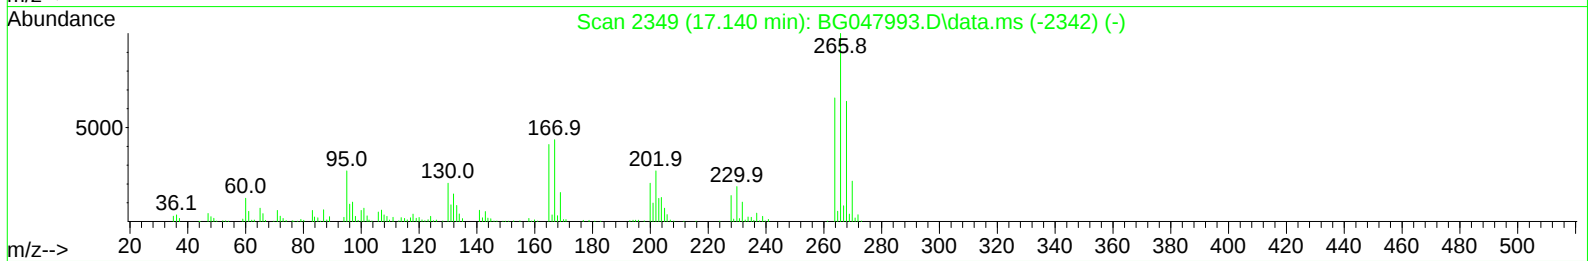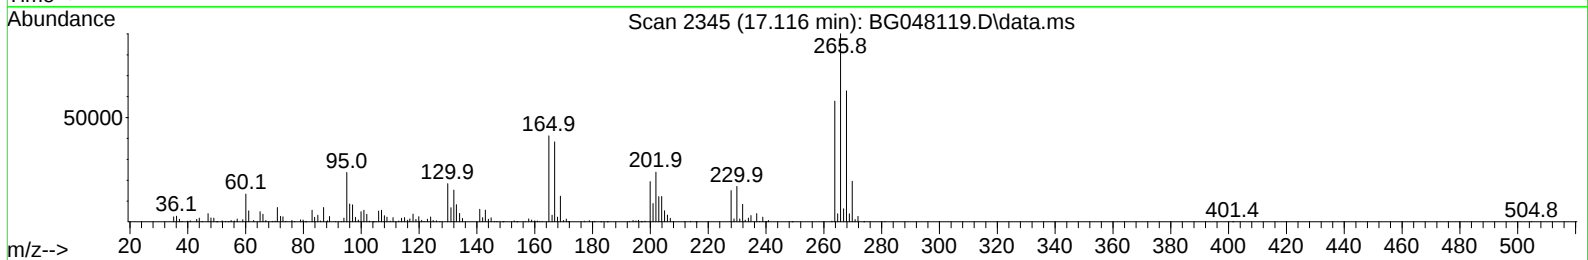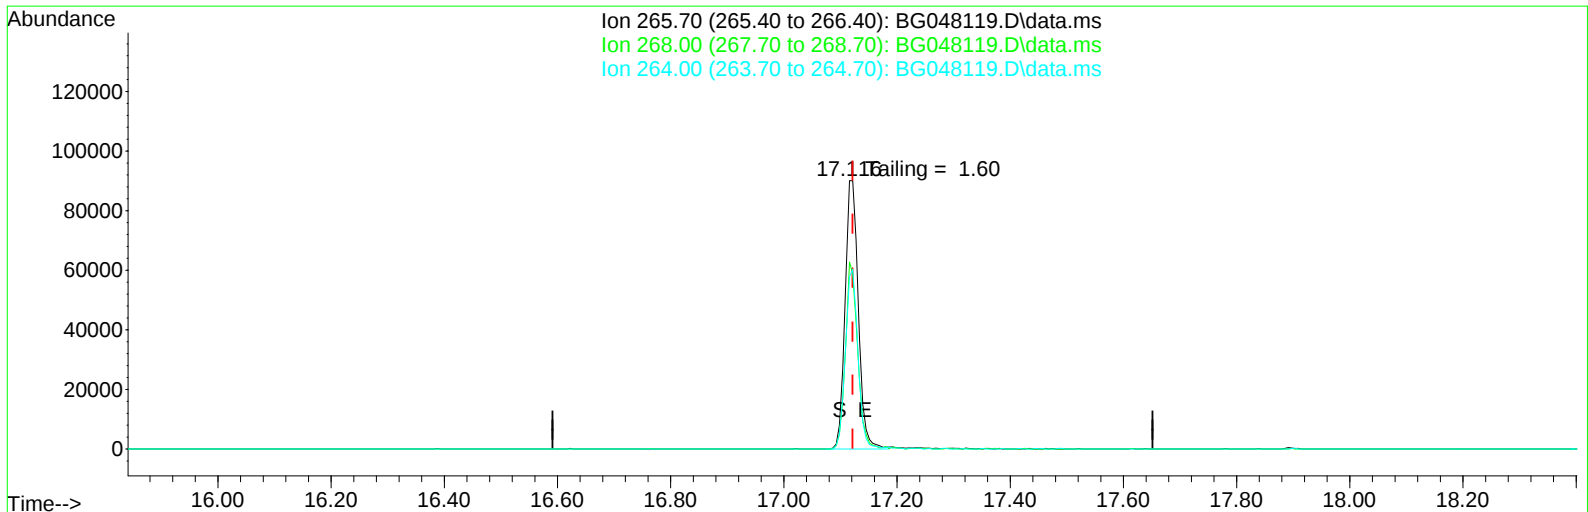

TIC: BG048119.D\data.ms

(70) Pentachlorophenol (C)

17.116min (-0.005) 278493.93 ng




response 147442

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	69.67
264.00	61.60	64.27
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG020921\
Data File : BG048119.D
Acq On : 9 Feb 2021 12:24
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: Feb 09 15:57:33 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG012521.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Feb 09 14:29:17 2021
Response via : Initial Calibration

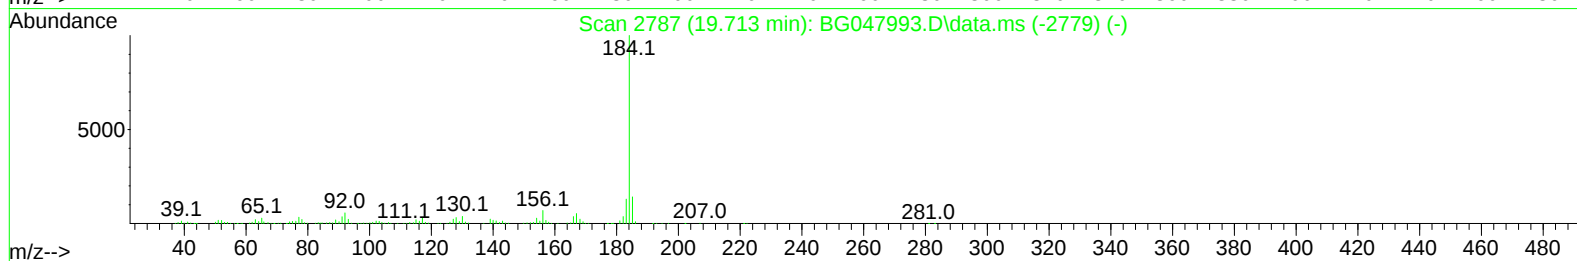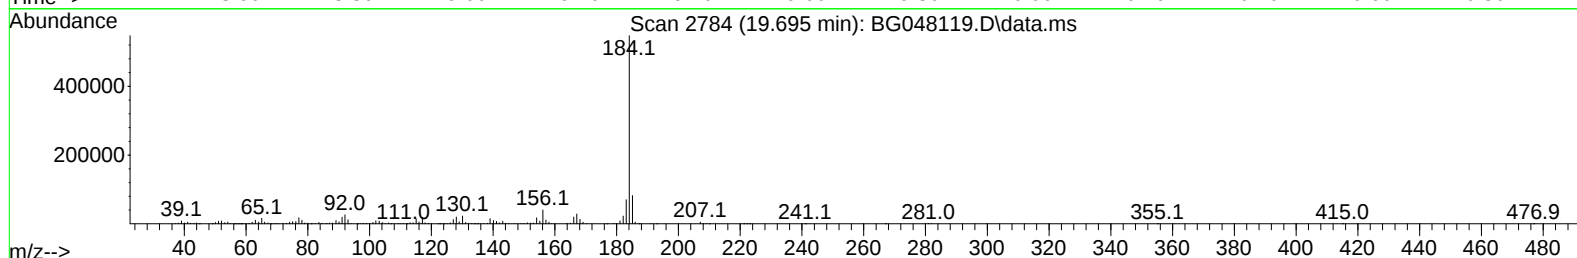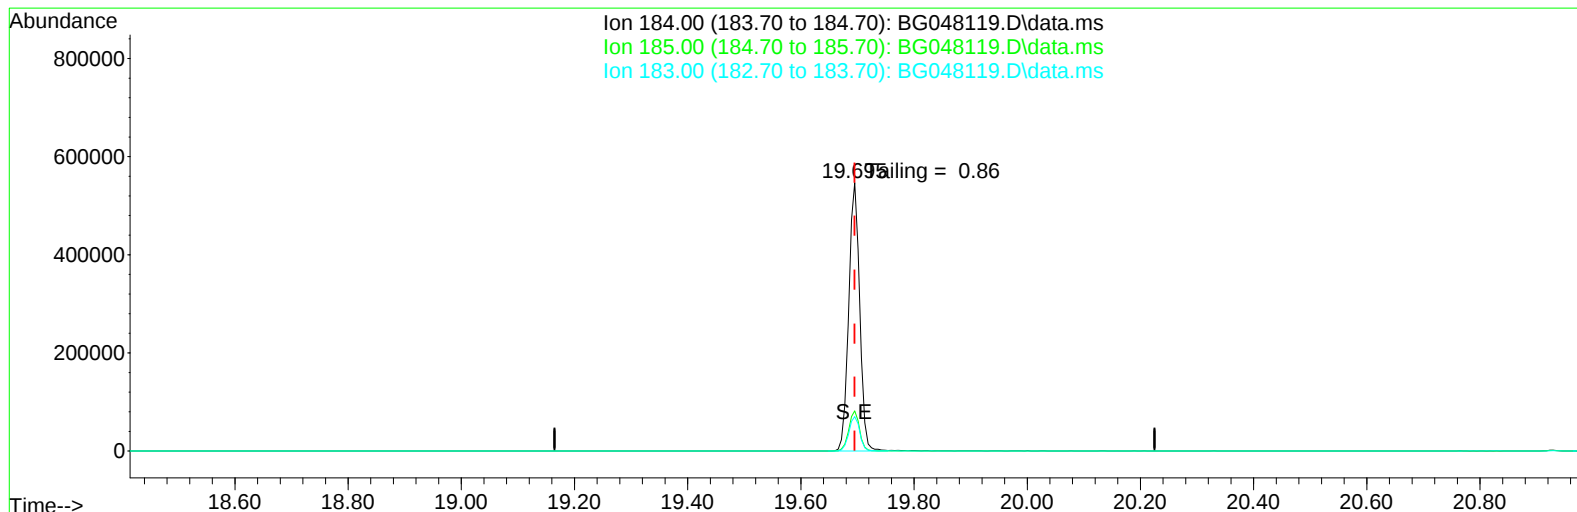

TIC: BG048119.D\data.ms

(77) Benzidine

19.695min (+ 0.001) 433581.39 ng

response 737969

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	14.98
183.00	13.20	12.81
0.00	0.00	0.00