
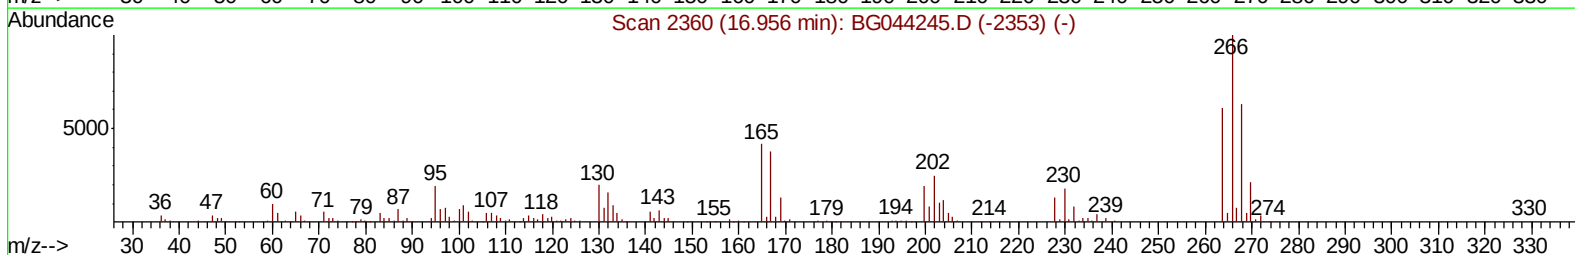
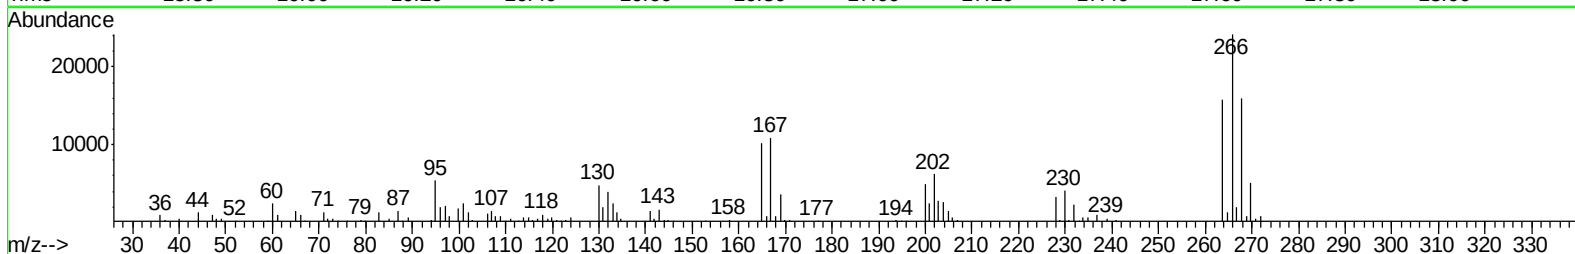


Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG021020\
Data File : BG044355.D
Acq On : 10 Feb 2020 12:40
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Feb 11 03:24:31 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG013020.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Feb 10 16:11:50 2020
Response via : Initial Calibration

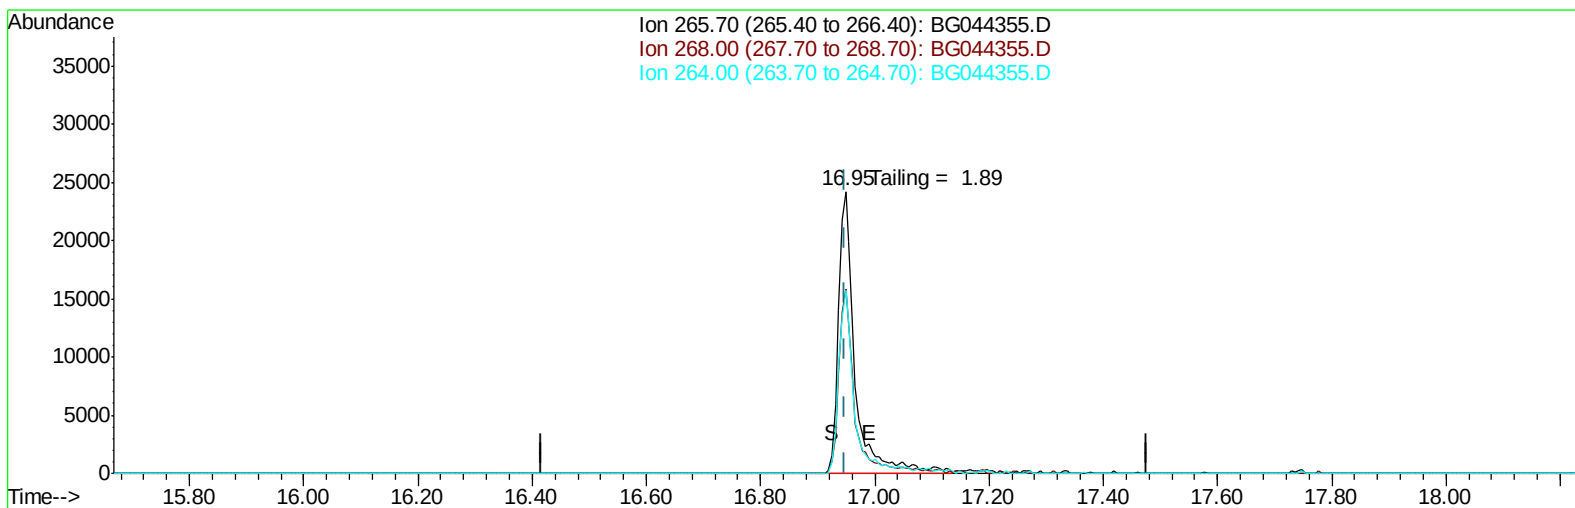

TIC: BG044355.D

(70) Pentachlorophenol (C)




16.948min (+0.001) 31260.73ng

response 45787

Ion	Exp%	Act%
265.70	100	100
268.00	63.20	65.67
264.00	60.90	64.97
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG021020\
 Data File : BG044355.D
 Acq On : 10 Feb 2020 12:40
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Feb 11 03:24:31 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG013020.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Feb 10 16:11:50 2020
 Response via : Initial Calibration

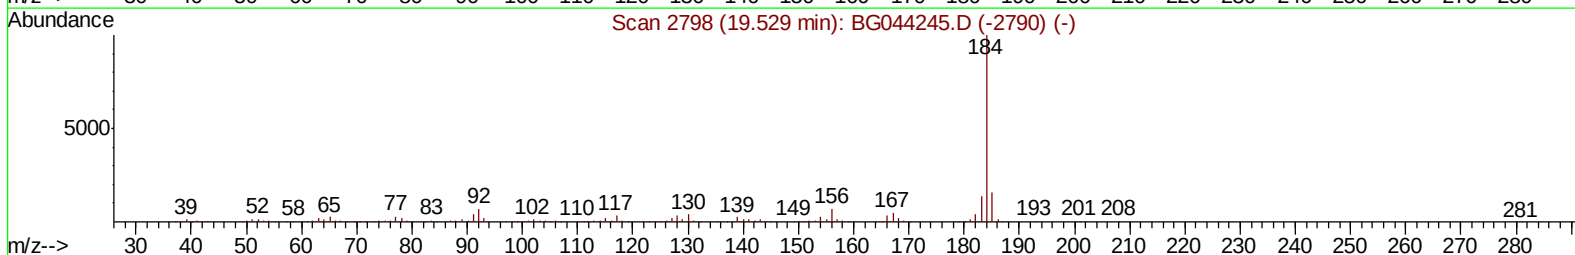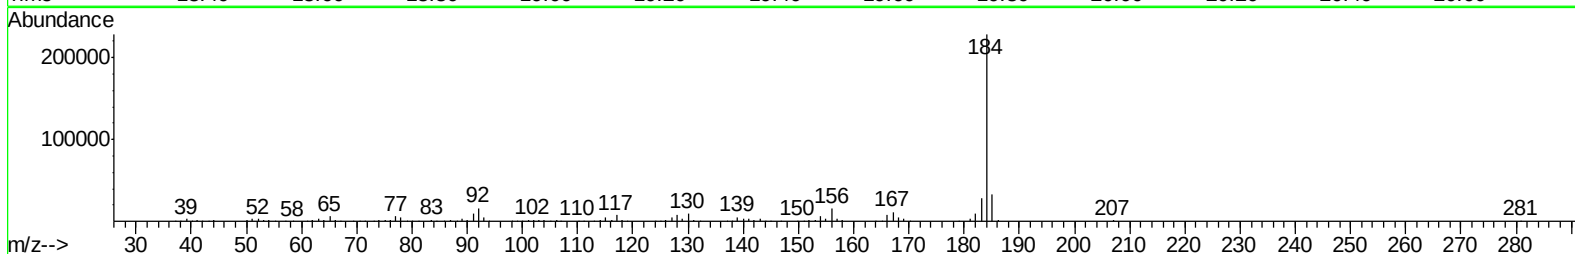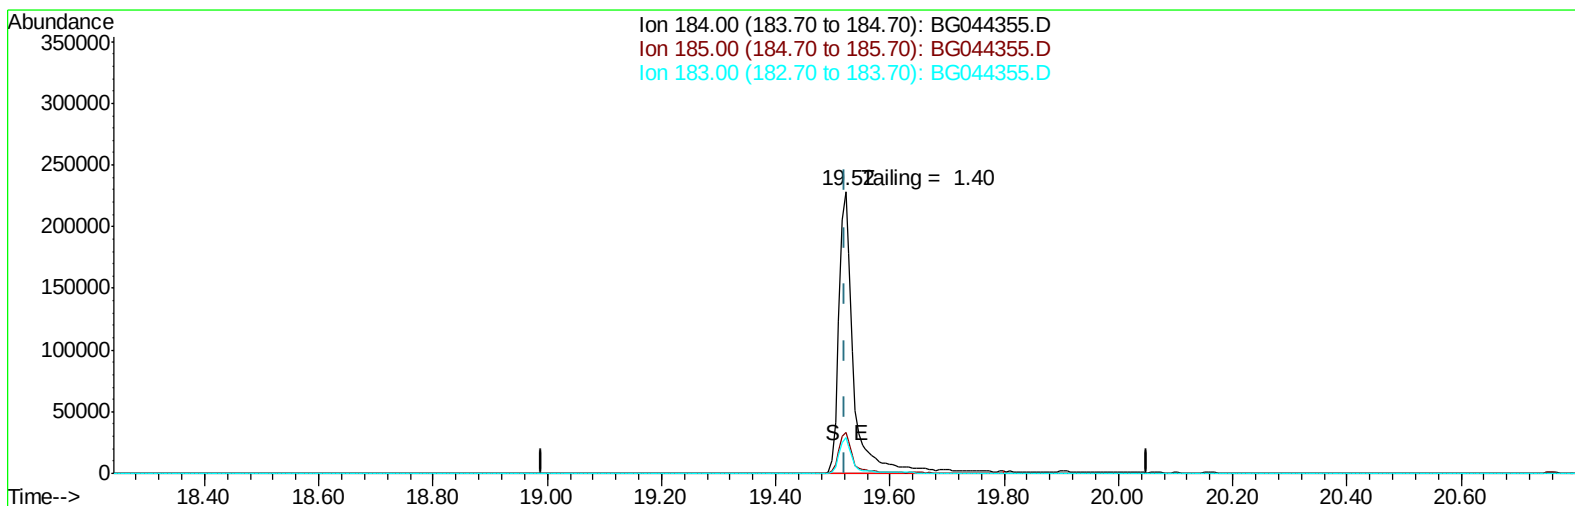

TIC: BG044355.D

(77) Benzidine

19.522min (+0.001) 253965.15ng

response 408574

Ion	Exp%	Act%
184.00	100	100
185.00	16.10	14.59
183.00	13.50	12.65
0.00	0.00	0.00