

Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG021020\
 Data File : BG044362.D
 Acq On : 10 Feb 2020 18:40
 Operator : CG/JU
 Sample : L1470-02
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 PE-1-(BASE)

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0
 Filtering: 5
 Min Area: 3 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG013020.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.479	400	407	420	rBV	714880	1172223	28.91%	6.400%
2	7.072	670	678	694	rBV	732220	1303933	32.16%	7.119%
3	7.900	811	819	829	rVB	186168	327579	8.08%	1.788%
4	8.223	867	874	883	rBV	573527	1014668	25.02%	5.540%
5	9.058	1007	1016	1034	rBV	427752	811787	20.02%	4.432%
6	10.703	1289	1296	1314	rVB	239680	474962	11.71%	2.593%
7	13.165	1707	1715	1730	rBV	1359156	2162713	53.33%	11.807%
8	14.005	1852	1858	1869	rBV	29505	56824	1.40%	0.310%
9	14.539	1941	1949	1962	rBV2	474927	786439	19.39%	4.294%
10	16.032	2196	2203	2222	rBV	1198769	1892720	46.68%	10.333%
11	17.283	2409	2416	2431	rBV	719145	1118385	27.58%	6.106%
12	19.898	2855	2861	2875	rBV	3002573	4055083	100.00%	22.139%
13	21.202	3078	3083	3090	rBV3	59509	107105	2.64%	0.585%
14	21.531	3131	3139	3150	rBV	752102	1285340	31.70%	7.017%
15	21.737	3170	3174	3178	rVB2	36819	45915	1.13%	0.251%
16	22.324	3268	3274	3280	rBV2	39605	66652	1.64%	0.364%
17	22.988	3382	3387	3394	rVB2	47629	86958	2.14%	0.475%
18	23.758	3511	3518	3526	rBV2	47872	100010	2.47%	0.546%
19	24.610	3653	3663	3689	rVB2	463917	1382195	34.09%	7.546%
20	25.750	3850	3857	3864	rVB4	23421	65022	1.60%	0.355%


Sum of corrected areas: 18316513

Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG021020\
Data File : BG044362.D
Acq On : 10 Feb 2020 18:40
Operator : CG/JU
Sample : L1470-02
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
PE-1-(BASE)

Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG013020.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST11.L
TIC Integration Parameters: LSCINT.P

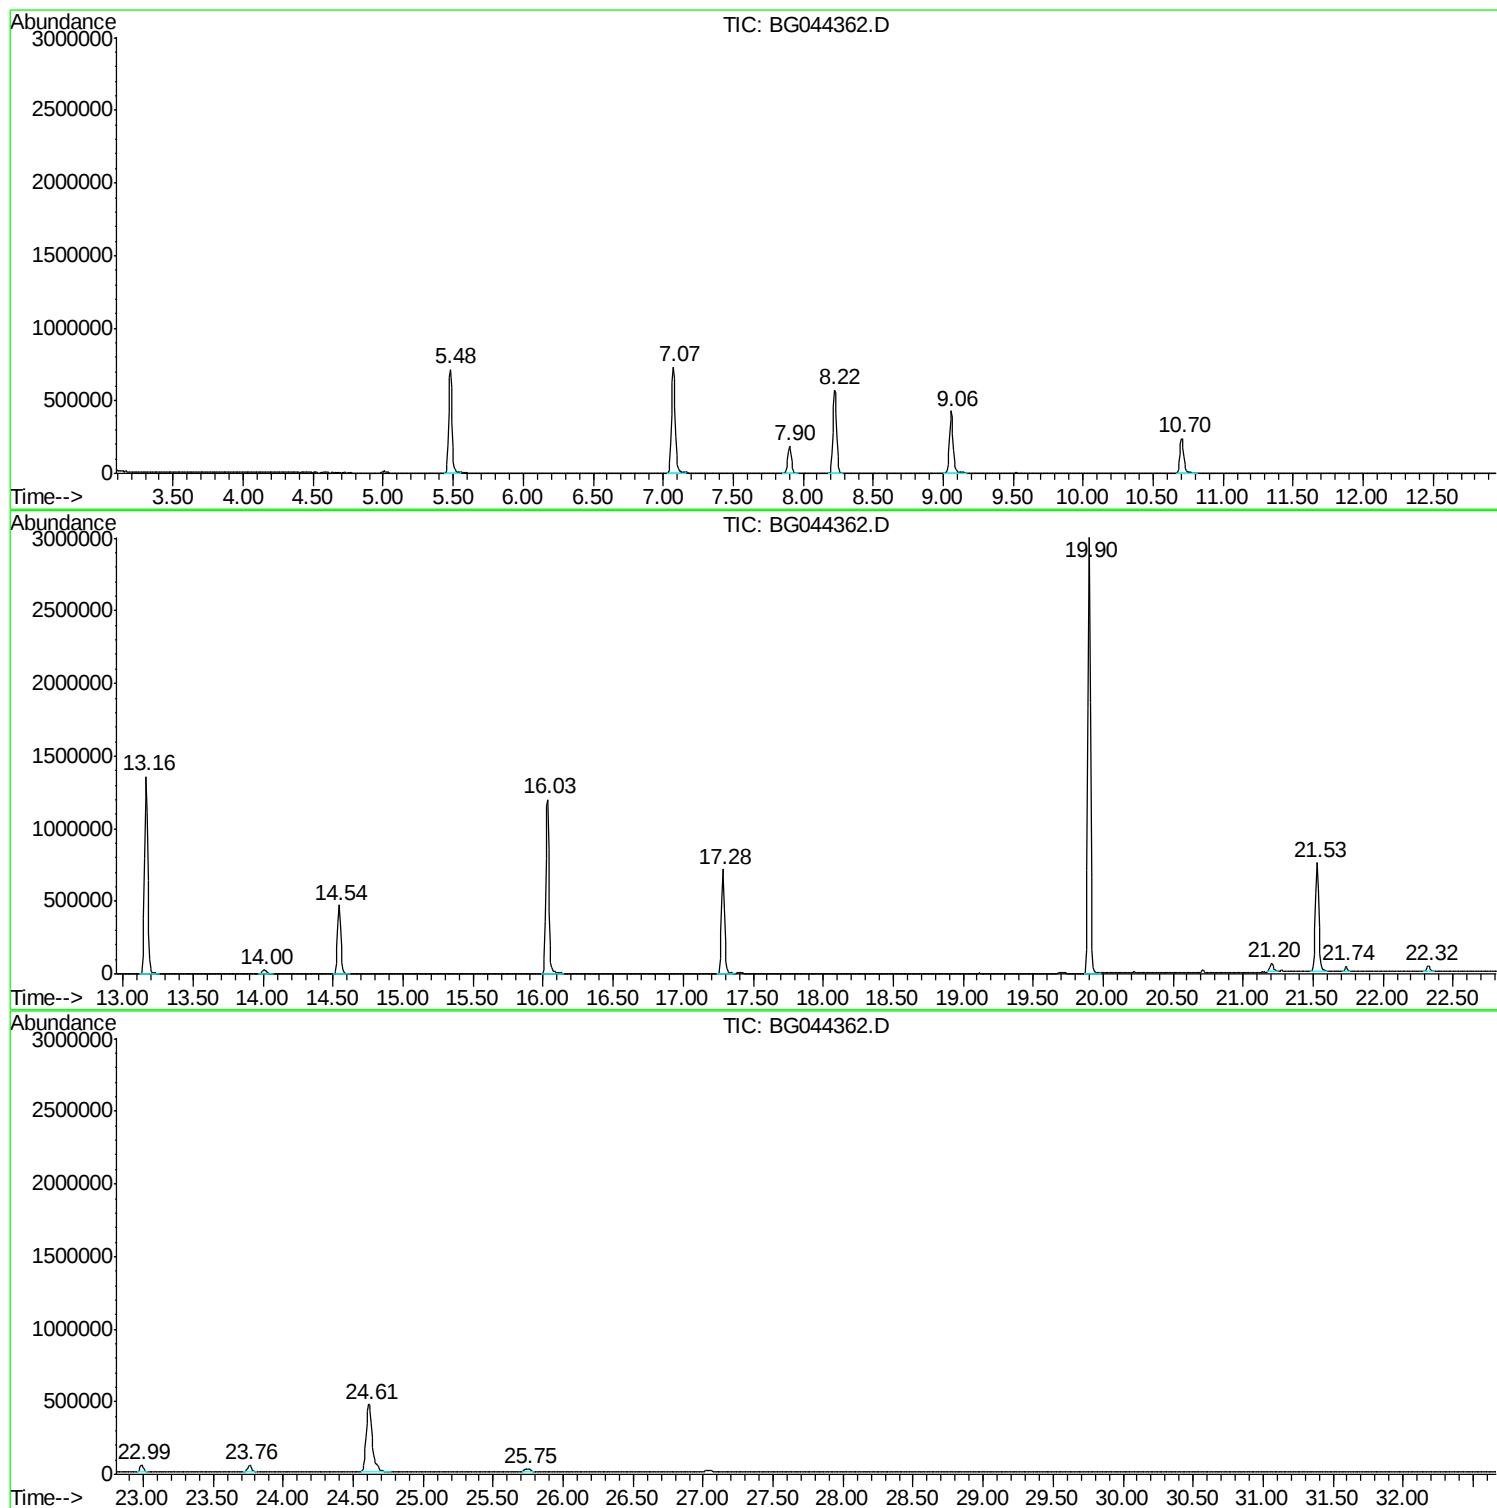

Data Path : Z:\SVOASRV\HPCHEM1\BNA_G\DATA\BG021020\
Data File : BG044362.D
Acq On : 10 Feb 2020 18:40
Operator : CG/JU
Sample : L1470-02
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
PE-1-(BASE)

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG013020.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\SVOASRV\HPCHEM1\BNA_G\DATA\BG021020\
Data File : BG044362.D
Acq On : 10 Feb 2020 18:40
Operator : CG/JU
Sample : L1470-02
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
PE-1-(BASE)

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG013020.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	---Internal Standard---
					# RT Resp Conc