


Data Path : Z:\svoasrv\HPCHEM1\BNA G\Data\BG021020\
 Data File : BG044355.D
 Acq On : 10 Feb 2020 12:40
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG013020.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Feb 10 16:11:50 2020

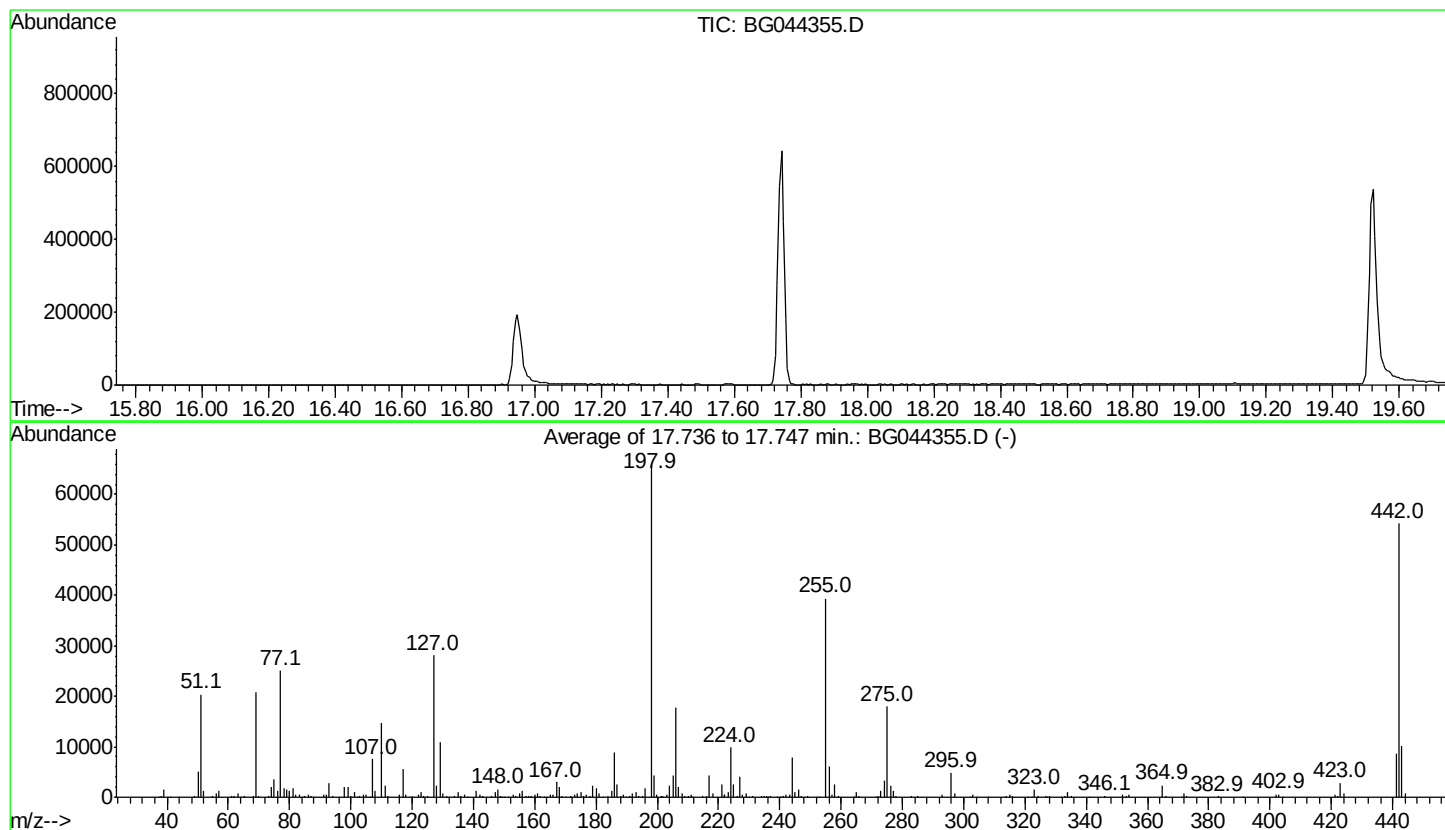

AutoFind: Scans 2493, 2494, 2495; Background Corrected with Scan 2486

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	31.1	20416	PASS
68	69	0.00	2	0.8	165	PASS
69	198	0.00	100	31.5	20694	PASS
70	69	0.00	2	0.7	152	PASS
127	198	10	80	42.7	28058	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	65712	PASS
199	198	5	9	6.7	4429	PASS
275	198	10	60	27.4	17980	PASS
365	198	1	100	3.5	2286	PASS
441	198	0.01	100	13.2	8685	PASS
442	198	50	100	82.4	54176	PASS
443	442	15	24	18.6	10094	PASS