


Data Path : Z:\svoasrv\HPCHEM1\BNA G\Data\BG021020\
 Data File : BG044368.D
 Acq On : 10 Feb 2020 23:55
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG013020.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Feb 10 16:11:50 2020

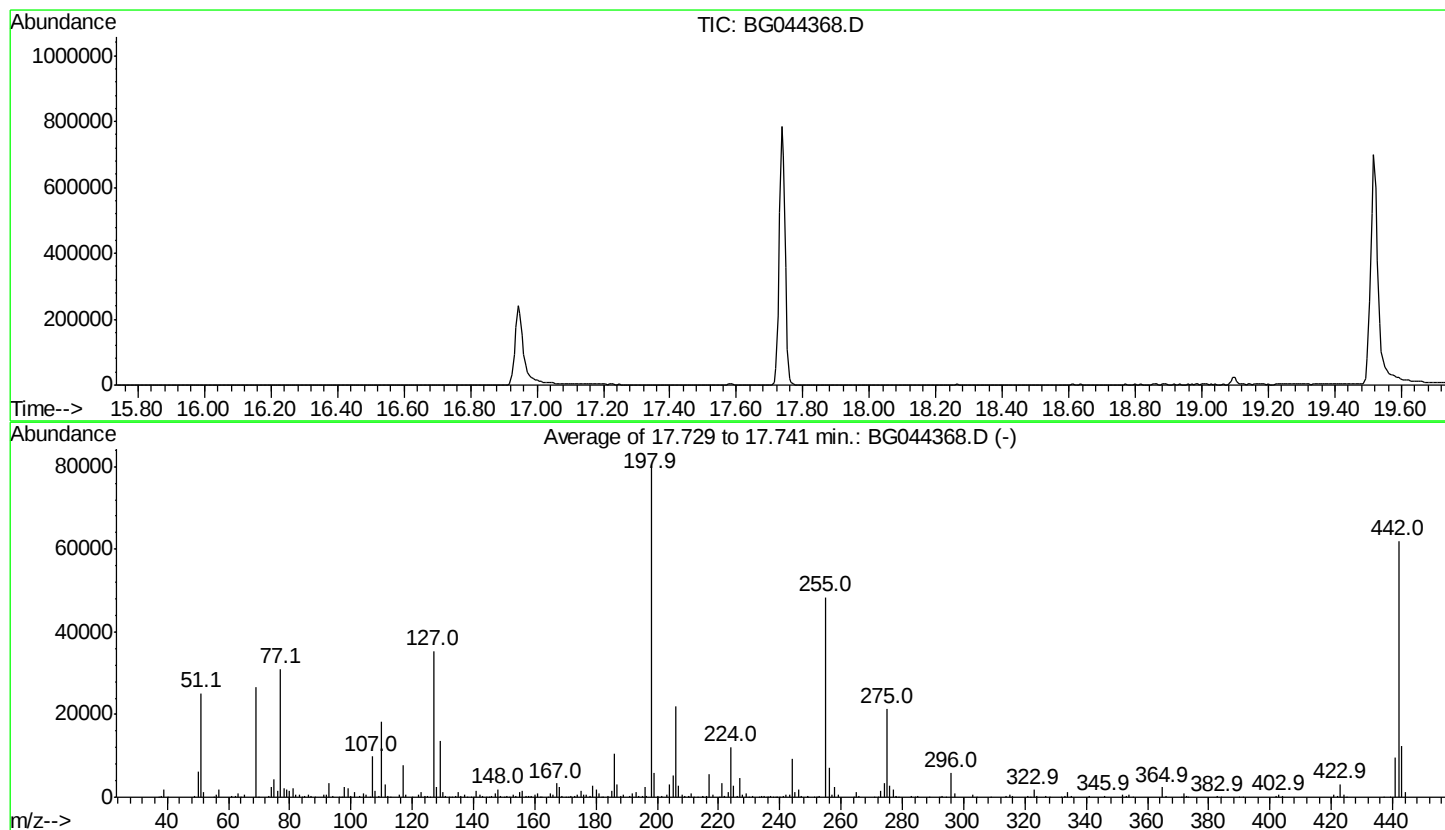

AutoFind: Scans 2492, 2493, 2494; Background Corrected with Scan 2486

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	31.3	25136	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	33.2	26653	PASS
70	69	0.00	2	0.5	131	PASS
127	198	10	80	44.1	35410	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	80224	PASS
199	198	5	9	7.3	5890	PASS
275	198	10	60	26.6	21379	PASS
365	198	1	100	3.0	2439	PASS
441	198	0.01	100	12.0	9607	PASS
442	198	50	100	77.2	61973	PASS
443	442	15	24	20.0	12368	PASS