
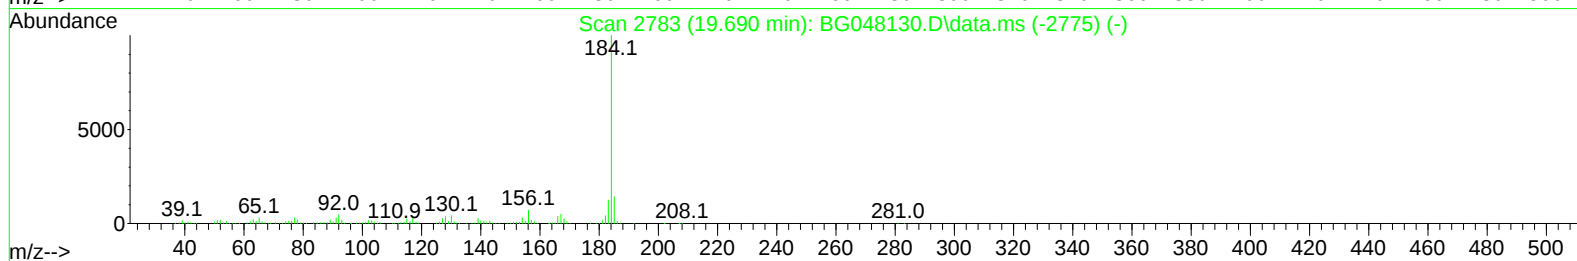
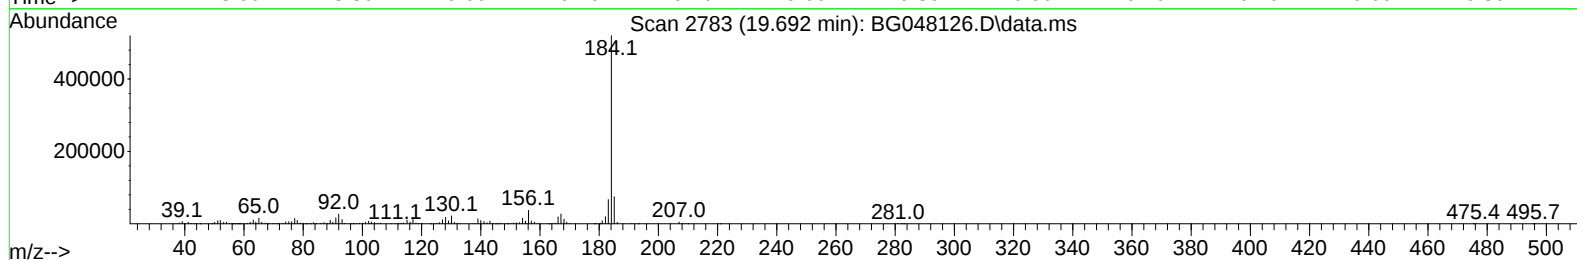


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG021021\
Data File : BG048126.D
Acq On : 10 Feb 2021 11:24
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Feb 10 13:27:18 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG021021.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Feb 10 13:22:14 2021
Response via : Initial Calibration

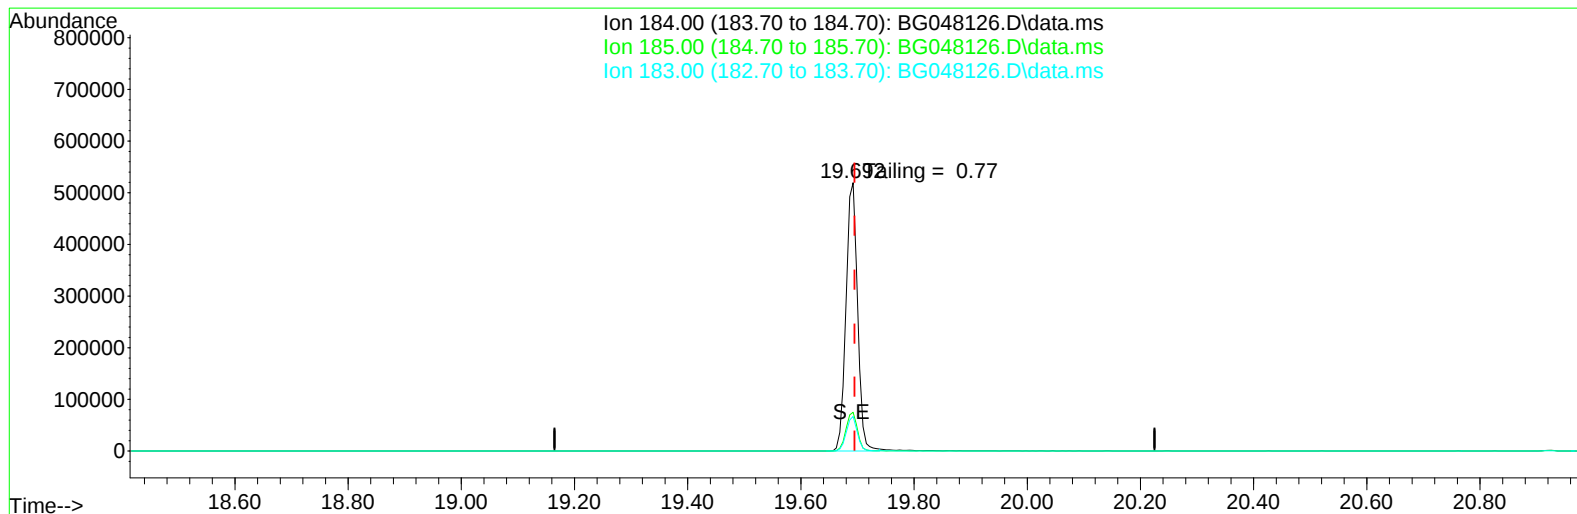

TIC: BG048126.D\data.ms

(77) Benzidine




19.692min (-0.002) 0.00 ng

response 740511

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	14.44
183.00	13.20	12.90
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG021021\
Data File : BG048126.D
Acq On : 10 Feb 2021 11:24
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Feb 10 13:27:18 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG021021.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Feb 10 13:22:14 2021
Response via : Initial Calibration

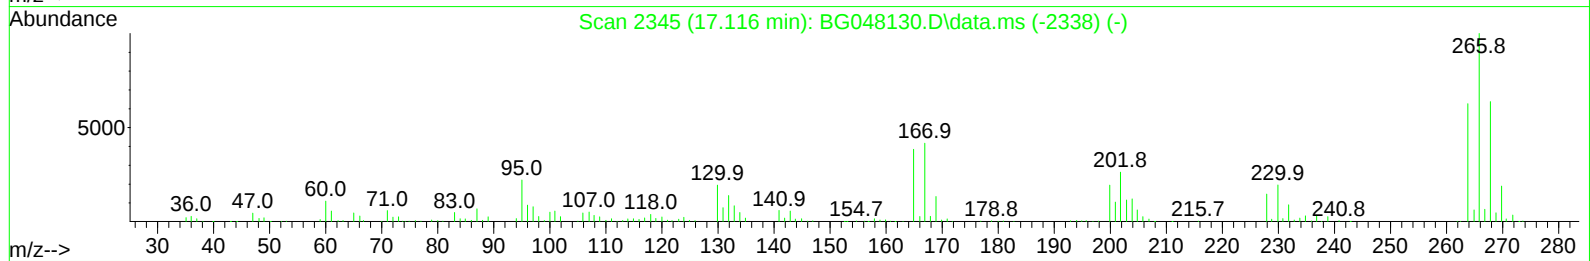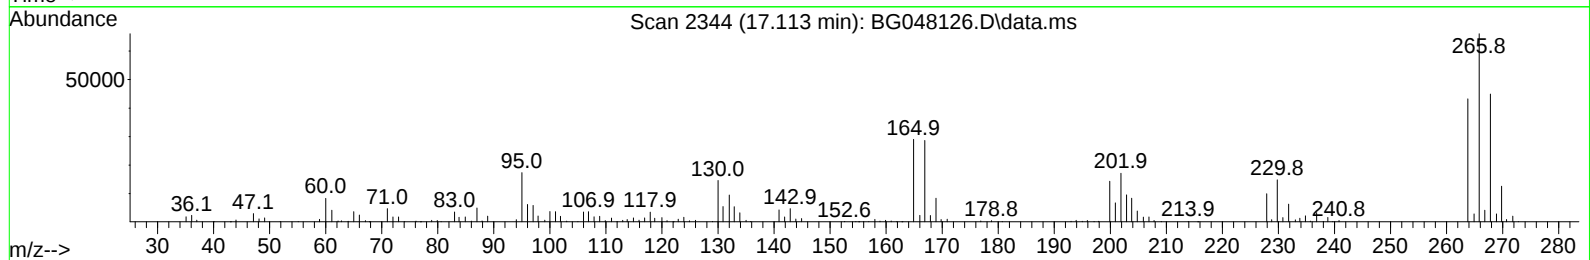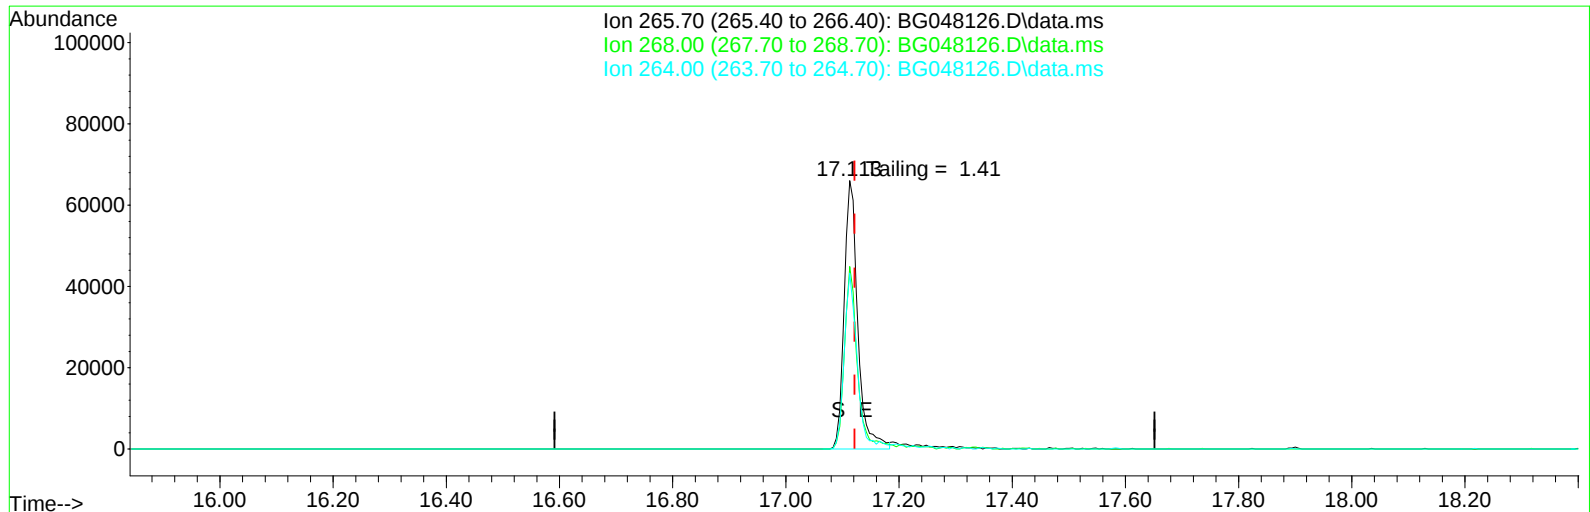

TIC: BG048126.D\data.ms

(70) Pentachlorophenol (C)

17.113min (-0.008) 19937.00 ng

response 113644

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	67.97
264.00	61.60	65.41
0.00	0.00	0.00