
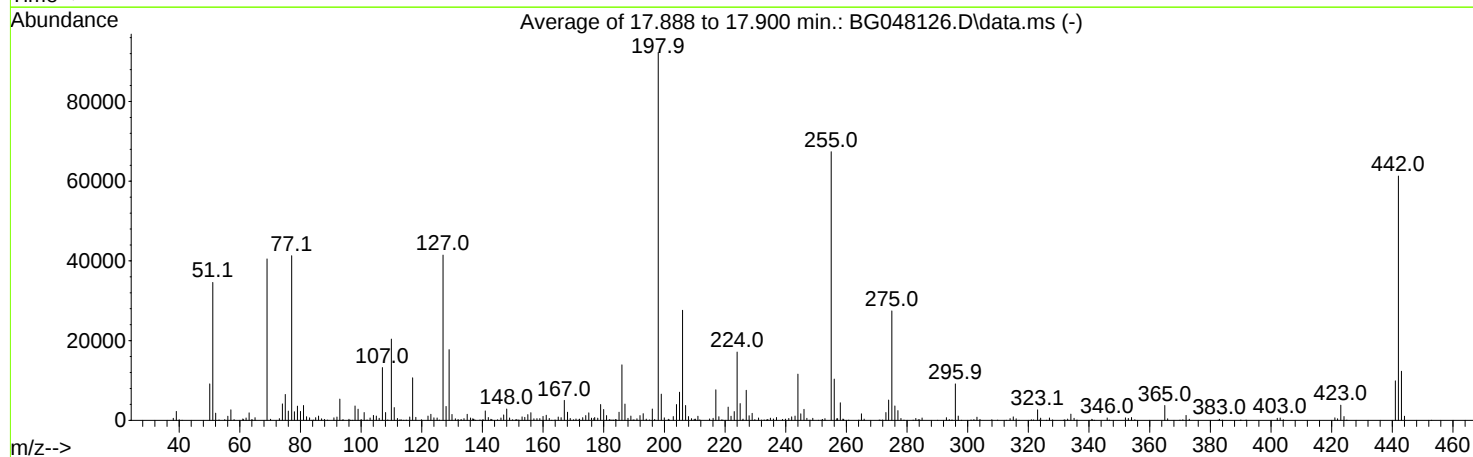


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG021021\
 Data File : BG048126.D
 Acq On : 10 Feb 2021 11:24
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG021021.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Feb 10 17:26:23 2021

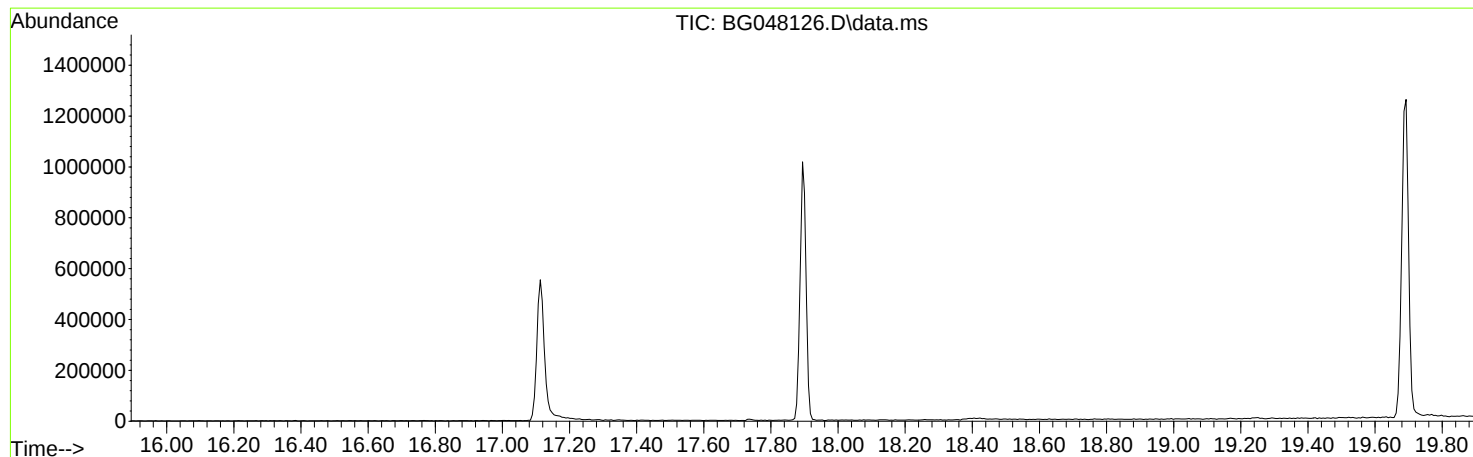

AutoFind: Scans 2476, 2477, 2478; Background Corrected with Scan 2470

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	37.5	34611	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	43.9	40501	PASS
70	69	0.00	2	0.7	285	PASS
127	198	10	80	44.9	41467	PASS
197	198	0.00	2	0.2	224	PASS
198	198	100	100	100.0	92283	PASS
199	198	5	9	7.1	6579	PASS
275	198	10	60	29.8	27467	PASS
365	198	1	100	4.1	3740	PASS
441	198	0.01	100	10.7	9913	PASS
442	198	50	100	66.4	61296	PASS
443	442	15	24	20.1	12315	PASS

Instrument :
BNA_G
ClientSampleId :
DFTPP




DDT Breakdown

Date	Instrument Name	DFTPP Data File
2/10/2021	BNA_G	<u>BG048126.D</u>
Compound Name	Response	Retention Time
DDT	388186	20.92
DDD	1781	20.52
DDE	542	19.97
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
2323	390509	0.59

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG021021\
Data File : BG048126.D
Acq On : 10 Feb 2021 11:24
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: Feb 10 13:27:18 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG021021.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Feb 10 13:22:14 2021
Response via : Initial Calibration

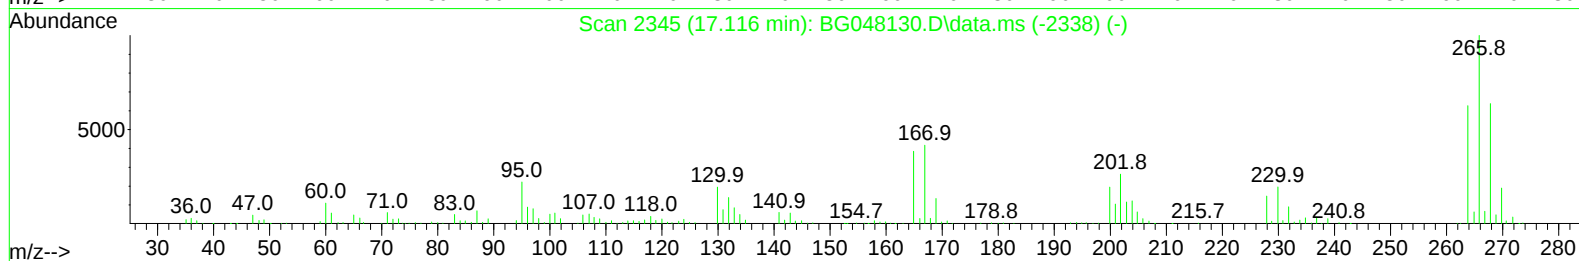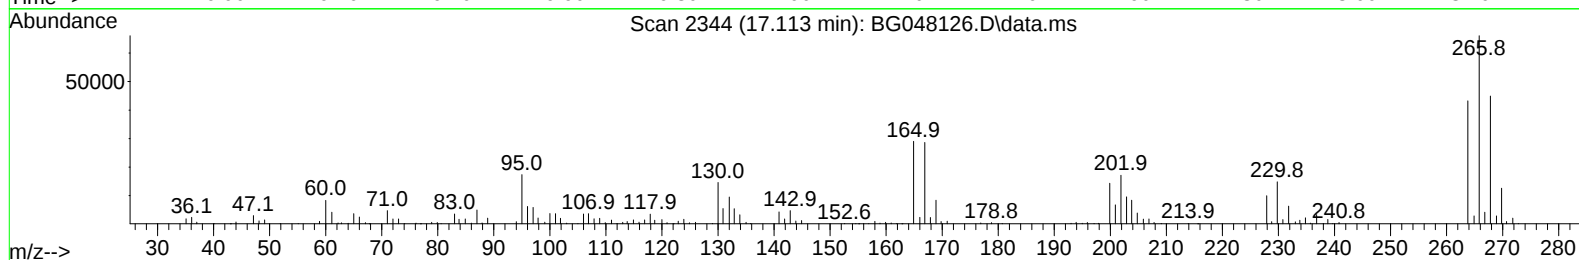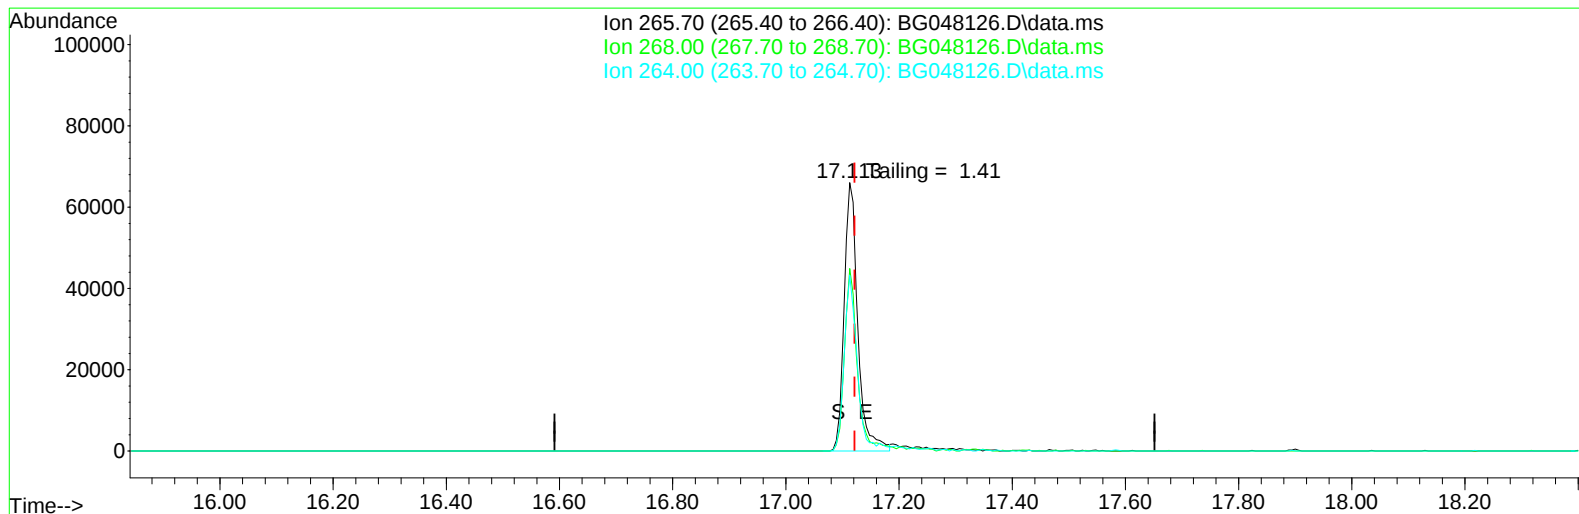

TIC: BG048126.D\data.ms

(70) Pentachlorophenol (C)

17.113min (-0.008) 19937.00 ng




response 113644

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	67.97
264.00	61.60	65.41
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG021021\
Data File : BG048126.D
Acq On : 10 Feb 2021 11:24
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: Feb 10 13:27:18 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG021021.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Feb 10 13:22:14 2021
Response via : Initial Calibration

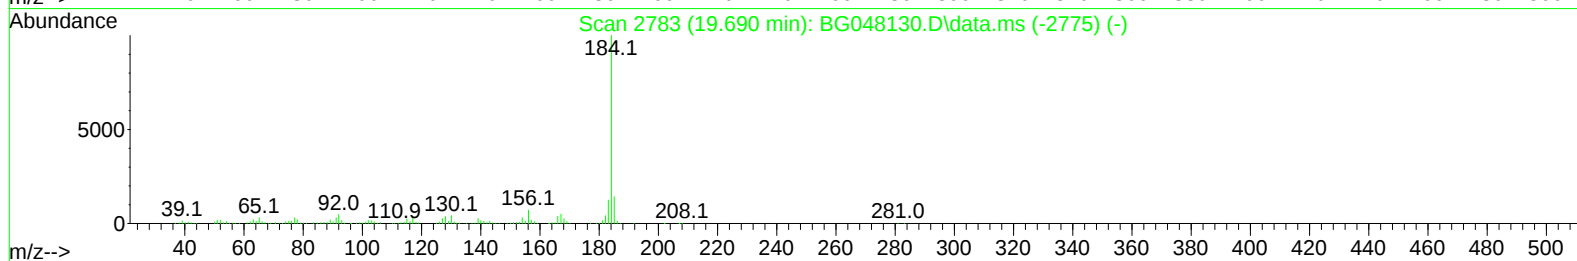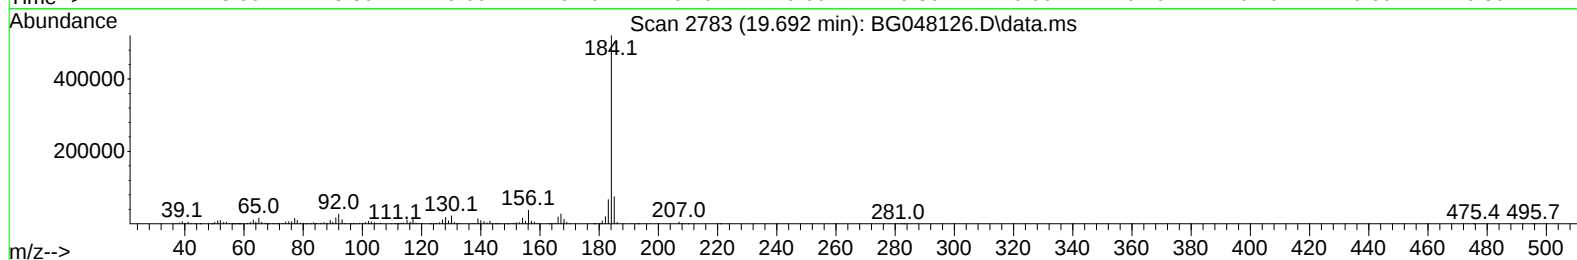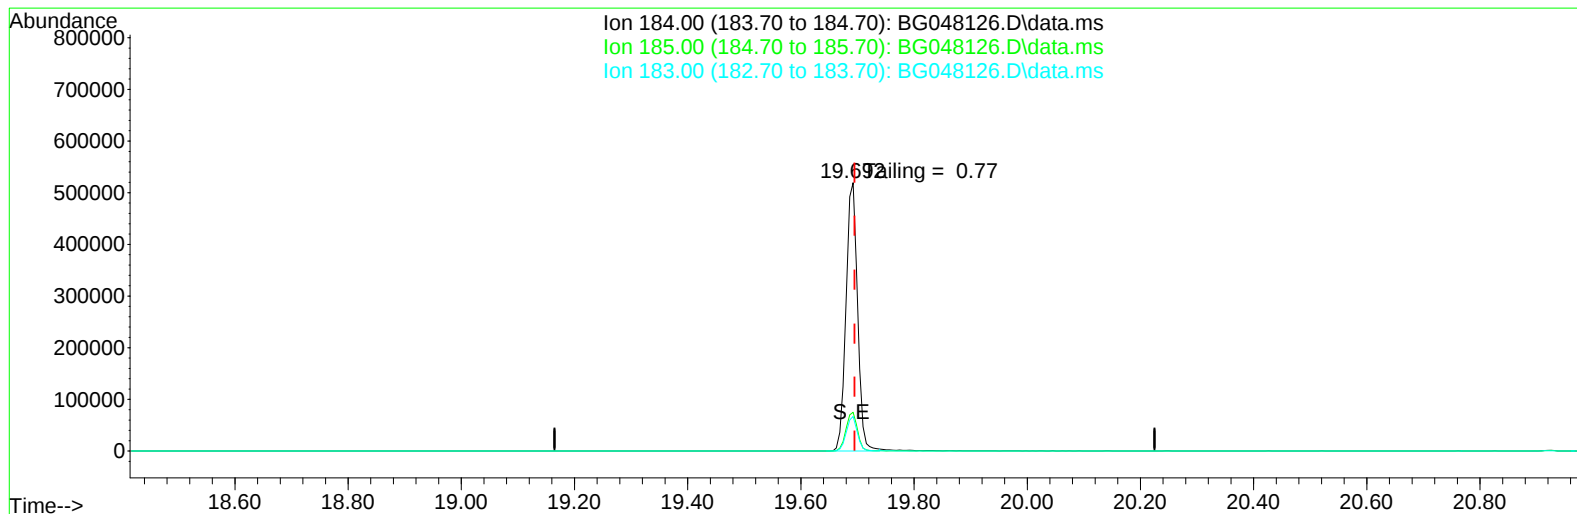

TIC: BG048126.D\data.ms

(77) Benzidine

19.692min (-0.002) 0.00 ng

response 740511

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	14.44
183.00	13.20	12.90
0.00	0.00	0.00