
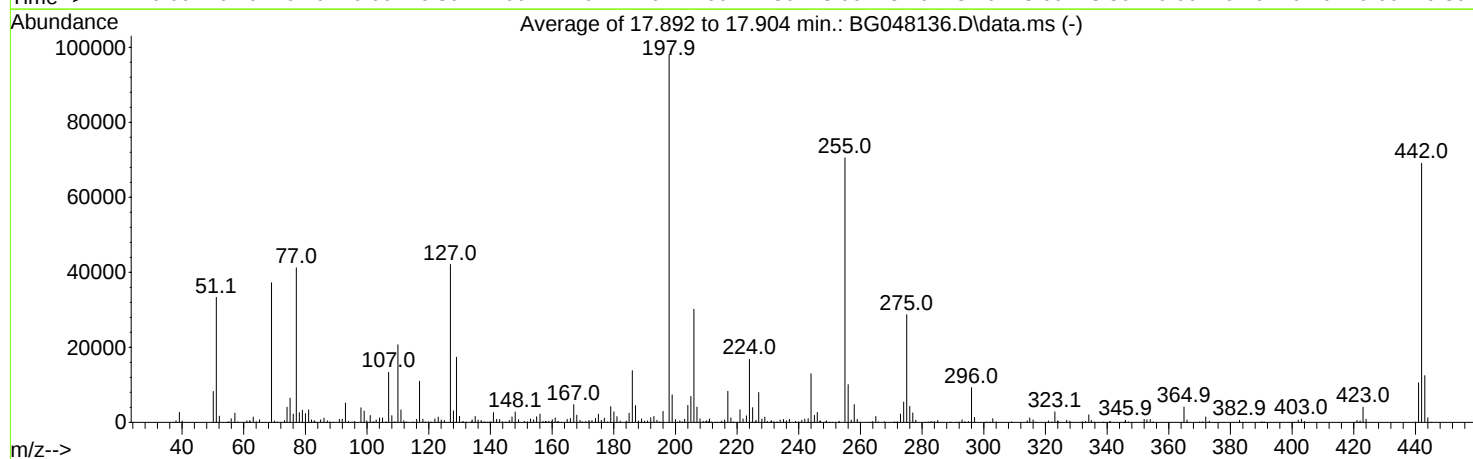


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG021121\
 Data File : BG048136.D
 Acq On : 11 Feb 2021 15:10
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG021021.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Feb 10 17:26:23 2021

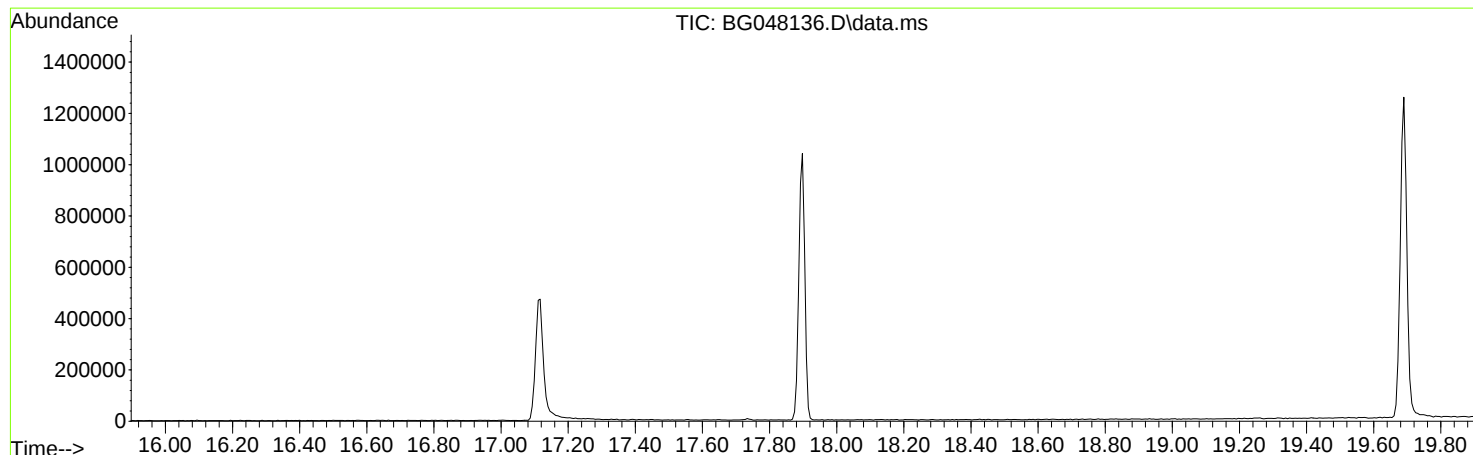

AutoFind: Scans 2477, 2478, 2479; Background Corrected with Scan 2469

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	34.0	33296	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	38.0	37221	PASS
70	69	0.00	2	0.9	331	PASS
127	198	10	80	42.9	42096	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	98069	PASS
199	198	5	9	7.5	7327	PASS
275	198	10	60	29.3	28723	PASS
365	198	1	100	4.2	4100	PASS
441	198	0.01	100	10.8	10555	PASS
442	198	50	100	70.4	69072	PASS
443	442	15	24	18.0	12449	PASS

Instrument :
BNA_G
ClientSampleId :
DFTPP




DDT Breakdown

Date	Instrument Name	DFTPP Data File
2/11/2021	BNA_G	<u>BG048136.D</u>
Compound Name	Response	Retention Time
DDT	379947	20.92
DDD	3139	20.47
DDE	596	19.99
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
3735	383682	0.97

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG021121\
Data File : BG048136.D
Acq On : 11 Feb 2021 15:10
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: Feb 11 16:23:21 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG021021.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Feb 10 17:26:23 2021
Response via : Initial Calibration

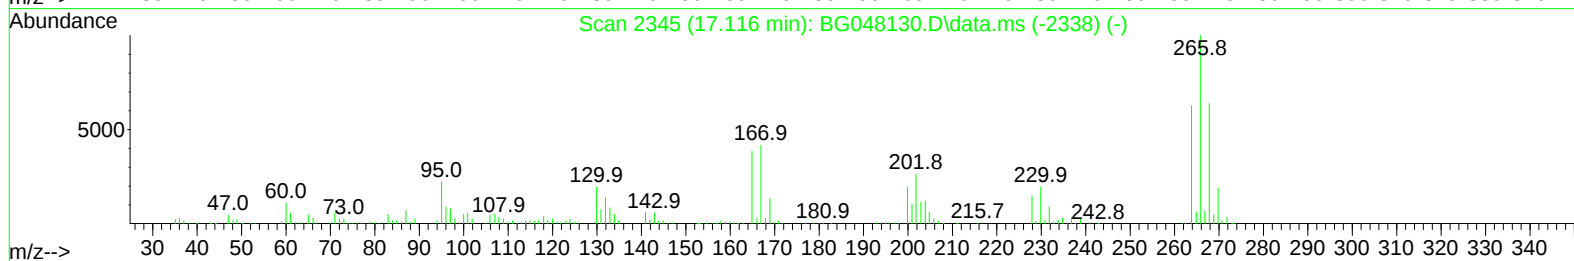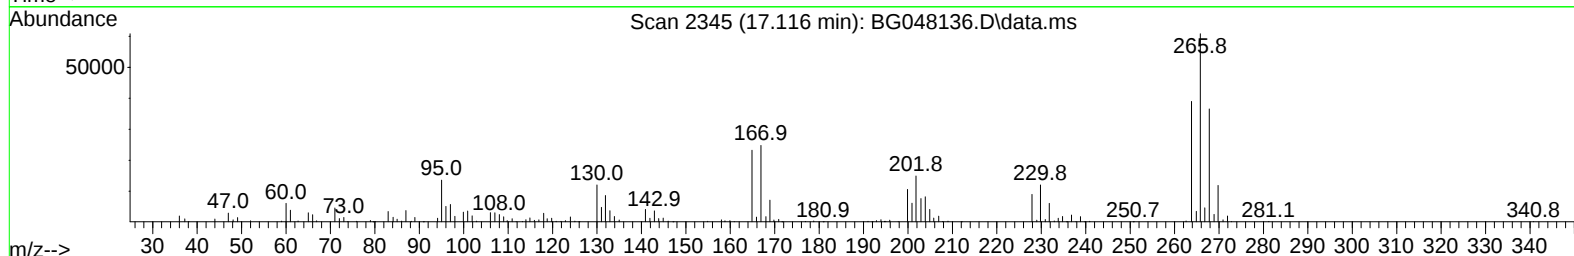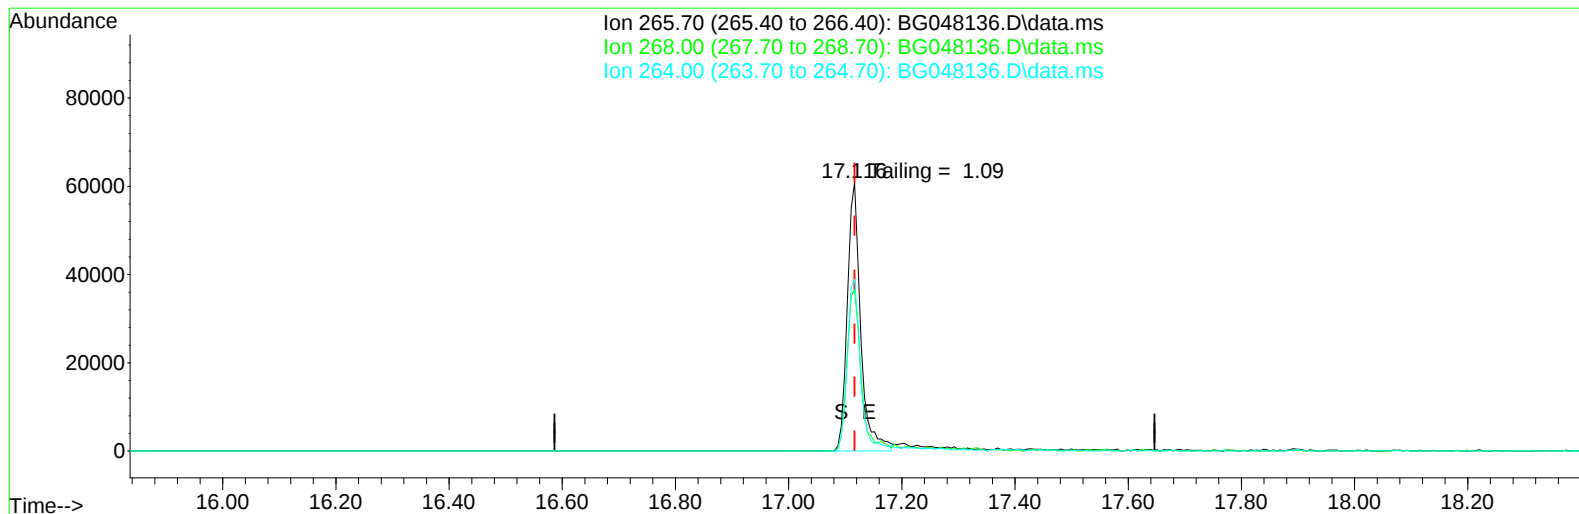

TIC: BG048136.D\data.ms

(70) Pentachlorophenol (C)

17.116min (+ 0.000) 159538.67 ng




response 101303

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	60.09
264.00	61.60	64.07
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG021121\
Data File : BG048136.D
Acq On : 11 Feb 2021 15:10
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: Feb 11 16:23:21 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG021021.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Feb 10 17:26:23 2021
Response via : Initial Calibration

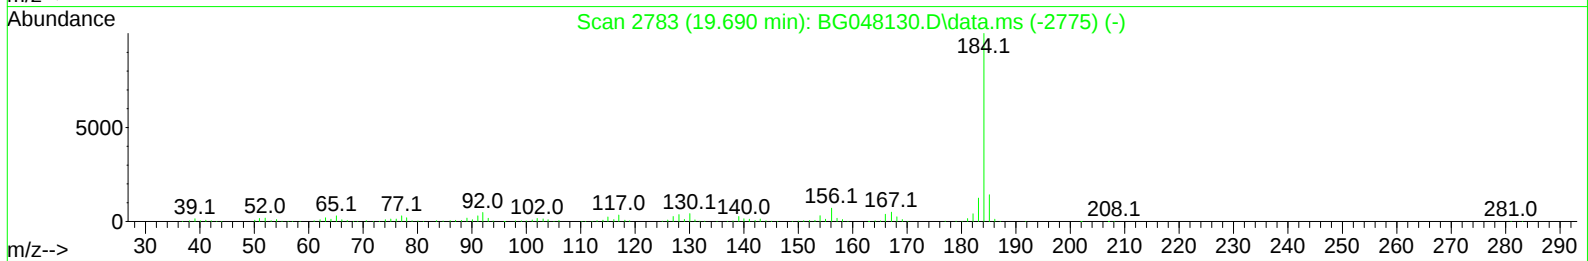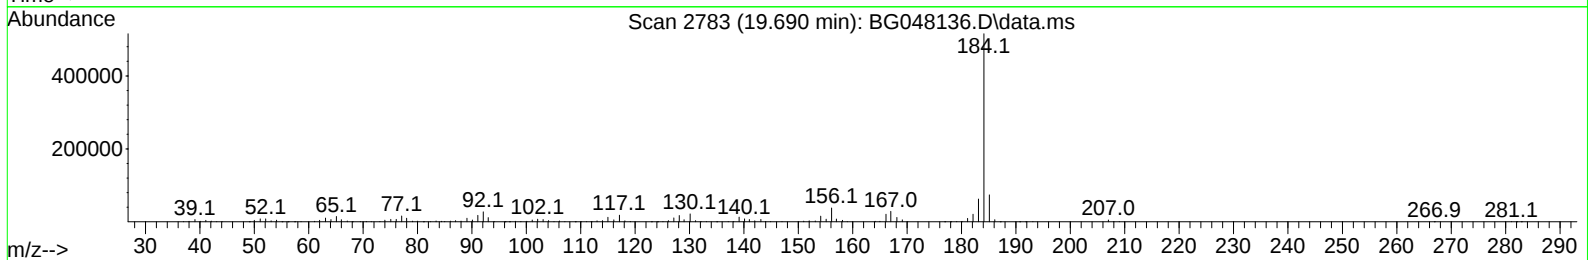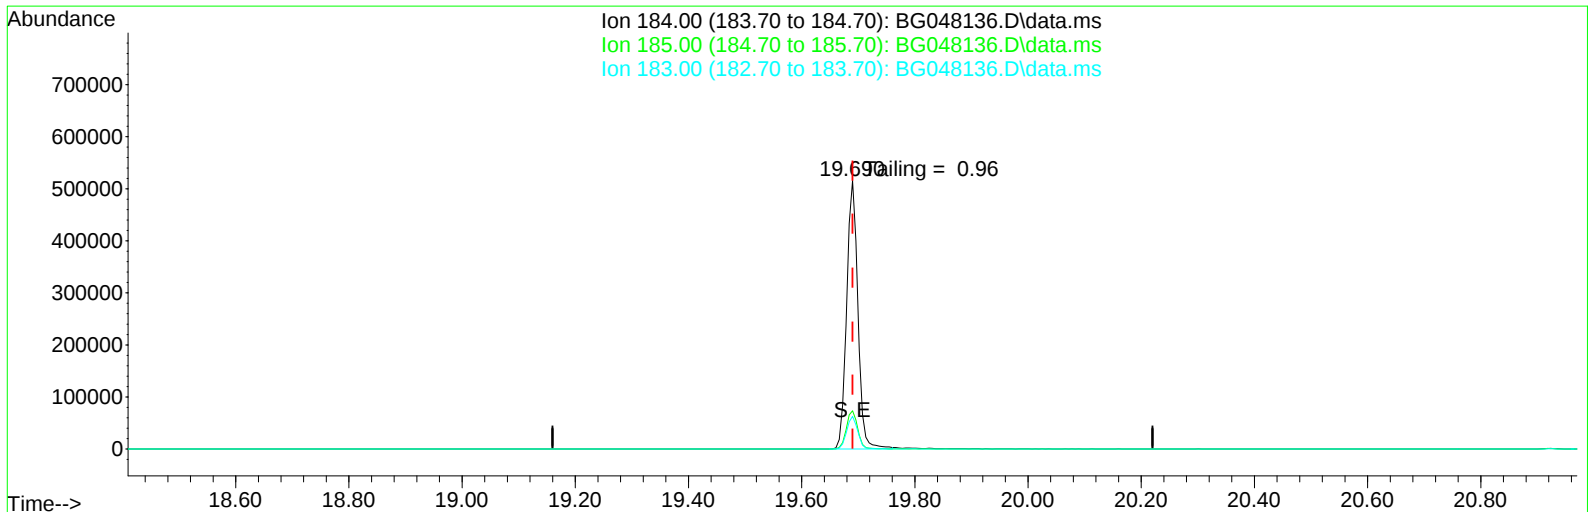

TIC: BG048136.D\data.ms

(77) Benzidine

19.690min (+ 0.000) 321012.44 ng

response 713243

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	14.29
183.00	13.20	12.16
0.00	0.00	0.00