
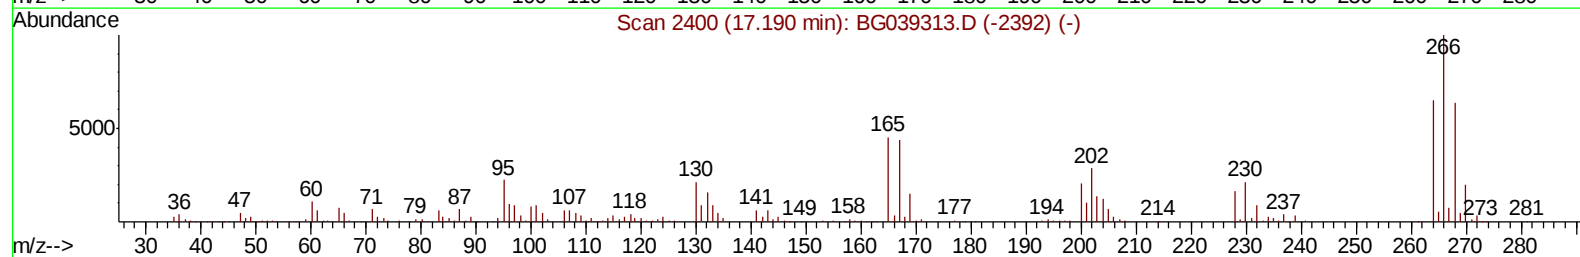
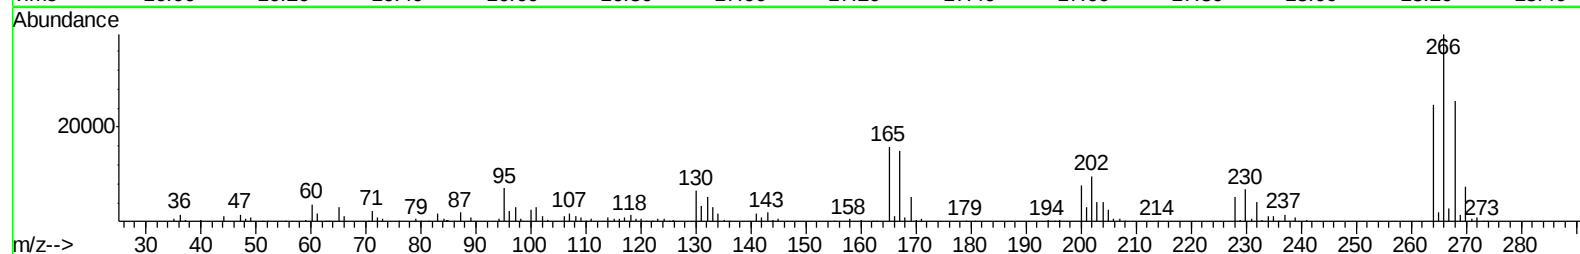


Data Path : Z:\SVOASRV\HPCHEM1\BNA_G\DATA\BG021119\
Data File : BG039430.D
Acq On : 11 Feb 2019 12:20
Operator : JU/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Feb 12 06:20:00 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG012919.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jan 29 15:41:51 2019
Response via : Initial Calibration

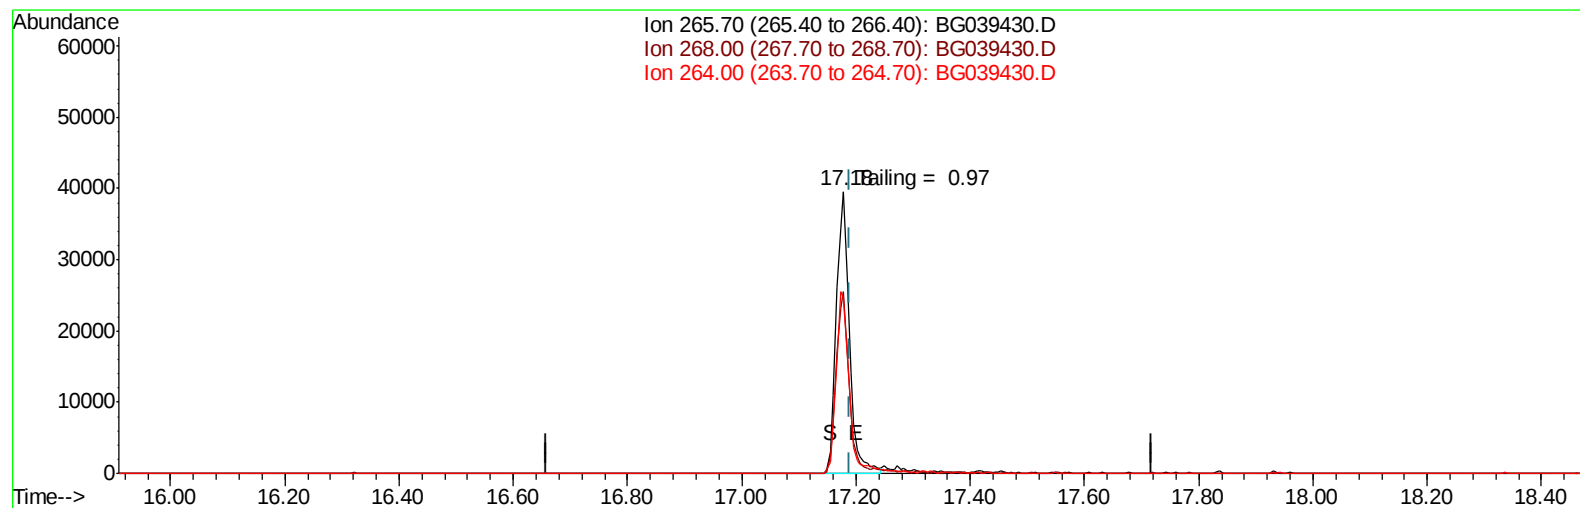

TIC: BG039430.D

(70) Pentachlorophenol (C)




17.178min (-0.011) 60159.93ng

response 61897

Ion	Exp%	Act%
265.70	100	100
268.00	63.90	64.50
264.00	65.10	62.45
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA_G\DATA\BG021119\
 Data File : BG039430.D
 Acq On : 11 Feb 2019 12:20
 Operator : JU/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Feb 12 06:20:00 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG012919.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Jan 29 15:41:51 2019
 Response via : Initial Calibration

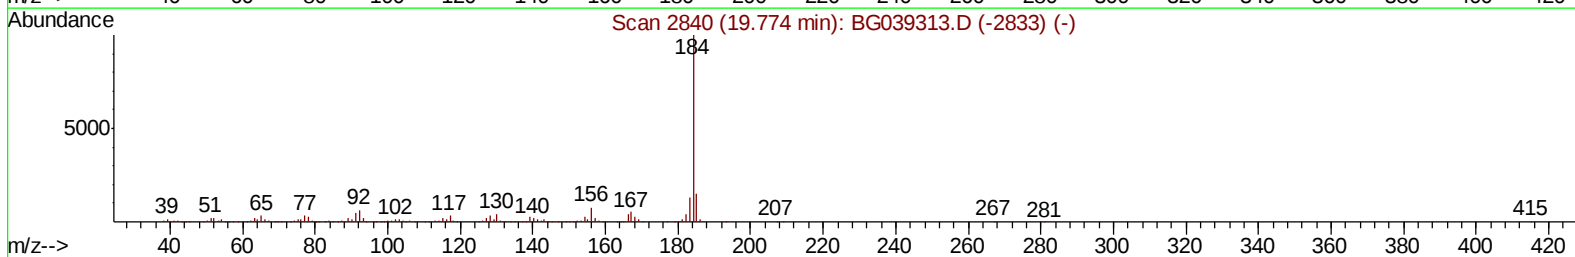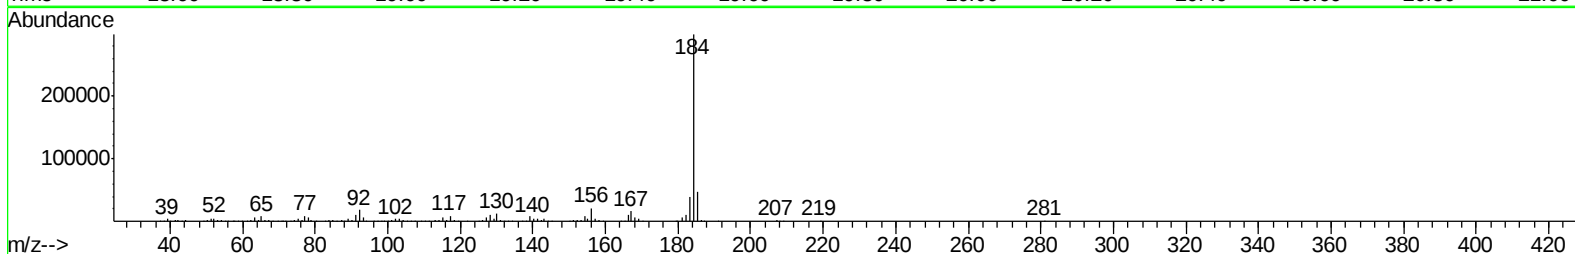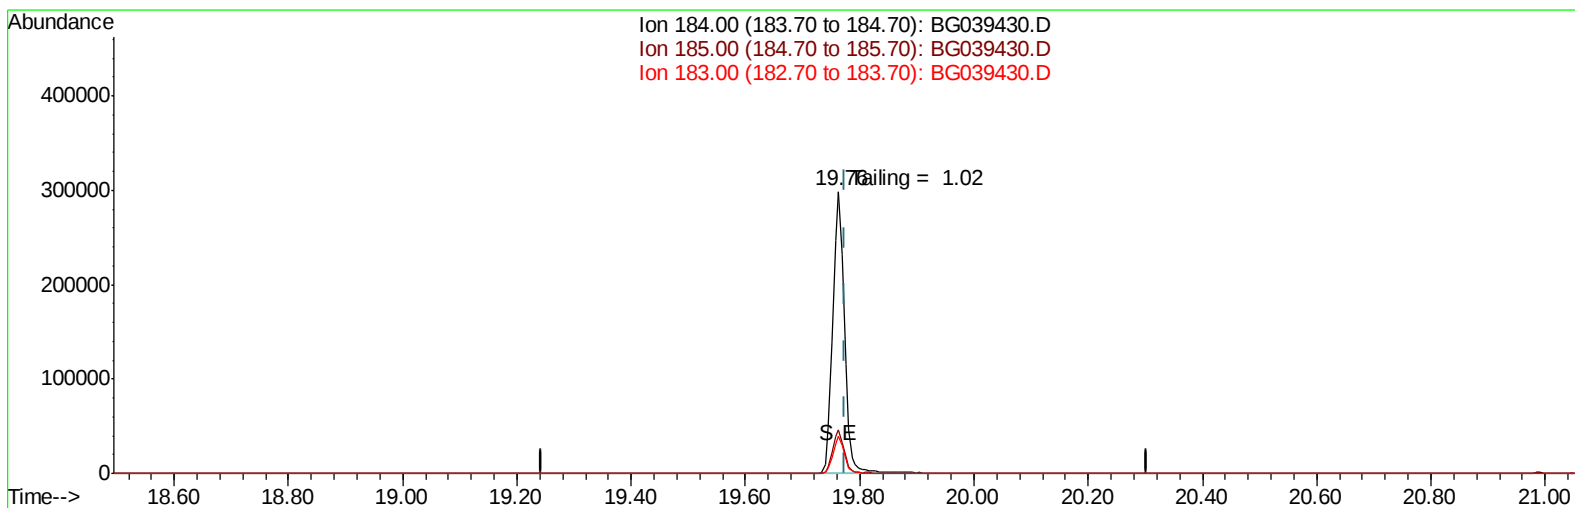

TIC: BG039430.D

(77) Benzidine

19.763min (-0.011) 109454.35ng

response 423446

Ion	Exp%	Act%
184.00	100	100
185.00	15.20	15.53
183.00	13.20	13.07
0.00	0.00	0.00