
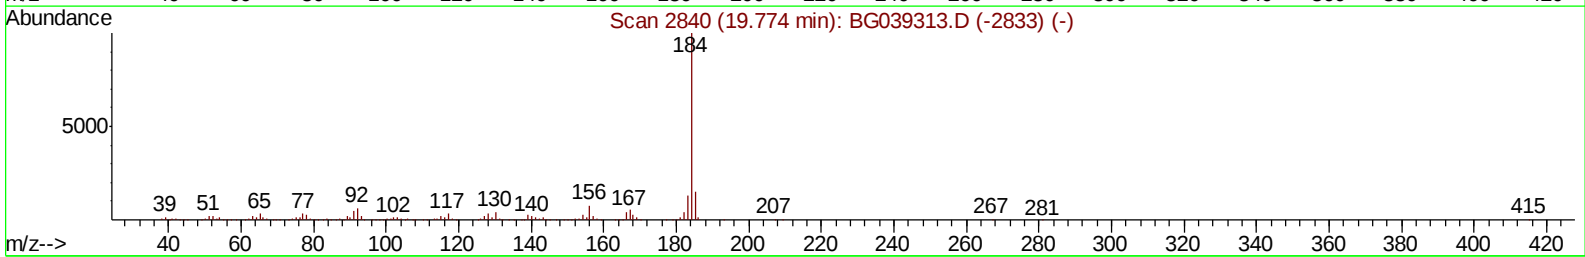
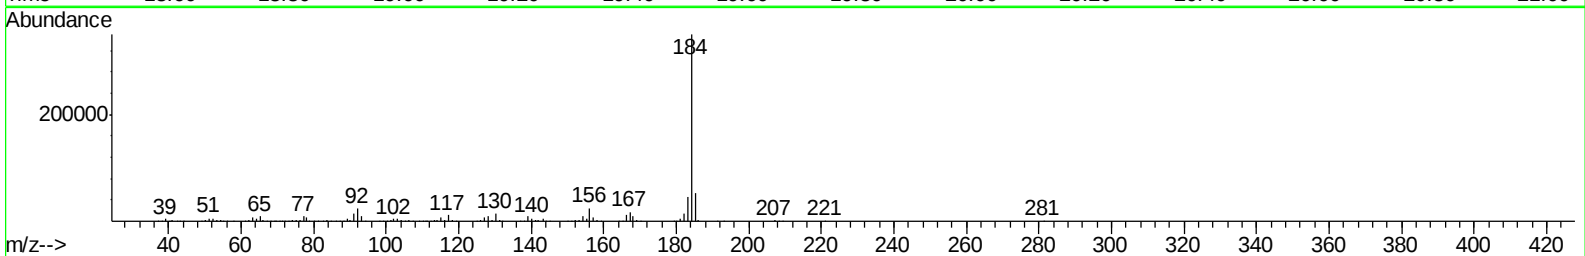


Data Path : Z:\SVOASRV\HPCHEM1\BNA_G\DATA\BG021119\
Data File : BG039450.D
Acq On : 12 Feb 2019 1:22
Operator : JU/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Feb 12 06:18:06 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG012919.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jan 29 15:41:51 2019
Response via : Initial Calibration

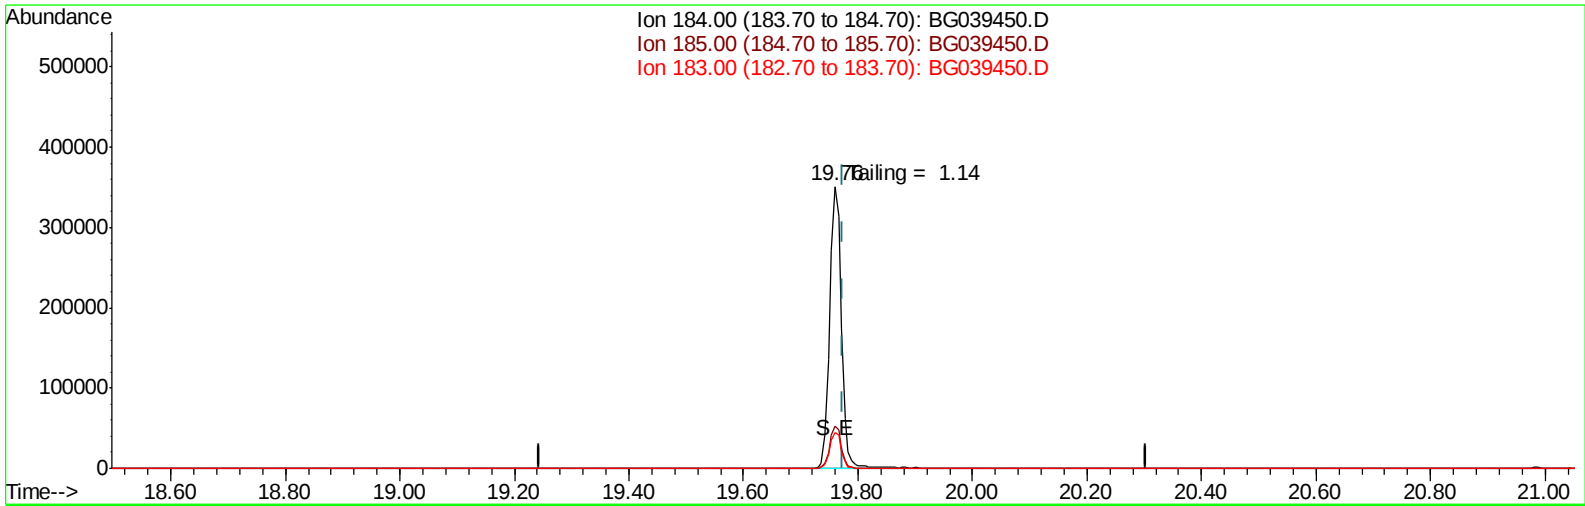

TIC: BG039450.D

(77) Benzidine




19.760min (-0.015) 115600.49ng

response 500284

Ion	Exp%	Act%
184.00	100	100
185.00	15.20	14.95
183.00	13.20	12.88
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA_G\DATA\BG021119\
Data File : BG039450.D
Acq On : 12 Feb 2019 1:22
Operator : JU/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Feb 12 06:18:06 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG012919.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jan 29 15:41:51 2019
Response via : Initial Calibration

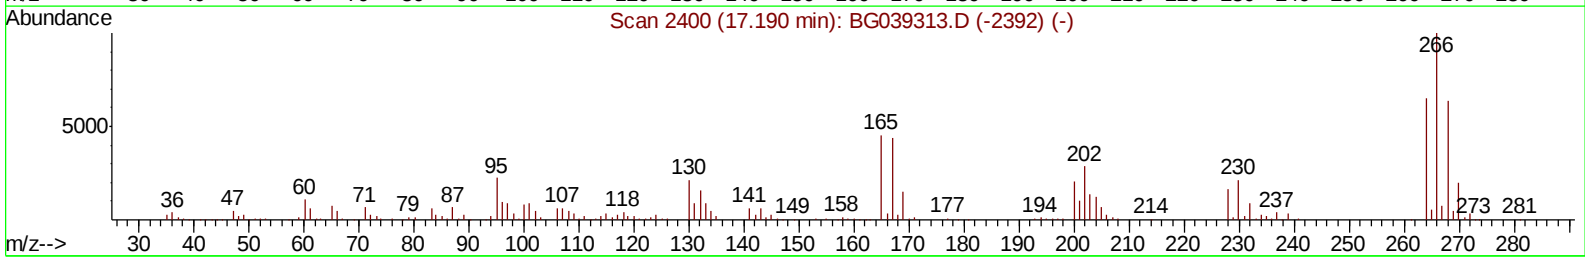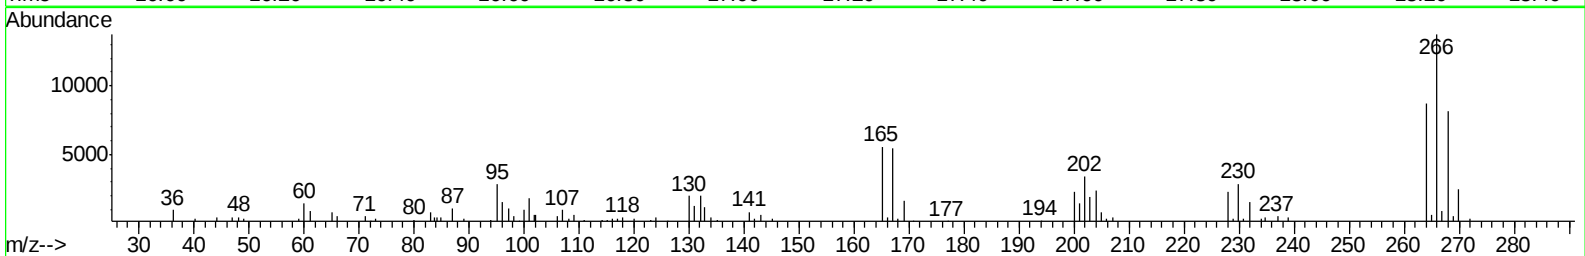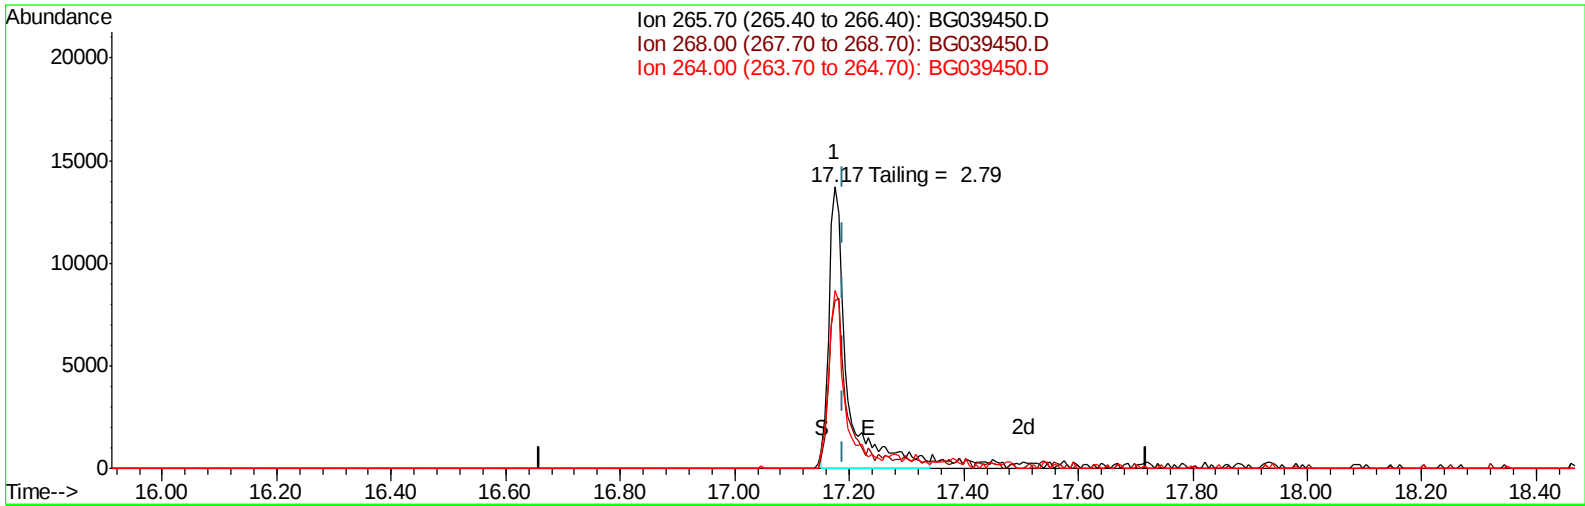

TIC: BG039450.D

(70) Pentachlorophenol (C)

17.175min (-0.015) 24485.82ng m

response 30686

Ion	Exp%	Act%
265.70	100	100
268.00	63.90	59.63
264.00	65.10	63.16
0.00	0.00	0.00