
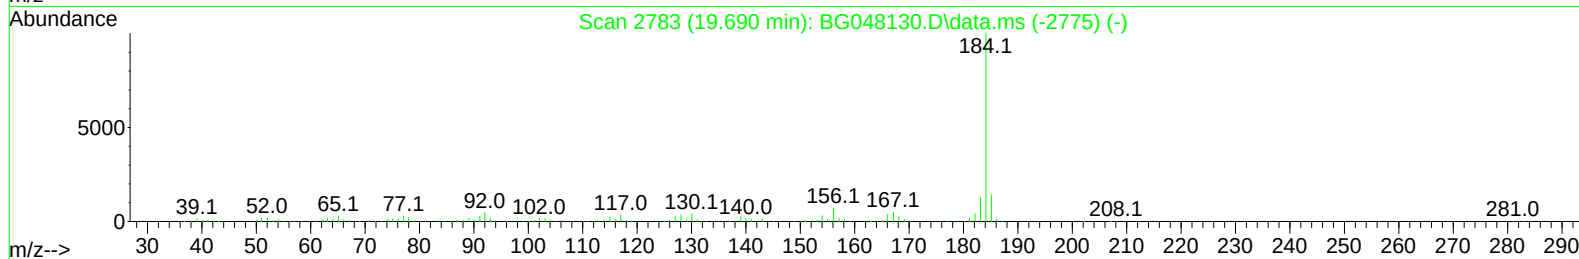
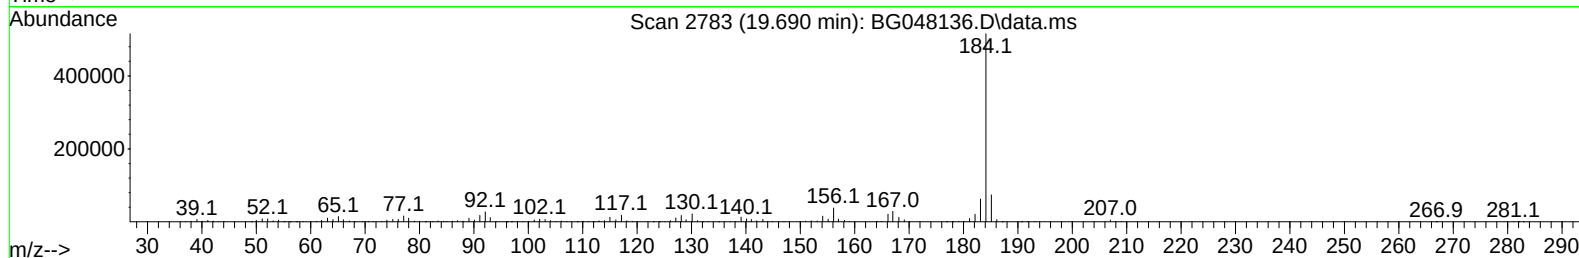


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG021121\
Data File : BG048136.D
Acq On : 11 Feb 2021 15:10
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Feb 11 16:23:21 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG021021.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Feb 10 17:26:23 2021
Response via : Initial Calibration

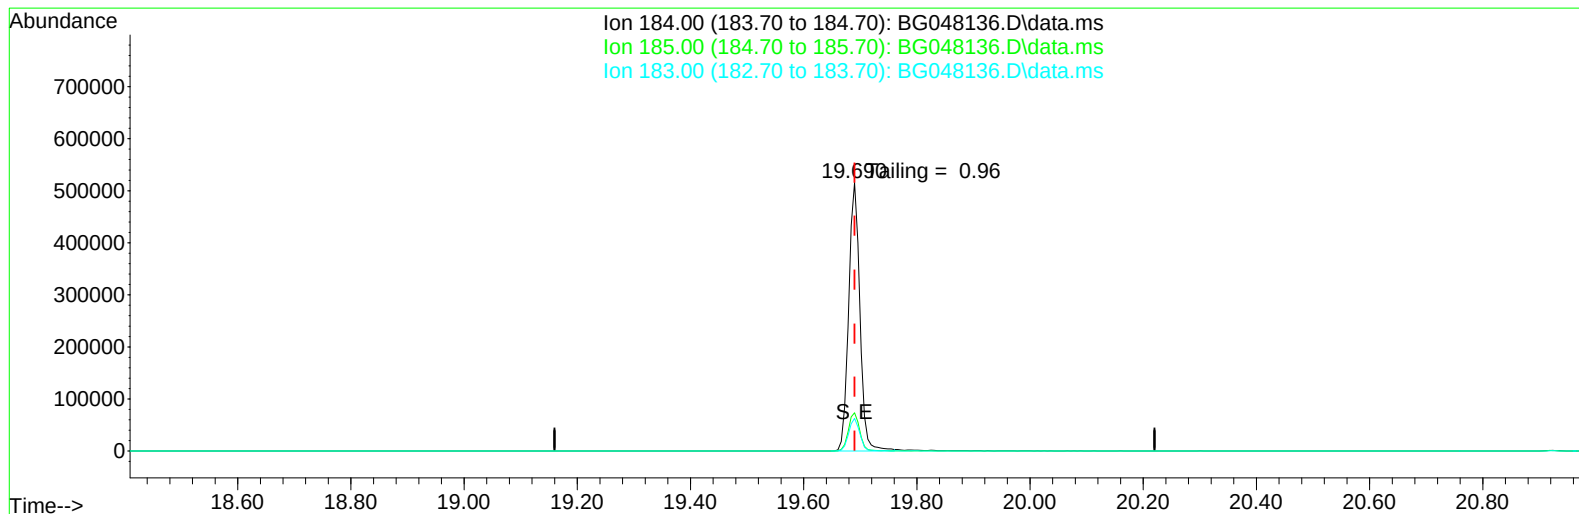

TIC: BG048136.D\data.ms

(77) Benzidine




19.690min (+ 0.000) 321012.44 ng

response 713243

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	14.29
183.00	13.20	12.16
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG021121\
Data File : BG048136.D
Acq On : 11 Feb 2021 15:10
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Feb 11 16:23:21 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG021021.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Feb 10 17:26:23 2021
Response via : Initial Calibration

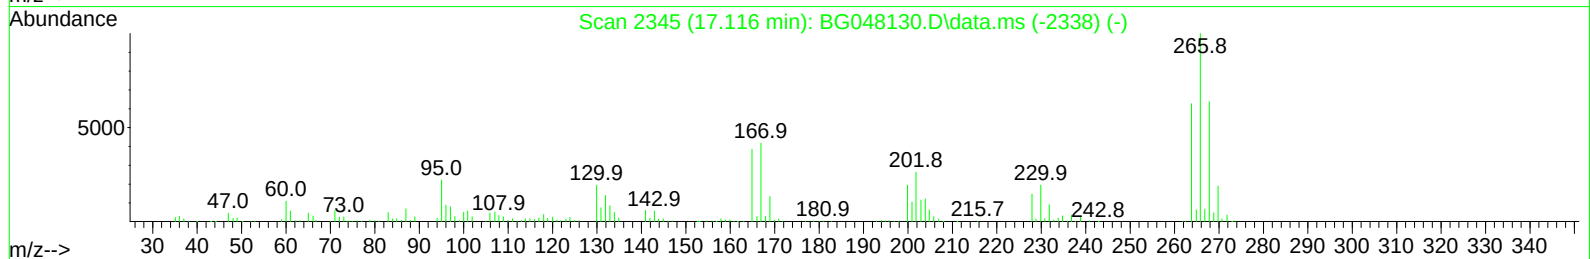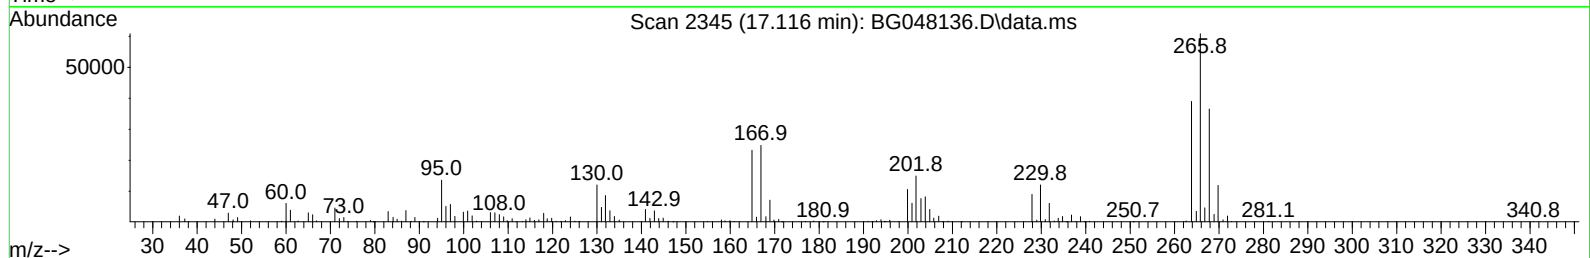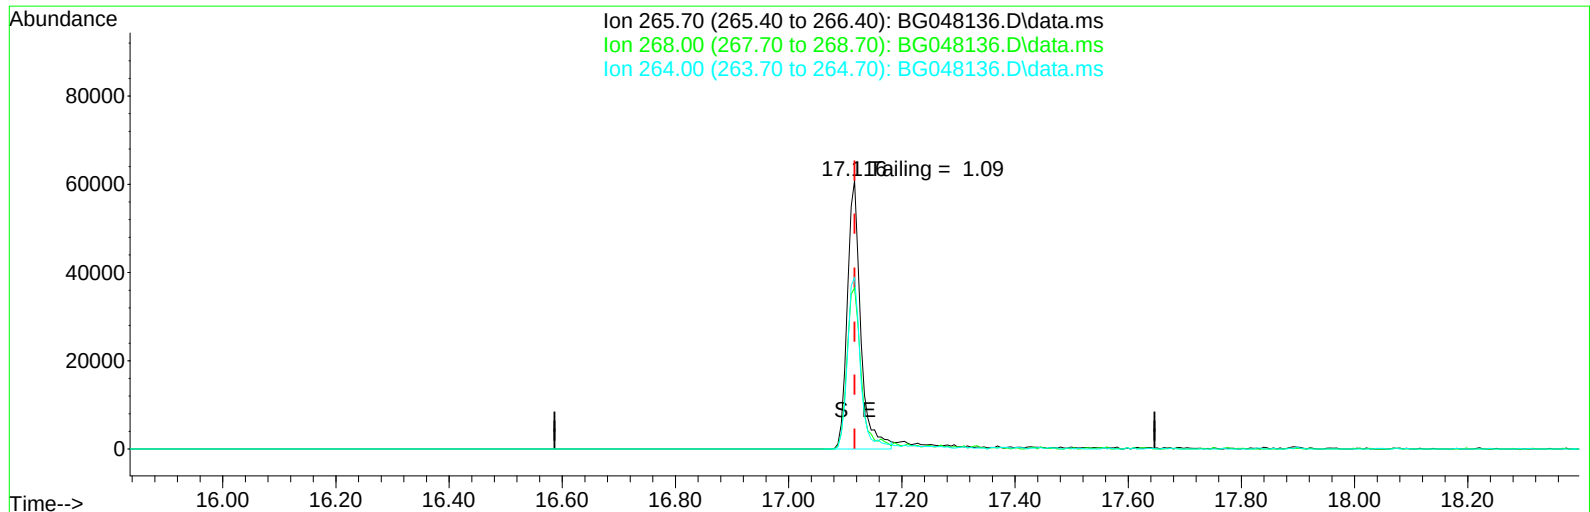

TIC: BG048136.D\data.ms

(70) Pentachlorophenol (C)

17.116min (+ 0.000) 159538.67 ng

response 101303

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	60.09
264.00	61.60	64.07
0.00	0.00	0.00