

Data Path : Z:\svoasrv\HPCHEM1\BNA\_G\Data\BG021121\  
 Data File : BG048138.D  
 Acq On : 11 Feb 2021 16:31  
 Operator : CG/JU  
 Sample : PB134579BL  
 Misc :  
 ALS Vial : 3 Sample Multiplier: 1

Instrument :  
 BNA\_G  
 ClientSampleId :  
 PB134579BL

Integration Parameters: rteint.p  
 Integrator: RTE  
 Smoothing : ON Filtering: 5  
 Sampling : 1 Min Area: 3 % of largest Peak  
 Start Thrs: 0.2 Max Peaks: 100  
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >  
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA\_G\METHODS\8270-BG021021.M  
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BG048138.D\data.ms

| peak<br># | R.T.<br>min | first<br>scan | max<br>scan | last<br>scan | PK<br>TY | peak<br>height | corr.<br>area | corr.<br>% max. | % of<br>total |
|-----------|-------------|---------------|-------------|--------------|----------|----------------|---------------|-----------------|---------------|
| 1         | 5.656       | 387           | 394         | 407          | rBV      | 872351         | 1382310       | 29.03%          | 8.282%        |
| 2         | 7.248       | 658           | 665         | 679          | rBV      | 852740         | 1473445       | 30.95%          | 8.828%        |
| 3         | 8.100       | 802           | 810         | 818          | rBV2     | 159085         | 264469        | 5.55%           | 1.585%        |
| 4         | 9.264       | 999           | 1008        | 1017         | rBV      | 526623         | 927513        | 19.48%          | 5.557%        |
| 5         | 10.915      | 1280          | 1289        | 1298         | rBV      | 203376         | 365386        | 7.67%           | 2.189%        |
| 6         | 13.353      | 1697          | 1704        | 1714         | rBV      | 1456361        | 2157412       | 45.31%          | 12.926%       |
| 7         | 14.728      | 1931          | 1938        | 1946         | rVB      | 353454         | 559912        | 11.76%          | 3.355%        |
| 8         | 16.208      | 2183          | 2190        | 2205         | rBV      | 1243213        | 1917302       | 40.27%          | 11.487%       |
| 9         | 17.466      | 2397          | 2404        | 2412         | rBV      | 542459         | 815193        | 17.12%          | 4.884%        |
| 10        | 20.068      | 2841          | 2847        | 2854         | rBV      | 3686277        | 4761131       | 100.00%         | 28.525%       |
| 11        | 21.737      | 3124          | 3131        | 3137         | rBV      | 688719         | 1059780       | 22.26%          | 6.349%        |
| 12        | 25.004      | 3677          | 3687        | 3698         | rVB2     | 345491         | 1006974       | 21.15%          | 6.033%        |




Sum of corrected areas: 16690827

Data Path : Z:\svoasrv\HPCHEM1\BNA\_G\Data\BG021121\  
Data File : BG048138.D  
Acq On : 11 Feb 2021 16:31  
Operator : CG/JU  
Sample : PB134579BL  
Misc :  
ALS Vial : 3 Sample Multiplier: 1

Instrument :  
BNA\_G  
ClientSampleId :  
PB134579BL

Quant Method : Z:\SVOASRV\HPCHEM1\BNA\_G\METHODS\8270-BG021021.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST11.L  
TIC Integration Parameters: LSCINT.P

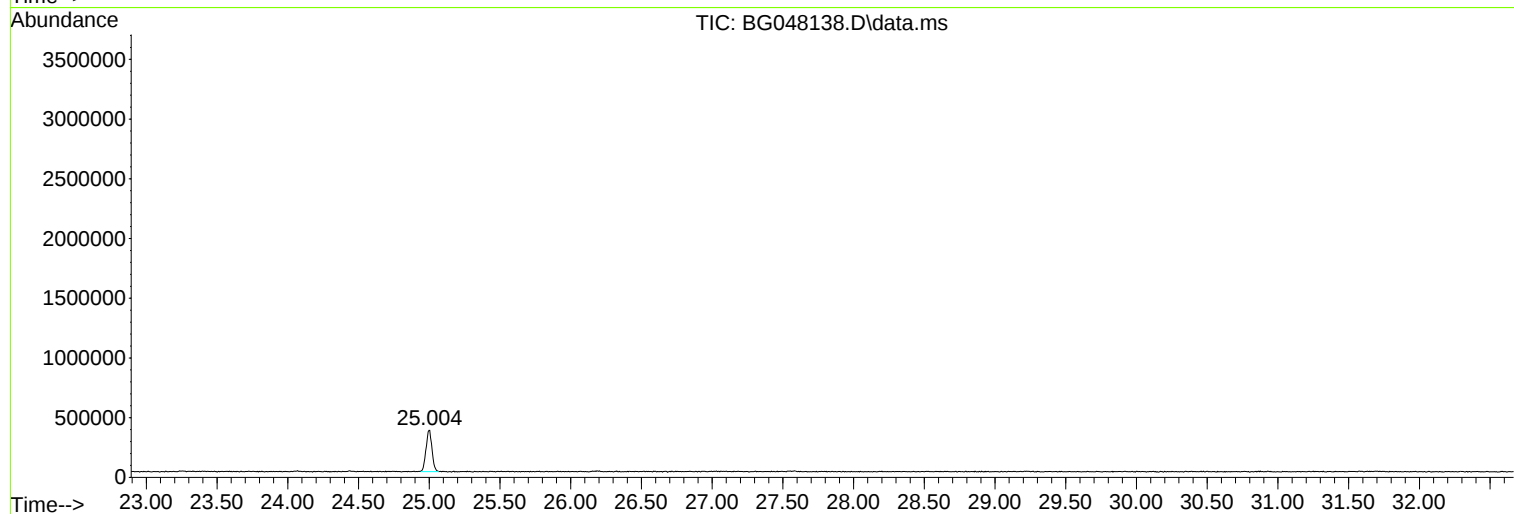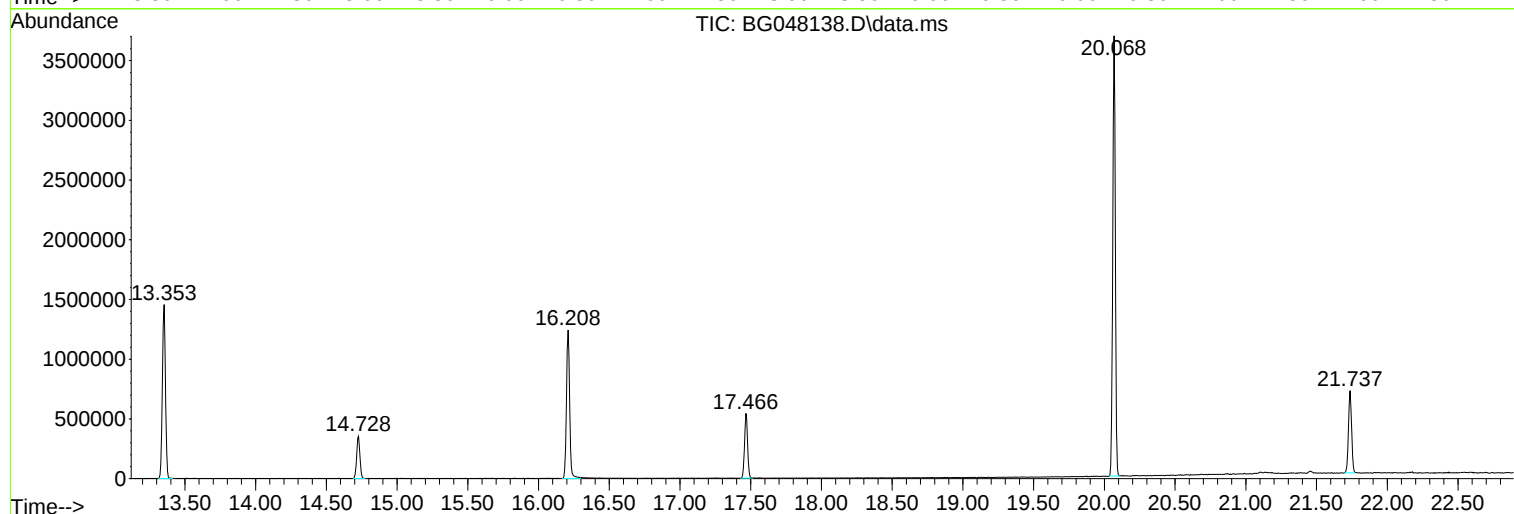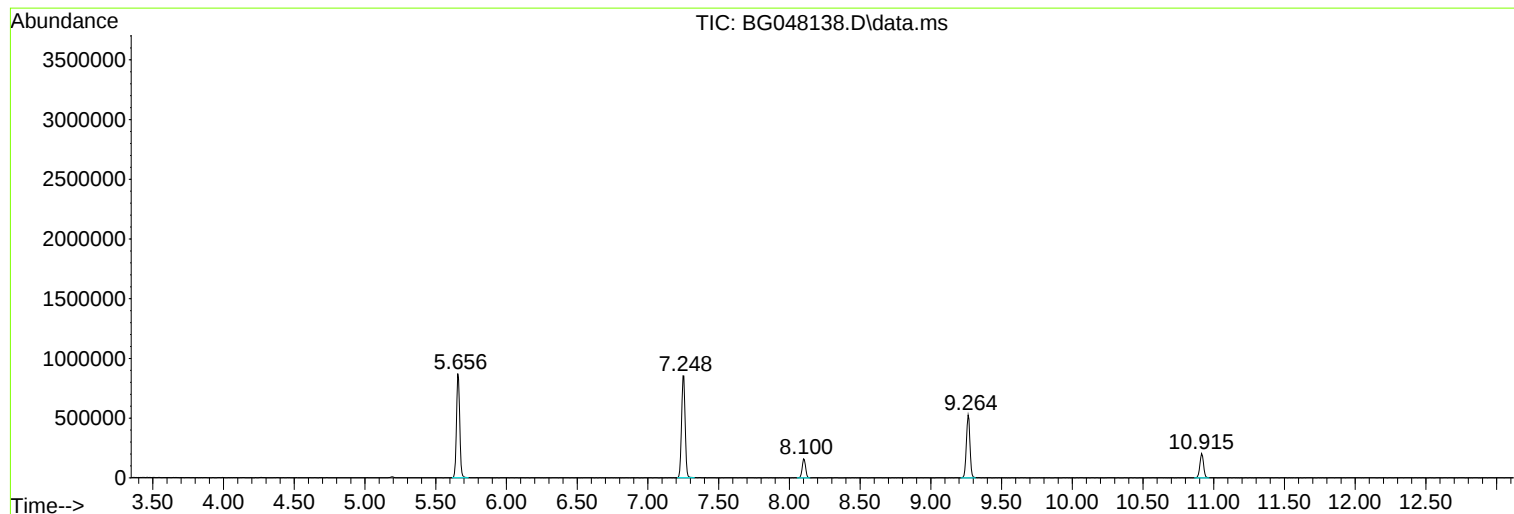

Data Path : Z:\svoasrv\HPCHEM1\BNA\_G\Data\BG021121\  
Data File : BG048138.D  
Acq On : 11 Feb 2021 16:31  
Operator : CG/JU  
Sample : PB134579BL  
Misc :  
ALS Vial : 3 Sample Multiplier: 1

Instrument :  
BNA\_G  
ClientSampleId :  
PB134579BL

Quant Method : Z:\SVOASRV\HPCHEM1\BNA\_G\METHODS\8270-BG021021.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST11.L  
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

\*\*\*\*\*

Data Path : Z:\svoasrv\HPCHEM1\BNA\_G\Data\BG021121\  
Data File : BG048138.D  
Acq On : 11 Feb 2021 16:31  
Operator : CG/JU  
Sample : PB134579BL  
Misc :  
ALS Vial : 3 Sample Multiplier: 1

Instrument :  
BNA\_G  
ClientSampleId :  
PB134579BL

Quant Method : Z:\SVOASRV\HPCHEM1\BNA\_G\METHODS\8270-BG021021.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST11.L  
TIC Integration Parameters: LSCINT.P

| TIC Top Hit name | RT | EstConc | Units | Response | # | RT | Resp | Conc |
|------------------|----|---------|-------|----------|---|----|------|------|
|------------------|----|---------|-------|----------|---|----|------|------|