
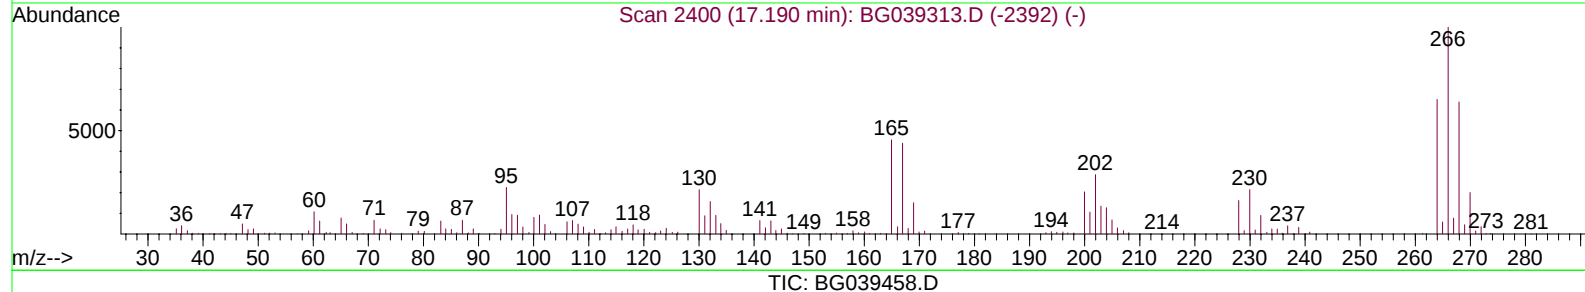
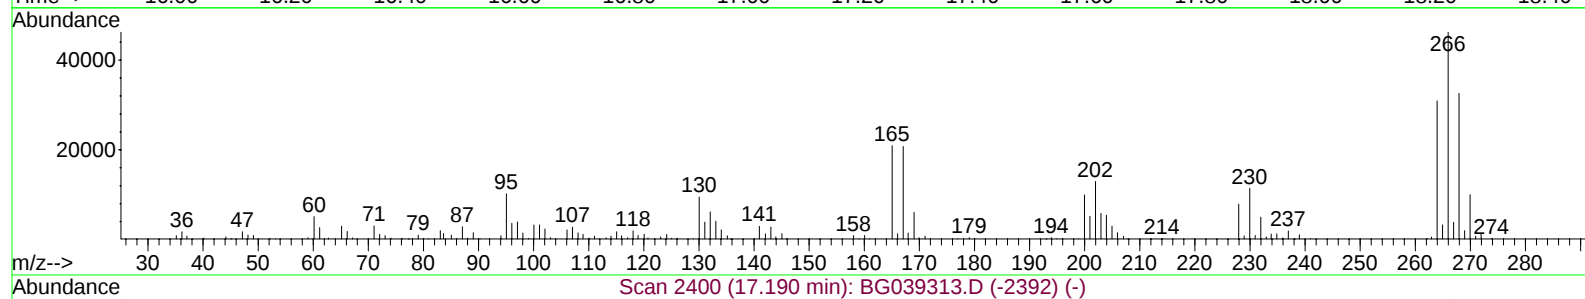


Data Path : Z:\svoasrv\HPCHEM1\BNA G\Data\BG021219\
Data File : BG039458.D
Acq On : 12 Feb 2019 11:14
Operator : JU/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Feb 12 17:54:56 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG012919.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jan 29 15:41:51 2019
Response via : Initial Calibration

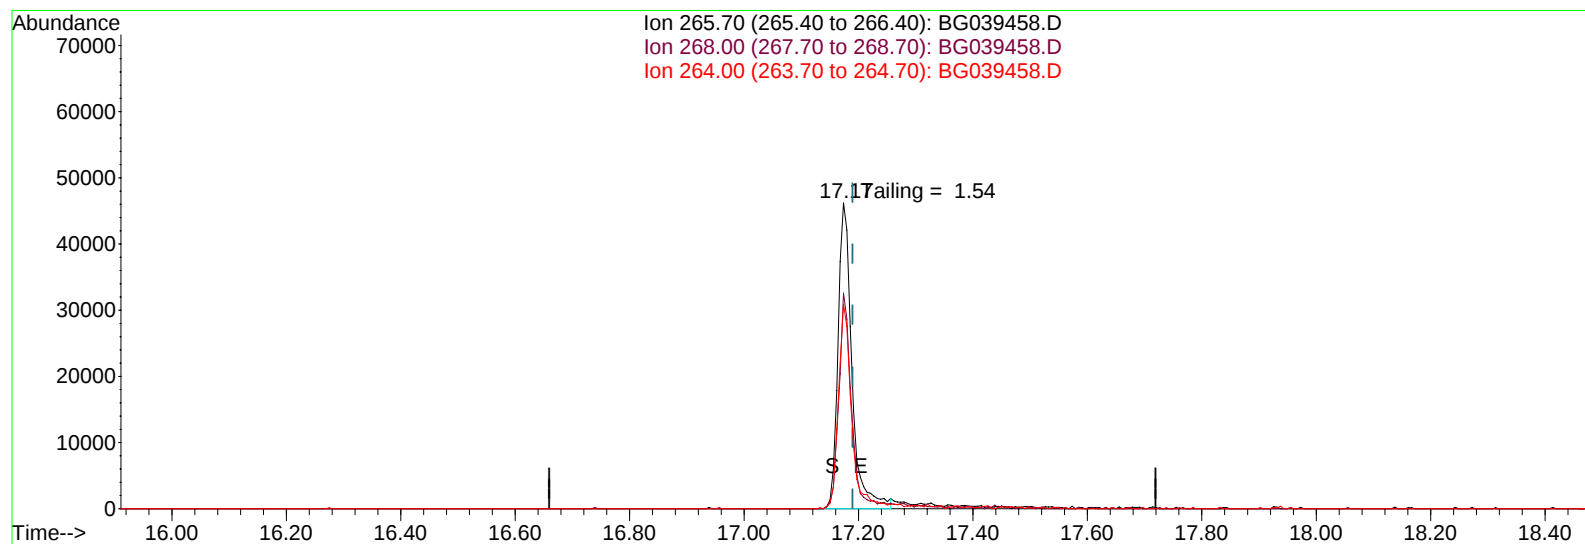

(70) Pentachlorophenol (C)




17.174min (-0.016) 158053.03ng

response 80697

Ion	Exp%	Act%
265.70	100	100
268.00	63.90	70.55
264.00	65.10	66.87
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA G\Data\BG021219\
 Data File : BG039458.D
 Acq On : 12 Feb 2019 11:14
 Operator : JU/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Feb 12 17:54:56 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG012919.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Jan 29 15:41:51 2019
 Response via : Initial Calibration

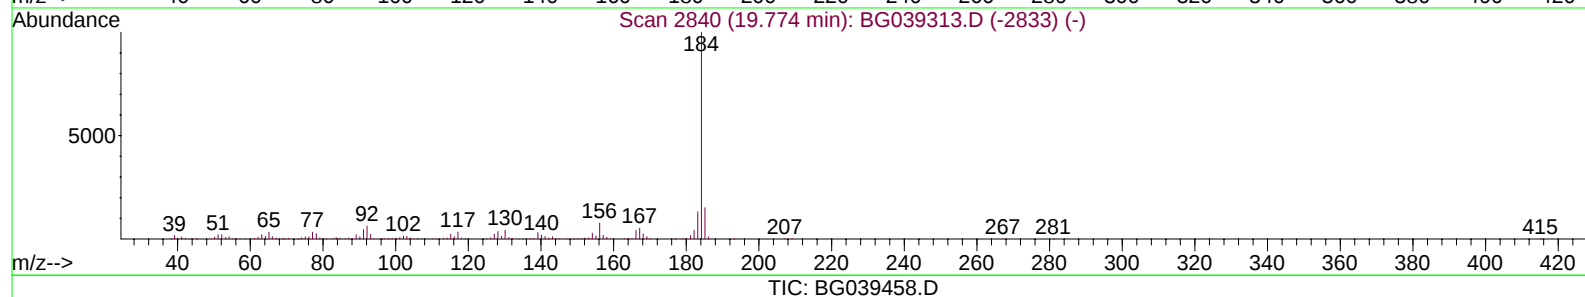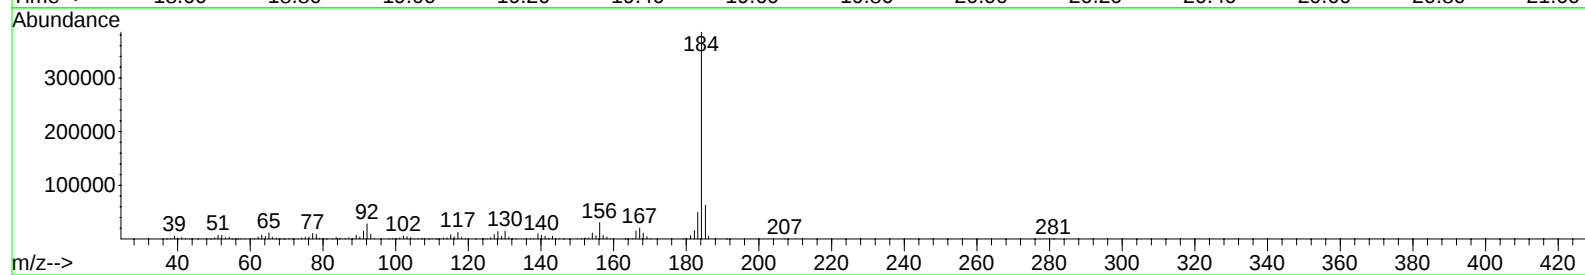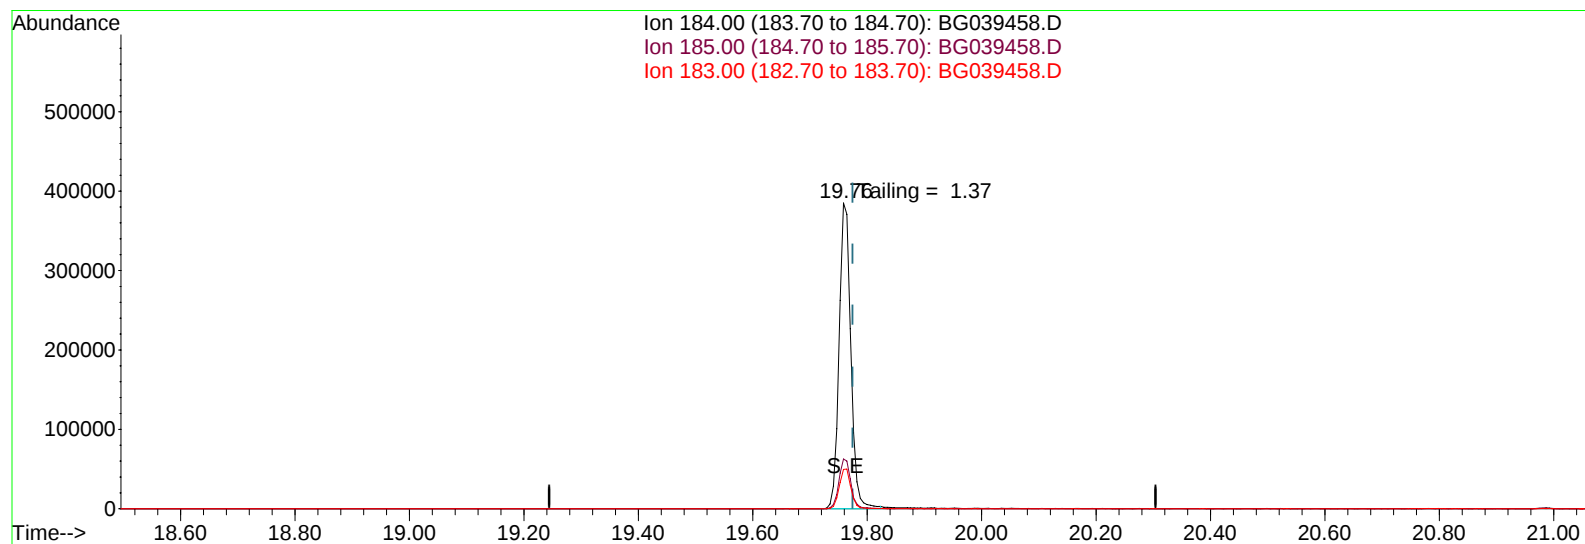

(77) Benzidine

19.759min (-0.016) 69336.14ng

response 552394

Ion	Exp%	Act%
184.00	100	100
185.00	15.20	16.26
183.00	13.20	12.88
0.00	0.00	0.00