
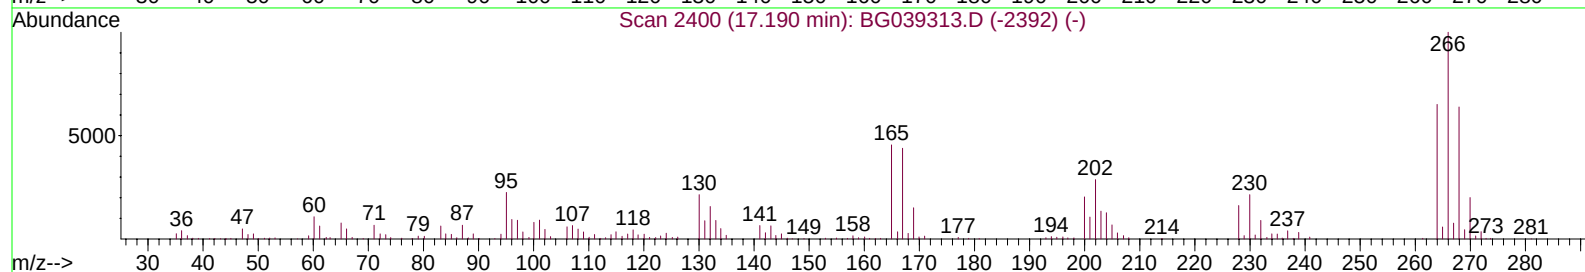
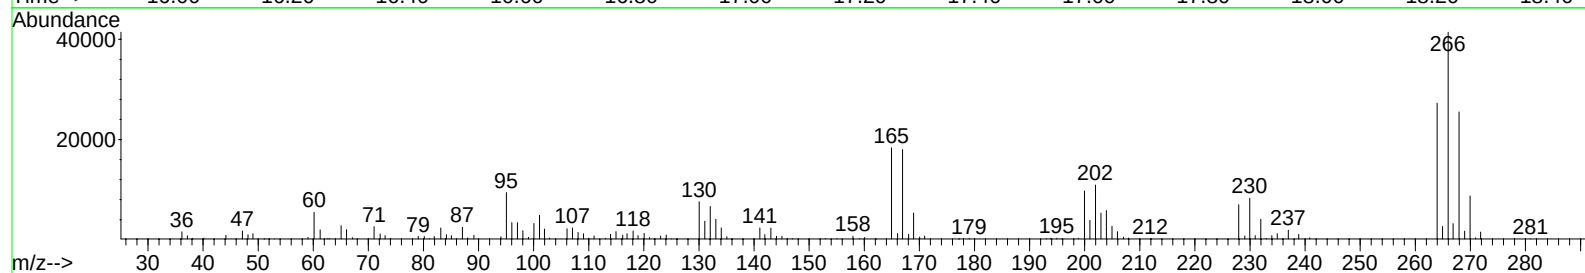


Data Path : Z:\svoasrv\HPCHEM1\BNA G\Data\BG021219\
Data File : BG039477.D
Acq On : 12 Feb 2019 23:52
Operator : JU/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Feb 13 00:28:02 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG012919.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jan 29 15:41:51 2019
Response via : Initial Calibration

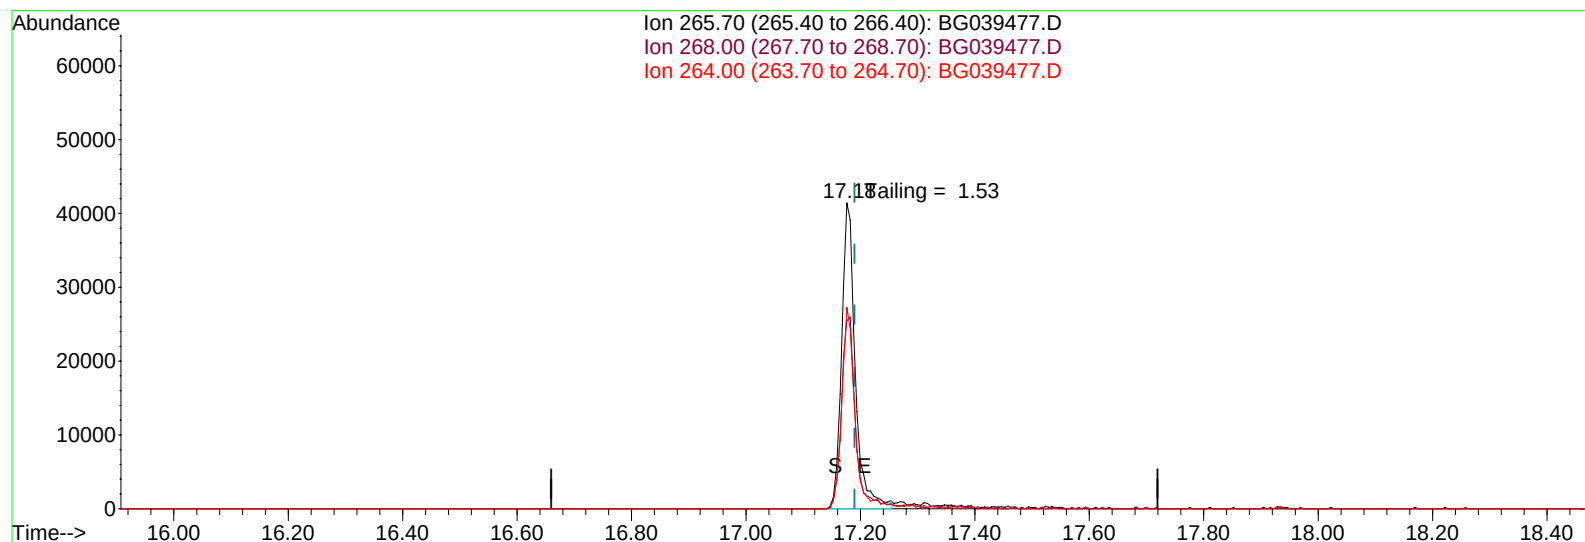

TIC: BG039477.D

(70) Pentachlorophenol (C)




17.176min (-0.013) 79380.64ng

response 68777

Ion	Exp%	Act%
265.70	100	100
268.00	63.90	61.60
264.00	65.10	65.85
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA G\Data\BG021219\
 Data File : BG039477.D
 Acq On : 12 Feb 2019 23:52
 Operator : JU/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Feb 13 00:28:02 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG012919.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Jan 29 15:41:51 2019
 Response via : Initial Calibration

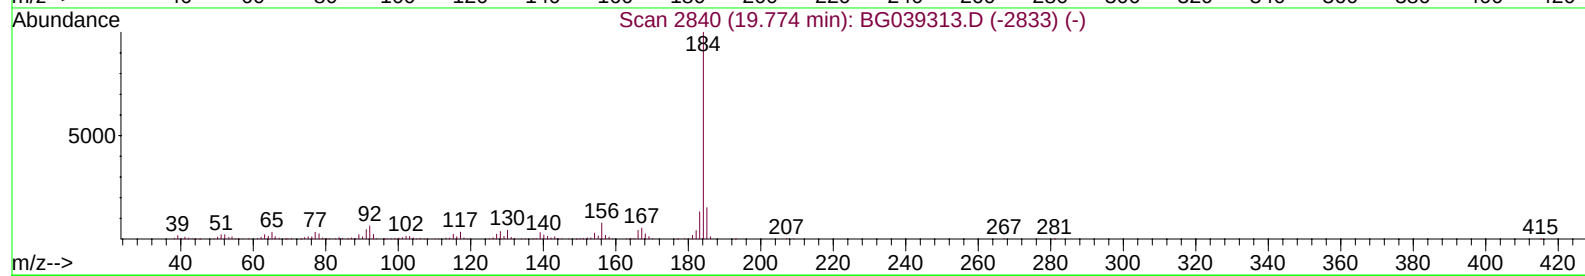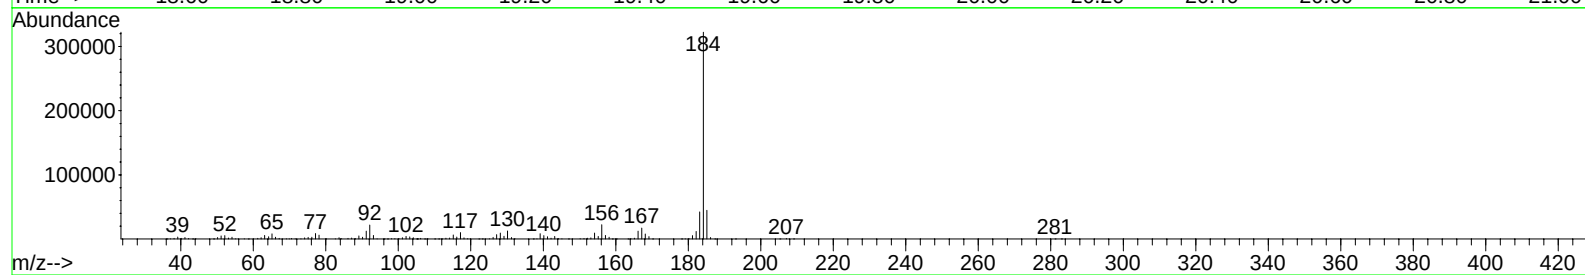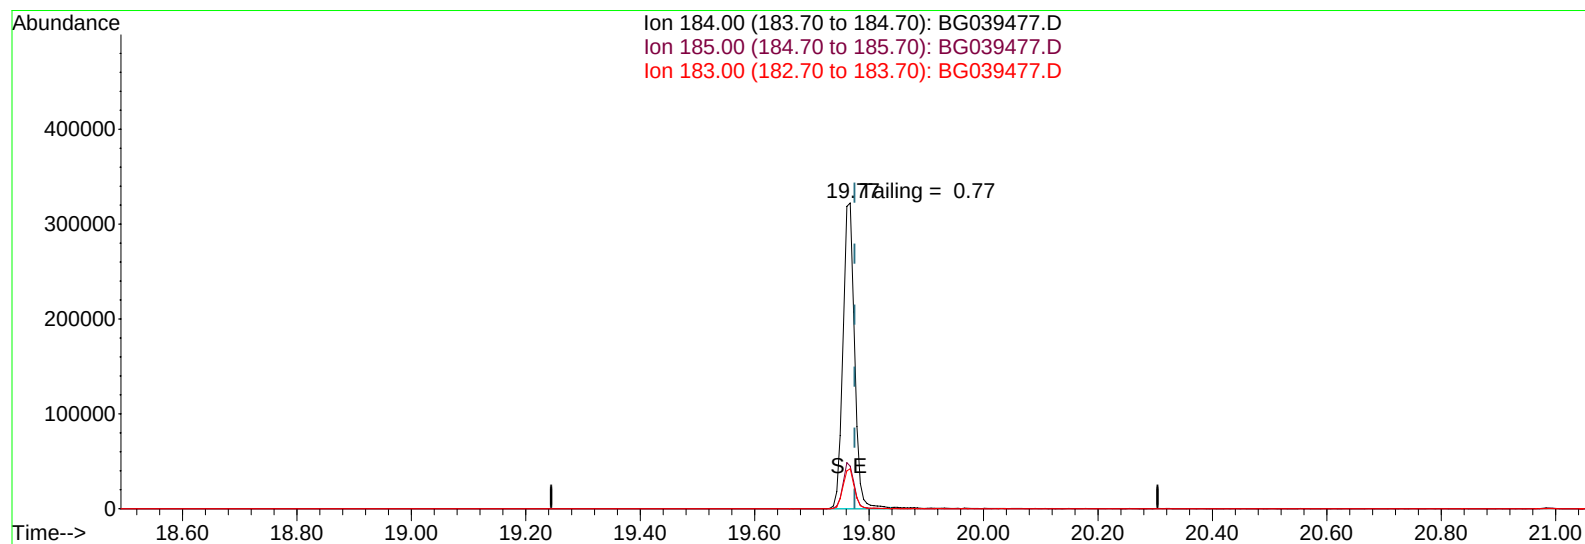

TIC: BG039477.D

(77) Benzidine

19.767min (-0.007) 0.00ng

response 455708

Ion	Exp%	Act%
184.00	100	100
185.00	15.20	13.92
183.00	13.20	13.10
0.00	0.00	0.00