

Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG021219\
 Data File : BG039471.D
 Acq On : 12 Feb 2019 19:53
 Operator : JU/SJ
 Sample : PB117058BL
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 PB117058BL

Quant Time: Feb 13 13:02:58 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG012919.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Jan 29 15:41:51 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.17	152	44544	20.00	ng	-0.01
21) Naphthalene-d8	10.99	136	195460	20.00	ng	-0.02
39) Acenaphthene-d10	14.79	164	142715	20.00	ng	-0.02
64) Phenanthrene-d10	17.54	188	361108	20.00	ng	-0.02
76) Chrysene-d12	21.83	240	360977	20.00	ng	-0.02
87) Perylene-d12	25.21	264	357973	20.00	ng	-0.03
System Monitoring Compounds						
5) 2-Fluorophenol	5.71	112	373570	143.54	ng	0.00
7) Phenol-d6	7.32	99	552401	144.19	ng	0.00
23) Nitrobenzene-d5	9.35	82	316510	101.16	ng	-0.02
42) 2,4,6-Tribromophenol	16.28	330	245149	159.52	ng	-0.01
45) 2-Fluorobiphenyl	13.42	172	833298	83.76	ng	-0.02
79) Terphenyl-d14	20.13	244	1366067	80.10	ng	-0.02


Target Compounds Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG021219\
Data File : BG039471.D
Acq On : 12 Feb 2019 19:53
Operator : JU/SJ
Sample : PB117058BL
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
PB117058BL

Quant Time: Feb 13 13:02:58 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG012919.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jan 29 15:41:51 2019
Response via : Initial Calibration

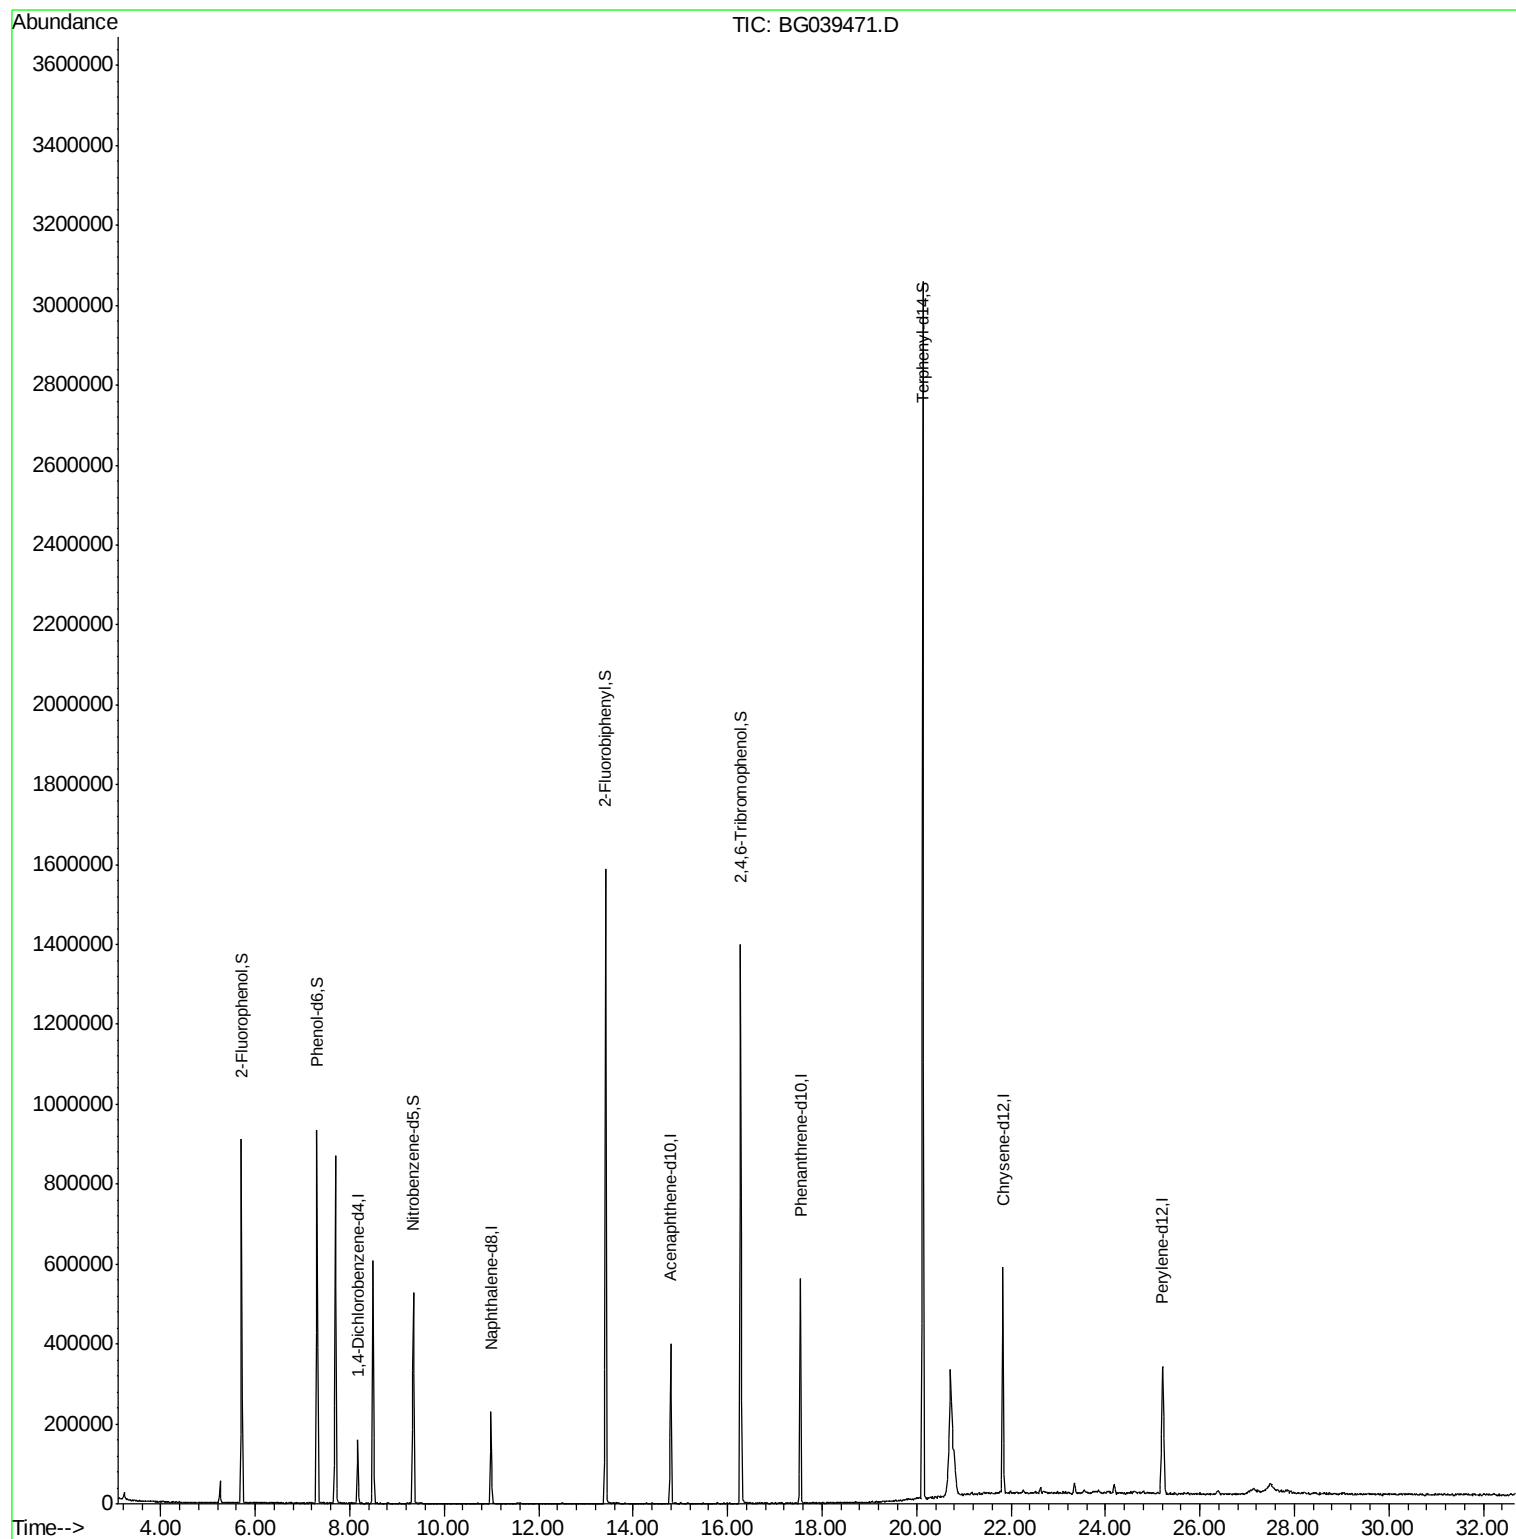

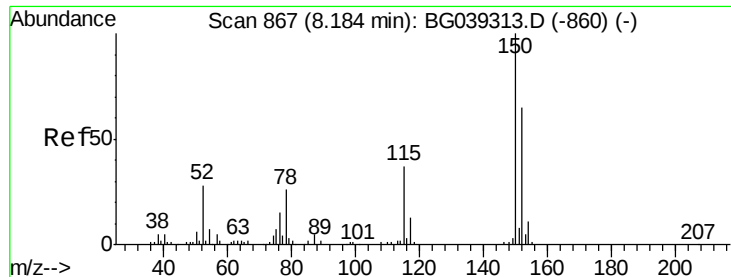


#1




1,4-Dichlorobenzene-d4
Concen: 20.000 ng
RT: 8.17 min Scan# 865
Delta R.T. -0.01 min
Lab File: BG039471.D
Acq: 12 Feb 2019 19:53

Instrument :
BNA_G
ClientSampleID :
PB117058BL

Tot Ion:152 Resp: 44544
Ion Ratio Lower Upper
152 100
150 155.6 123.7 185.5
115 59.0 45.9 68.9

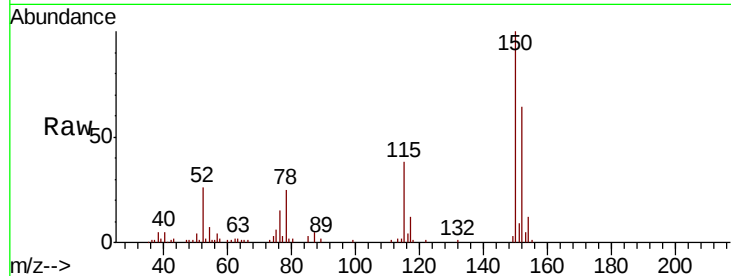


Abundance Ion 152.00 (151.70 to 152.70): E
Ion 150.00 (149.70 to 150.70): E
Ion 115.00 (114.70 to 115.70): E

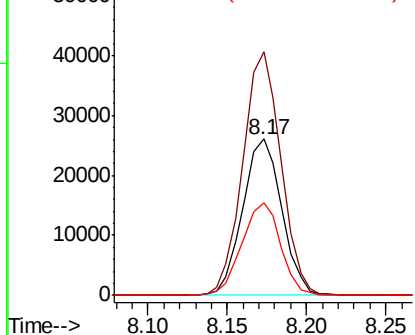



#5


2-Fluorophenol
Concen: 143.536 ng
RT: 5.71 min Scan# 446
Delta R.T. -0.01 min
Lab File: BG039471.D
Acq: 12 Feb 2019 19:53

Tgt Ion:112 Resp: 373570
Ion Ratio Lower Upper
112 100
64 70.2 57.8 86.8
63 36.5 29.8 44.6



Abundance Ion 112.00 (111.70 to 112.70): E
Ion 64.00 (63.70 to 64.70): BG
Ion 63.00 (62.70 to 63.70): BG

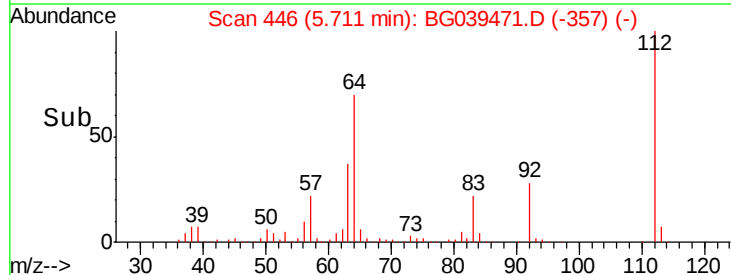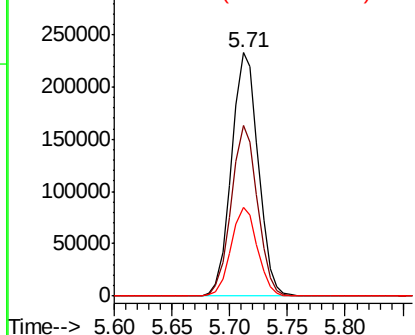

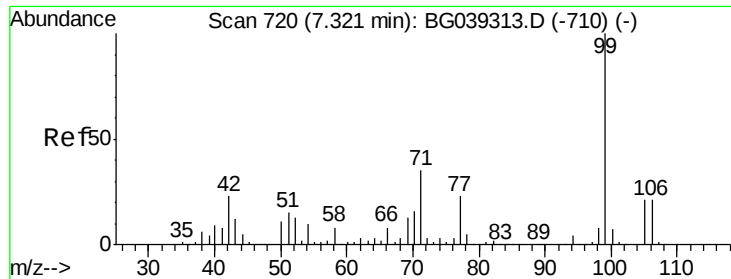

#7

Phenol-d6

Concen: 144.193 ng

RT: 7.32 min Scan# 719

Delta R.T. -0.01 min

Lab File: BG039471.D

Acq: 12 Feb 2019 19:53

Instrument :

BNA_G

ClientSampleId :

PB117058BL


Tot Ion: 99 Resp: 552401

Ion Ratio Lower Upper




99 100

42 19.7 18.2 27.2

71 34.5 28.0 42.0

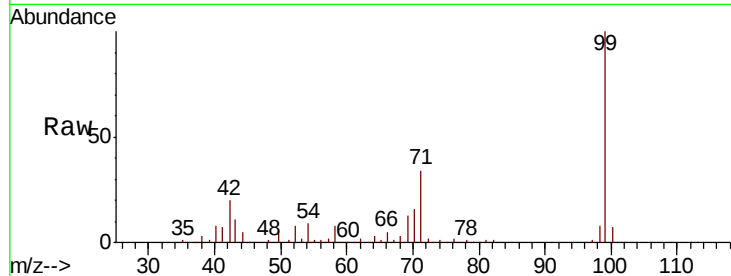

Abundance Ion 99.00 (98.70 to 99.70): BGC
Ion 42.00 (41.70 to 42.70): BGC
Ion 71.00 (70.70 to 71.70): BGC

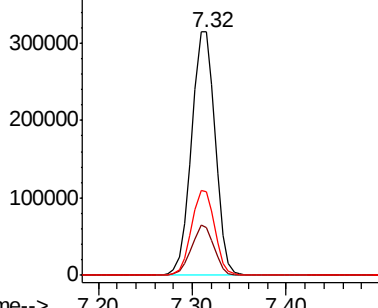

#21

Naphthalene-d8

Concen: 20.000 ng

RT: 10.99 min Scan# 1345

Delta R.T. -0.02 min

Lab File: BG039471.D

Acq: 12 Feb 2019 19:53

Tgt Ion: 136 Resp: 195460


Ion Ratio Lower Upper

136 100



137 10.6 9.1 13.7


54 10.7 9.4 14.2

68 6.1 4.2 6.4



Abundance Ion 136.00 (135.70 to 136.70): BGC
Ion 137.00 (136.70 to 137.70): BGC
Ion 54.00 (53.70 to 54.70): BGC
Ion 68.00 (67.70 to 68.70): BGC




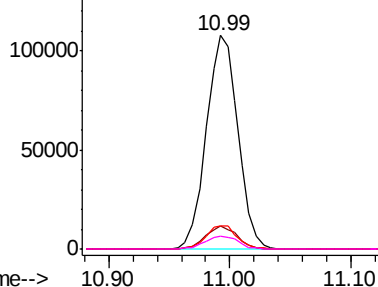




#23
Nitrobenzene-d5
Concen: 101.161 ng
RT: 9.35 min Scan# 1065
Delta R.T. -0.02 min
Lab File: BG039471.D
Acq: 12 Feb 2019 19:53




Instrument :
BNA_G
ClientSampleId :
PB117058BL


Tot Ion	Ratio	Lower	Upper
82	100		
128	43.1	31.3	46.9
54	57.8	50.9	76.3

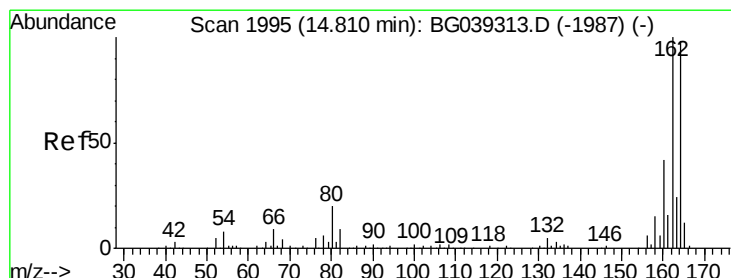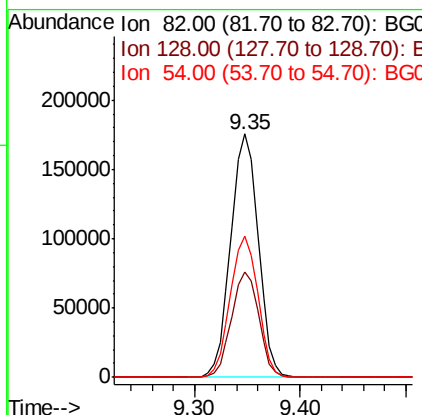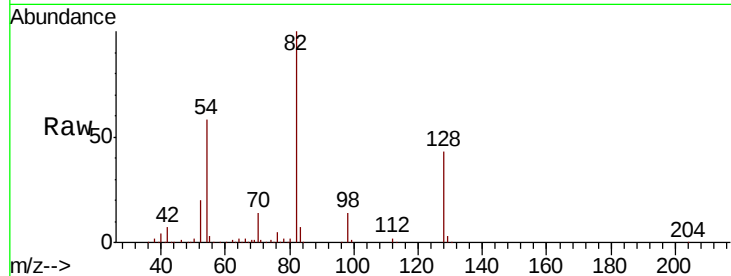

#39
Acenaphthene-d10
Concen: 20.000 ng
RT: 14.79 min Scan# 1992
Delta R.T. -0.02 min
Lab File: BG039471.D
Acq: 12 Feb 2019 19:53

Tgt Ion	Ratio	Lower	Upper
164	100		
162	99.8	81.6	122.4
160	42.3	34.2	51.2

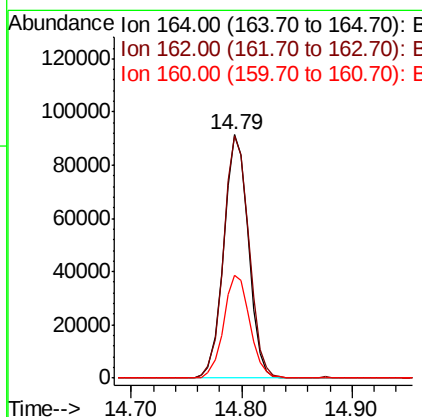


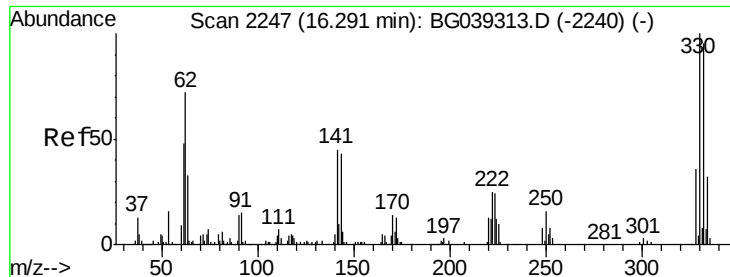




#42
 2,4,6-Tribromophenol
 Concen: 159.520 ng
 RT: 16.28 min Scan# 2245
 Delta R.T. -0.01 min
 Lab File: BG039471.D
 Acq: 12 Feb 2019 19:53

Instrument :
 BNA_G
 ClientSampleId :
 PB117058BL

Tot Ion:330 Resp: 245149
 Ion Ratio Lower Upper
 330 100
 332 96.9 75.7 113.5
 141 40.4 35.6 53.4

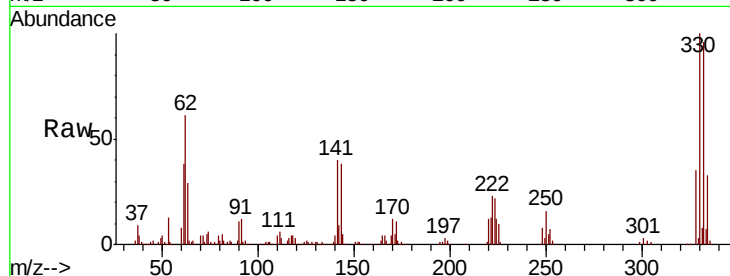


Abundance Ion 329.80 (329.50 to 330.50): E
 Ion 331.80 (331.50 to 332.50): E
 Ion 141.00 (140.70 to 141.70): E

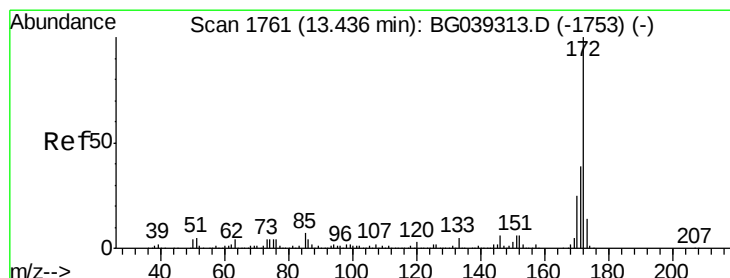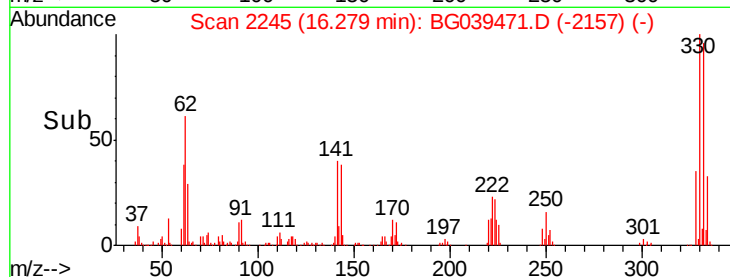
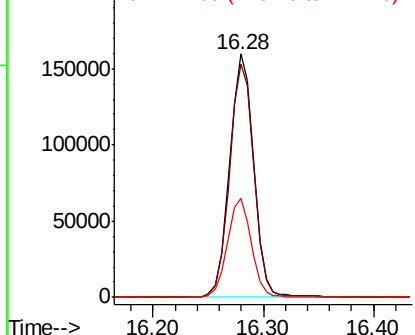



#45
 2-Fluorobiphenyl
 Concen: 83.762 ng
 RT: 13.42 min Scan# 1758
 Delta R.T. -0.02 min
 Lab File: BG039471.D
 Acq: 12 Feb 2019 19:53

Tgt Ion:172 Resp: 833298
 Ion Ratio Lower Upper
 172 100
 171 36.9 30.8 46.2
 170 24.1 20.2 30.4

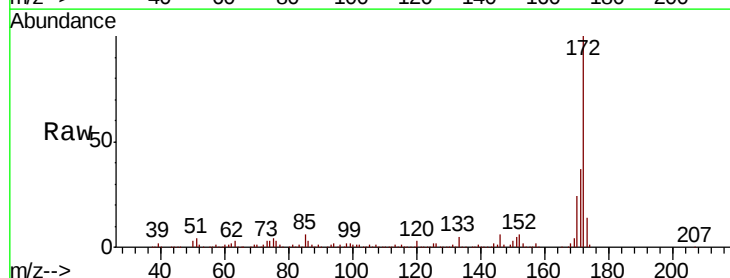

Abundance Ion 172.00 (171.70 to 172.70): E
 Ion 171.00 (170.70 to 171.70): E
 Ion 170.00 (169.70 to 170.70): E

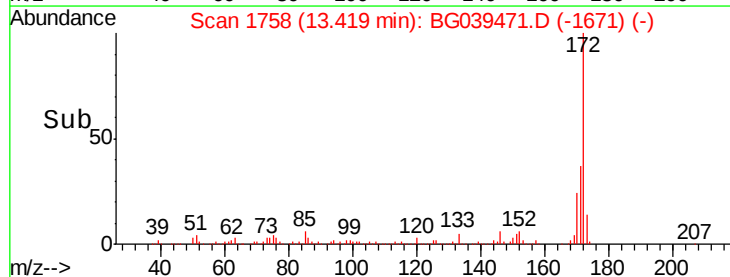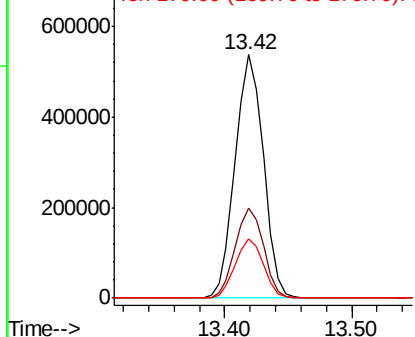



#64

Phenanthrene-d10

Concen: 20.000 ng

RT: 17.54 min Scan# 2459

Delta R.T. -0.02 min

Lab File: BG039471.D

Acq: 12 Feb 2019 19:53

Instrument :

BNA_G

ClientSampleId :

PB117058BL


Tot Ion:188 Resp: 361108

Ion Ratio Lower Upper

188 100

94 7.7 6.9 10.3




80 9.1 8.1 12.1

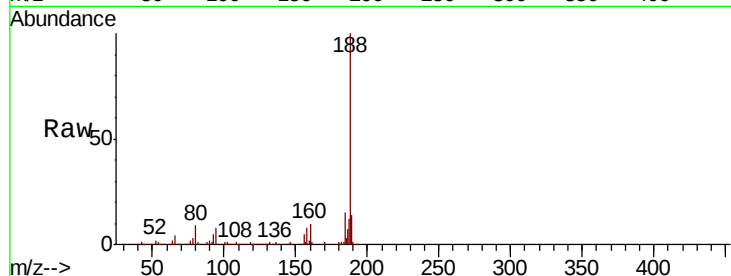

Abundance Ion 188.00 (187.70 to 188.70): E

Ion 94.00 (93.70 to 94.70): BG

Ion 80.00 (79.70 to 80.70): BG

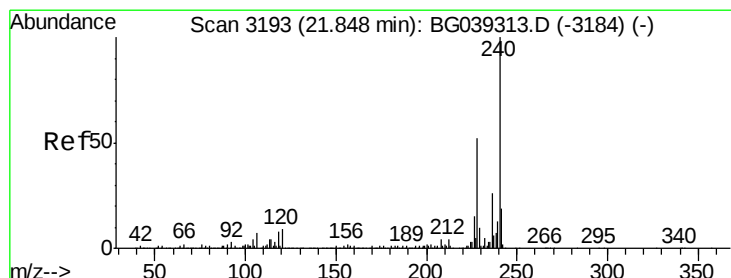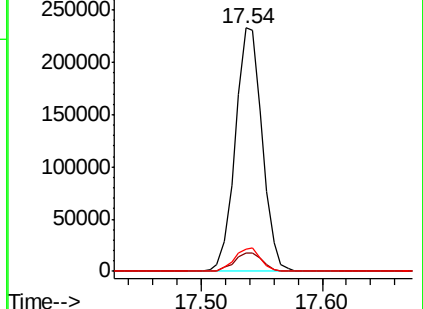

#76

Chrysene-d12

Concen: 20.000 ng

RT: 21.83 min Scan# 3190

Delta R.T. -0.02 min

Lab File: BG039471.D

Acq: 12 Feb 2019 19:53


Tgt Ion:240 Resp: 360977

Ion Ratio Lower Upper

240 100

120 7.9 7.0 10.6



236 26.1 21.0 31.4




Abundance Ion 240.00 (239.70 to 240.70): E

Ion 120.00 (119.70 to 120.70): E

Ion 236.00 (235.70 to 236.70): E

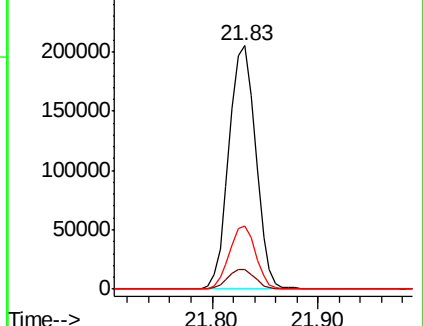



#79

Terphenyl-d14

Concen: 80.103 ng

RT: 20.13 min Scan# 2901

Delta R.T. -0.02 min

Lab File: BG039471.D

Acq: 12 Feb 2019 19:53

Instrument :


BNA_G

ClientSampleId :

PB117058BL

Tot Ion:244 Resp: 1366067




Ion	Ratio	Lower	Upper
244	100		
212	9.1	7.3	10.9
122	9.9	8.4	12.6

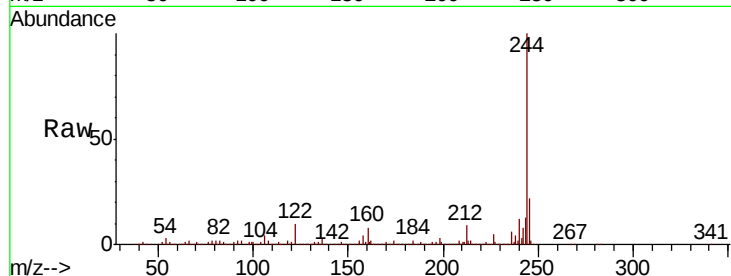

Abundance Ion 244.00 (243.70 to 244.70): E

Ion 212.00 (211.70 to 212.70): E

Ion 122.00 (121.70 to 122.70): E

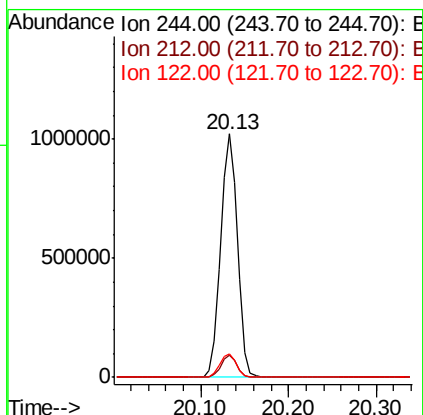

#87

Perylene-d12

Concen: 20.000 ng

RT: 25.21 min Scan# 3766


Delta R.T. -0.03 min

Lab File: BG039471.D

Acq: 12 Feb 2019 19:53

Tgt Ion:264 Resp: 357973

Ion	Ratio	Lower	Upper
264	100		
260	23.1	18.2	27.4
265	22.1	18.5	27.7



Abundance Ion 264.00 (263.70 to 264.70): E

Ion 260.00 (259.70 to 260.70): E

Ion 265.00 (264.70 to 265.70): E

