


Data Path : Z:\SVOASRV\HPCHEM1\BNA_G\DATA\BG021219\
 Data File : BG039458.D
 Acq On : 12 Feb 2019 11:14
 Operator : JU/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG012919.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Jan 29 15:41:51 2019

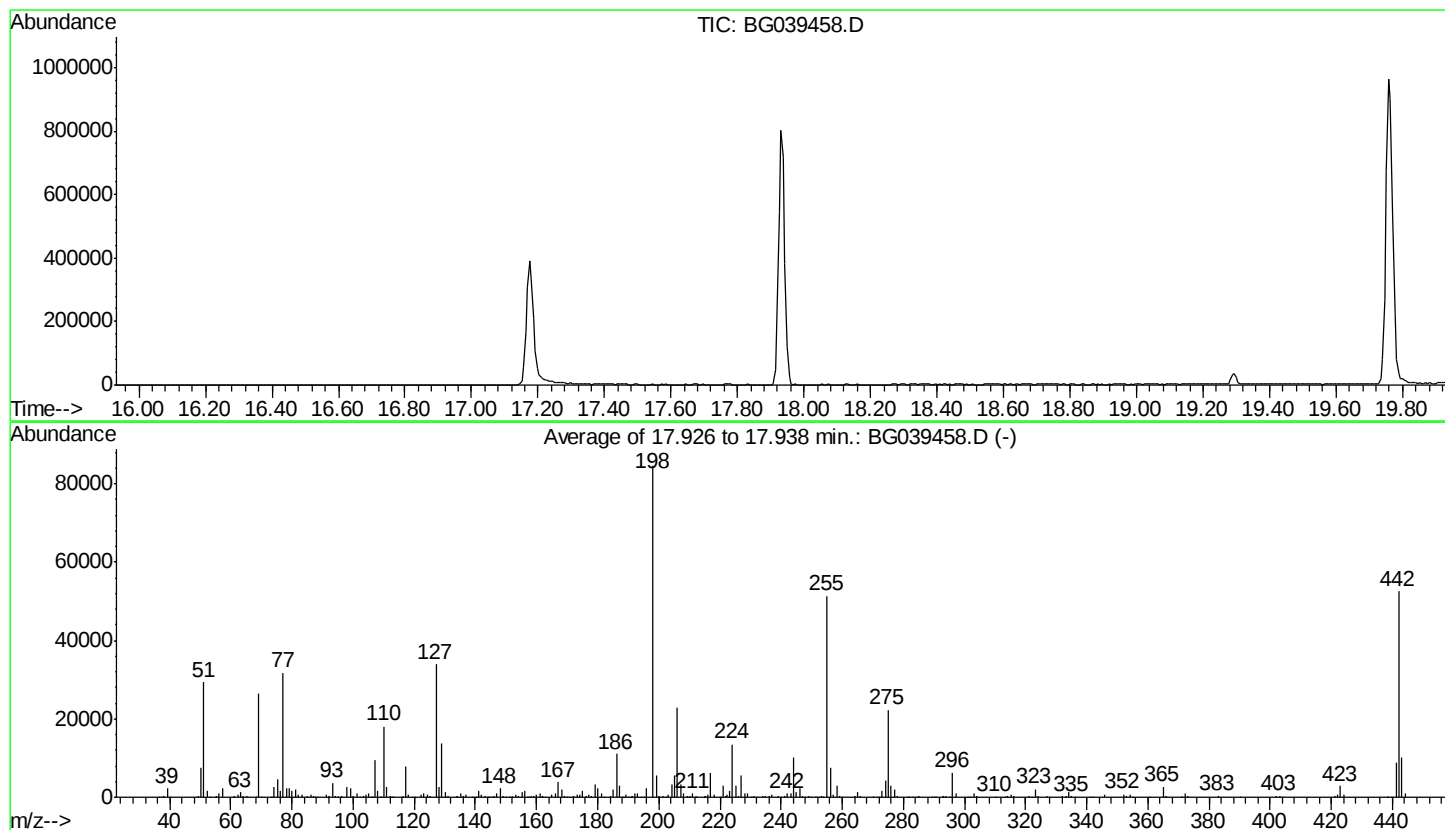

AutoFind: Scans 2526, 2527, 2528; Background Corrected with Scan 2520

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	34.7	29365	PASS
68	69	0.00	2	0.6	154	PASS
69	198	0.00	100	31.4	26576	PASS
70	69	0.00	2	0.2	50	PASS
127	198	10	80	40.0	33877	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	84642	PASS
199	198	5	9	6.6	5603	PASS
275	198	10	60	26.3	22296	PASS
365	198	1	100	3.2	2721	PASS
441	198	0.01	100	10.3	8757	PASS
442	198	50	100	62.1	52562	PASS
443	442	15	24	19.0	10013	PASS