


Data Path : Z:\SVOASRV\HPCHEM1\BNA_G\DATA\BG021219\
 Data File : BG039477.D
 Acq On : 12 Feb 2019 23:52
 Operator : JU/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG012919.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Jan 29 15:41:51 2019

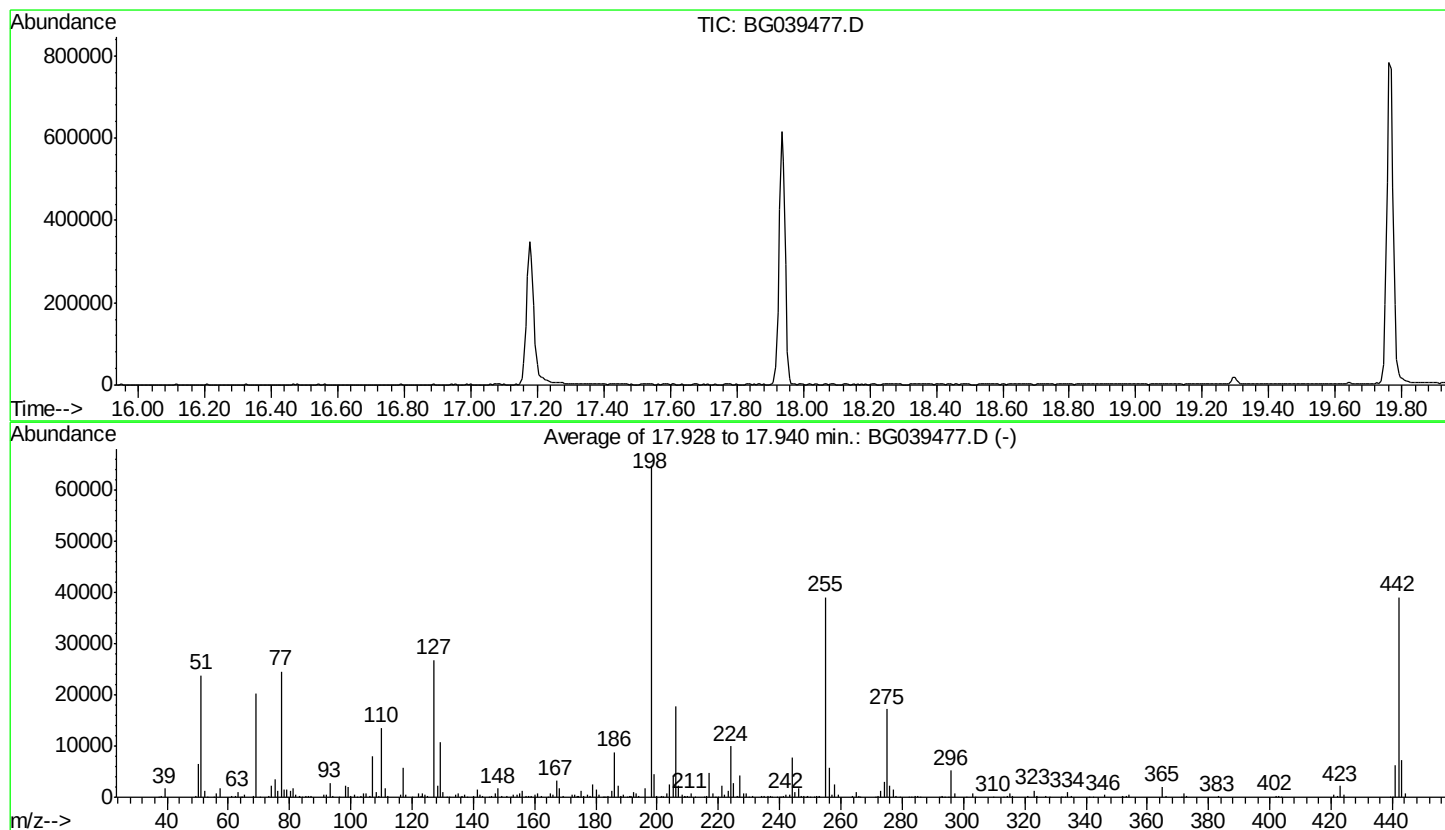

AutoFind: Scans 2526, 2527, 2528; Background Corrected with Scan 2519

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	36.9	23856	PASS
68	69	0.00	2	0.8	155	PASS
69	198	0.00	100	31.4	20301	PASS
70	69	0.00	2	0.3	63	PASS
127	198	10	80	41.5	26856	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	64701	PASS
199	198	5	9	6.9	4494	PASS
275	198	10	60	26.6	17219	PASS
365	198	1	100	3.2	2064	PASS
441	198	0.01	100	9.8	6310	PASS
442	198	50	100	60.3	39013	PASS
443	442	15	24	18.9	7354	PASS