
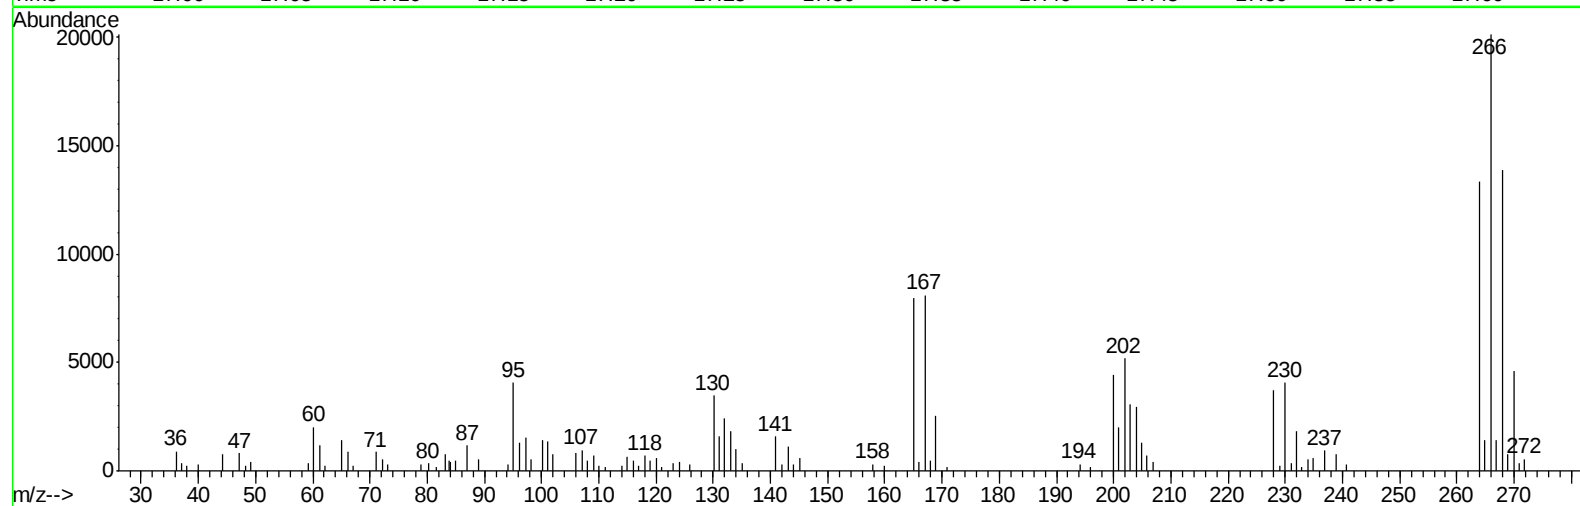


Data Path : Z:\svoasrv\HPCHEM1\BNA G\Data\BG021319\
Data File : BG039489.D
Acq On : 13 Feb 2019 15:16
Operator : JU/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Feb 14 07:24:23 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG012919.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jan 29 15:41:51 2019
Response via : Initial Calibration

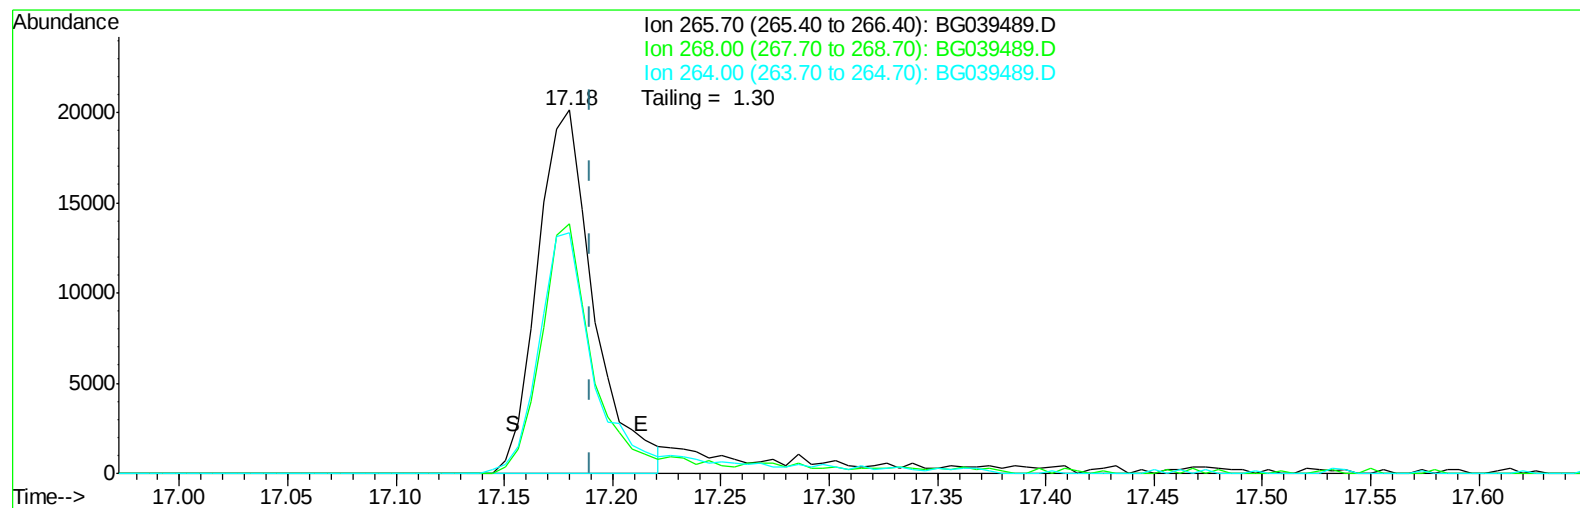

TIC: BG039489.D

(70) Pentachlorophenol (C)



17.180min (-0.010) 19517.89ng

response 38955

Ion	Exp%	Act%
265.70	100	100
268.00	63.90	68.79
264.00	65.10	66.26
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA G\Data\BG021319\
Data File : BG039489.D
Acq On : 13 Feb 2019 15:16
Operator : JU/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Feb 14 07:24:23 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG012919.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jan 29 15:41:51 2019
Response via : Initial Calibration

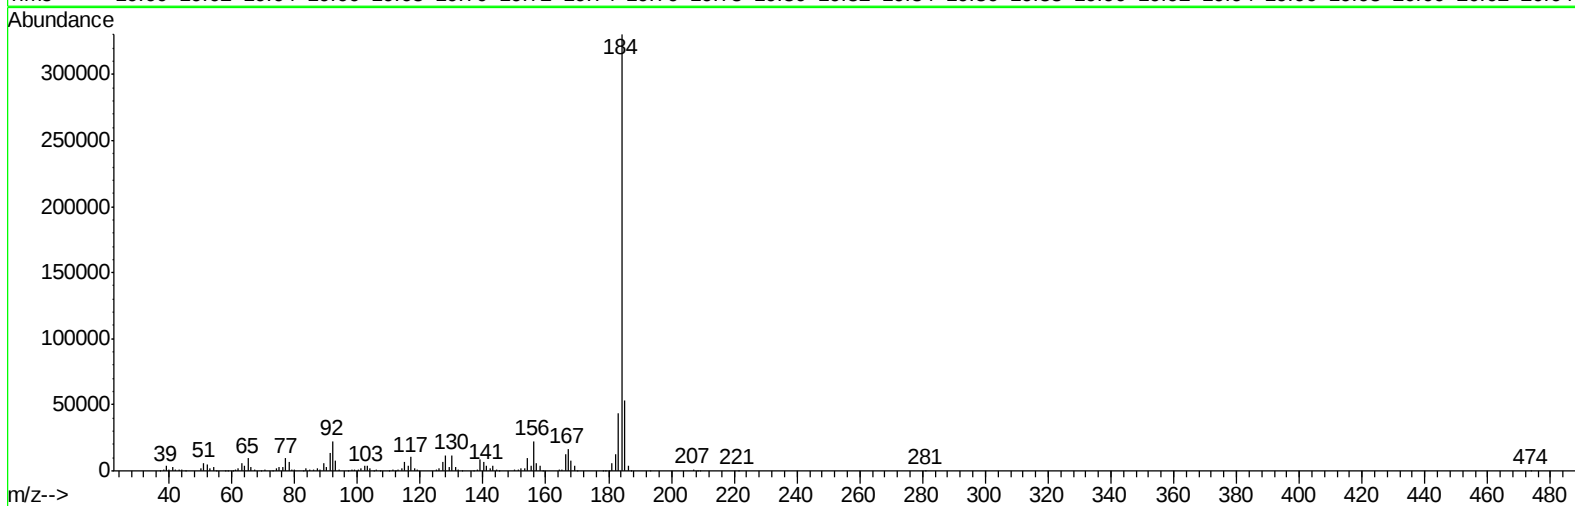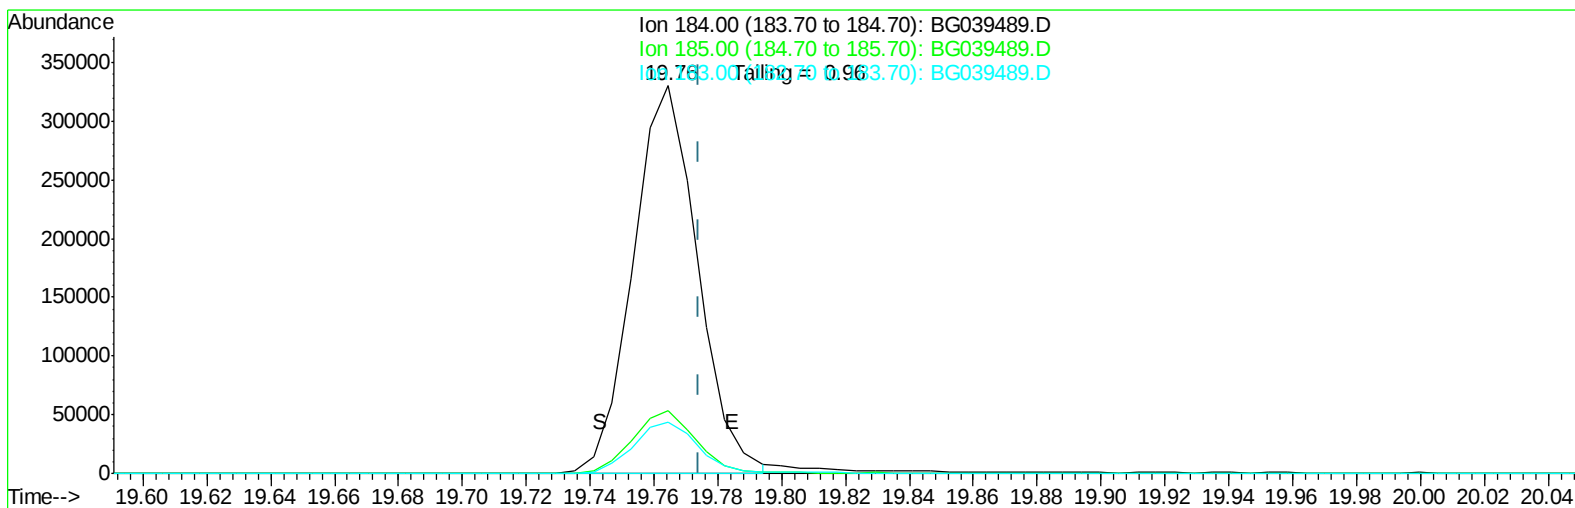

TIC: BG039489.D

(77) Benzidine

19.765min (-0.010) 115512.90ng

response 477182

Ion	Exp%	Act%
184.00	100	100
185.00	15.20	16.10
183.00	13.20	13.14
0.00	0.00	0.00