


Data Path : Z:\svoasrv\HPCHEM1\BNA G\Data\BG021319\
 Data File : BG039489.D
 Acq On : 13 Feb 2019 15:16
 Operator : JU/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG012919.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Jan 29 15:41:51 2019

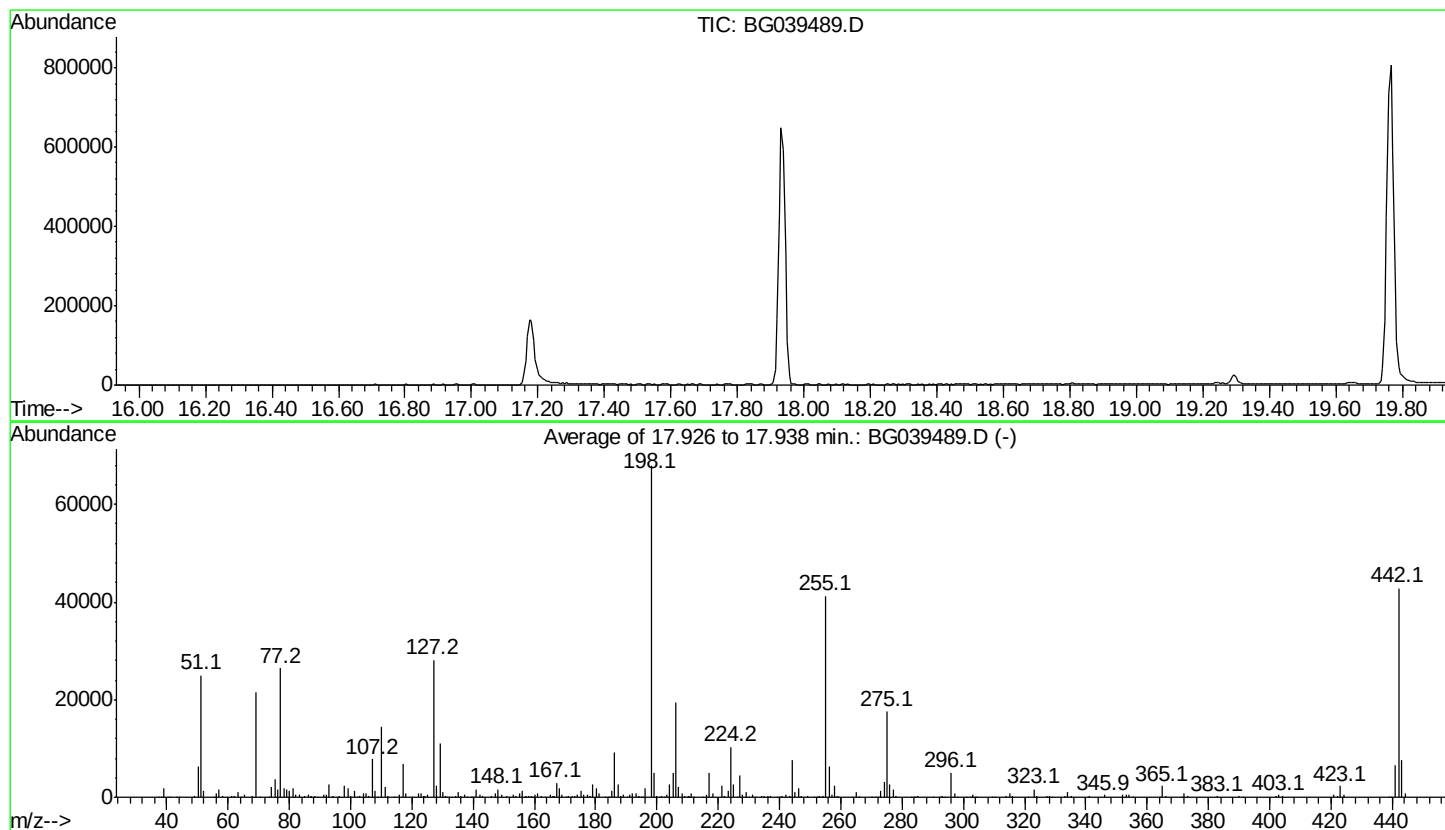

AutoFind: Scans 2526, 2527, 2528; Background Corrected with Scan 2520

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	36.7	24930	PASS
68	69	0.00	2	0.7	155	PASS
69	198	0.00	100	31.7	21525	PASS
70	69	0.00	2	0.3	67	PASS
127	198	10	80	41.5	28194	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	67938	PASS
199	198	5	9	7.2	4870	PASS
275	198	10	60	25.7	17450	PASS
365	198	1	100	3.5	2356	PASS
441	198	0.01	100	9.8	6656	PASS
442	198	50	100	62.9	42762	PASS
443	442	15	24	18.0	7708	PASS