
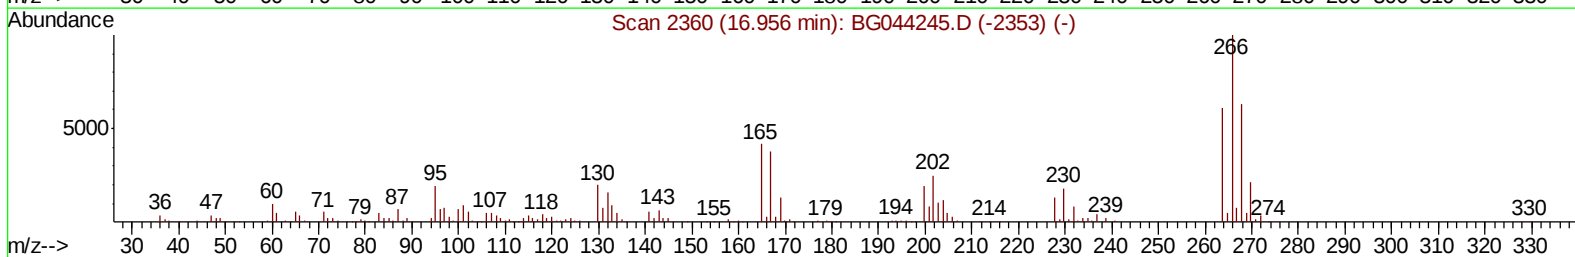
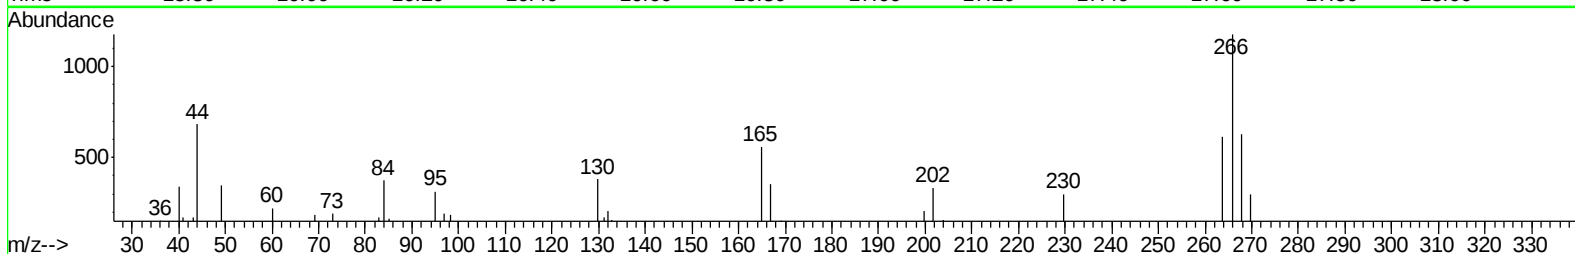


Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG021320\
Data File : BG044419.D
Acq On : 13 Feb 2020 15:23
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Feb 14 04:41:59 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG013020.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Feb 10 16:11:50 2020
Response via : Initial Calibration

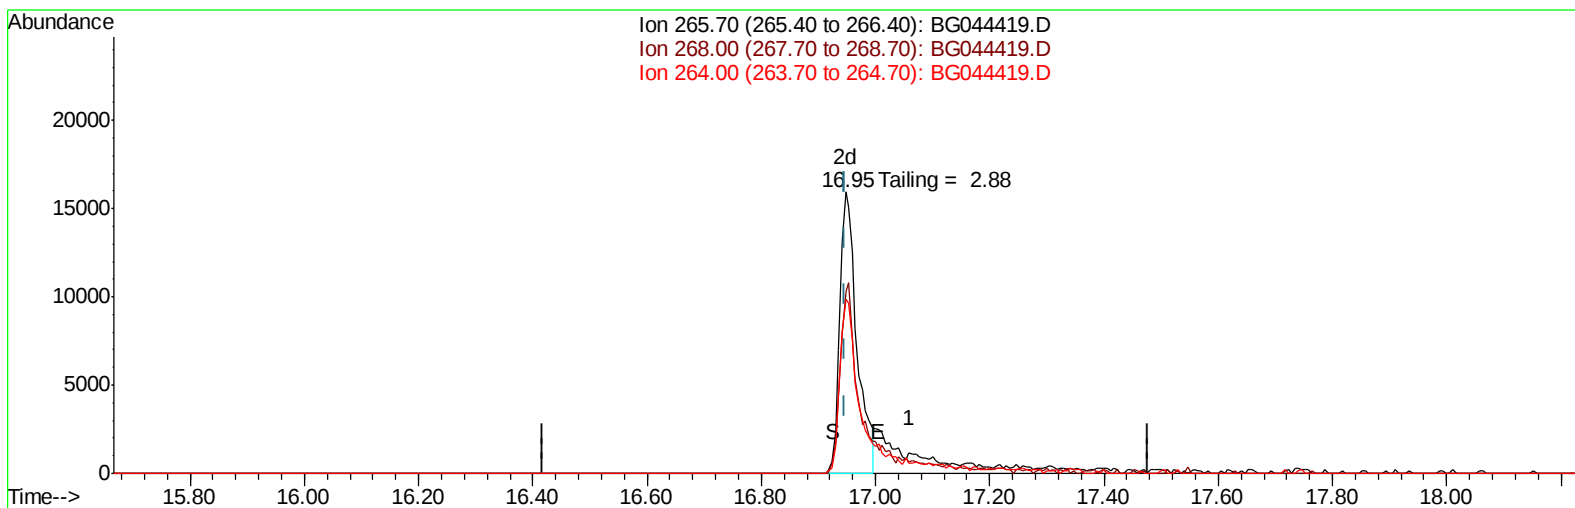

TIC: BG044419.D

(70) Pentachlorophenol (C)




17.059min (+0.111) 1178.99ng

response 2289

Ion	Exp%	Act%
265.70	100	100
268.00	63.20	53.61
264.00	60.90	52.17
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG021320\
Data File : BG044419.D
Acq On : 13 Feb 2020 15:23
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Feb 14 04:41:59 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG013020.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Feb 10 16:11:50 2020
Response via : Initial Calibration

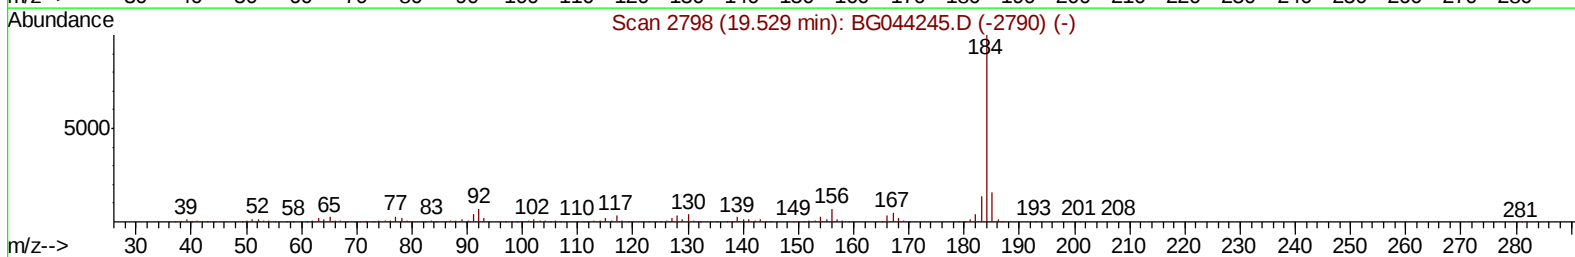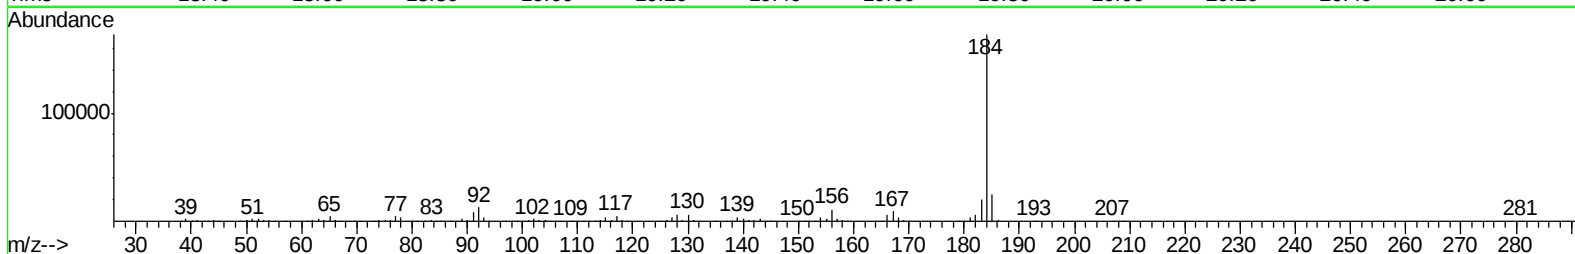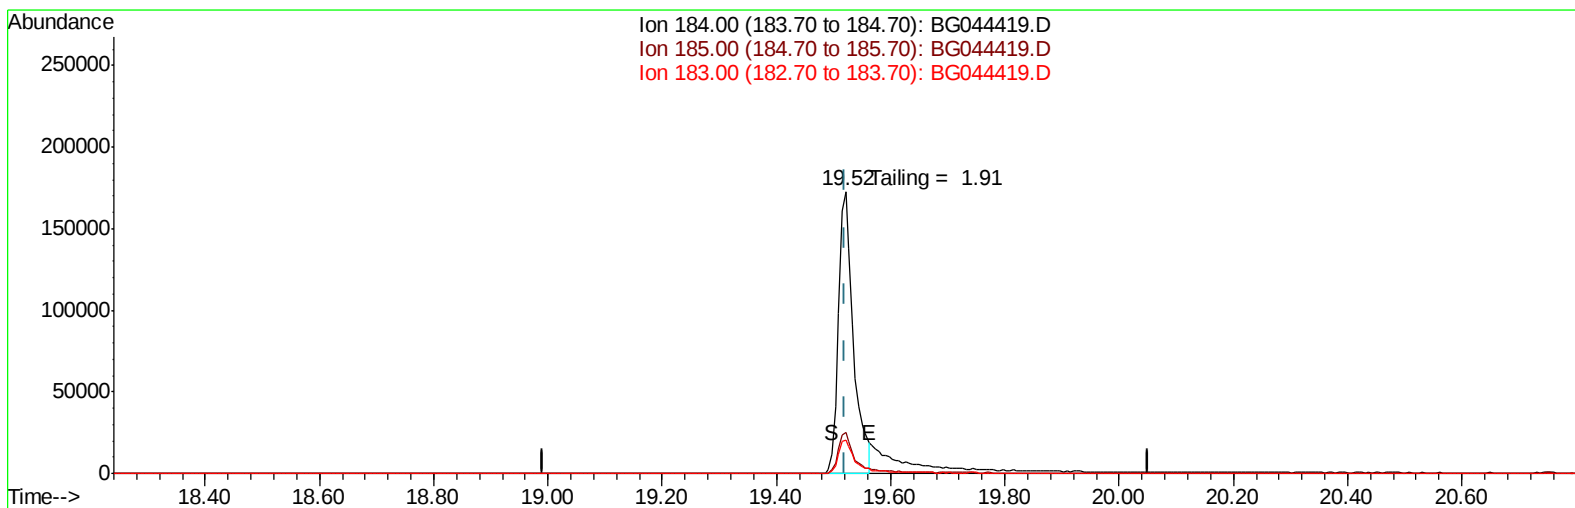

TIC: BG044419.D

(77) Benzidine

19.521min (-0.001) 0.00ng

response 386261

Ion	Exp%	Act%
184.00	100	100
185.00	16.10	14.62
183.00	13.50	11.92
0.00	0.00	0.00